
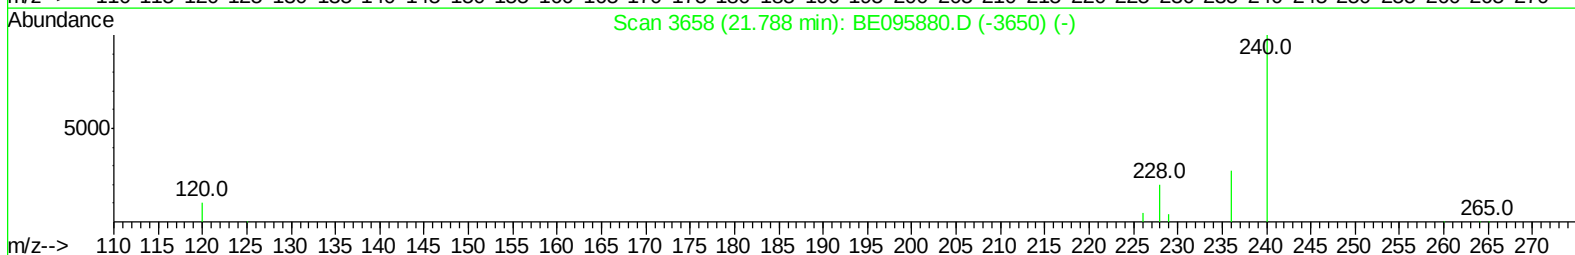
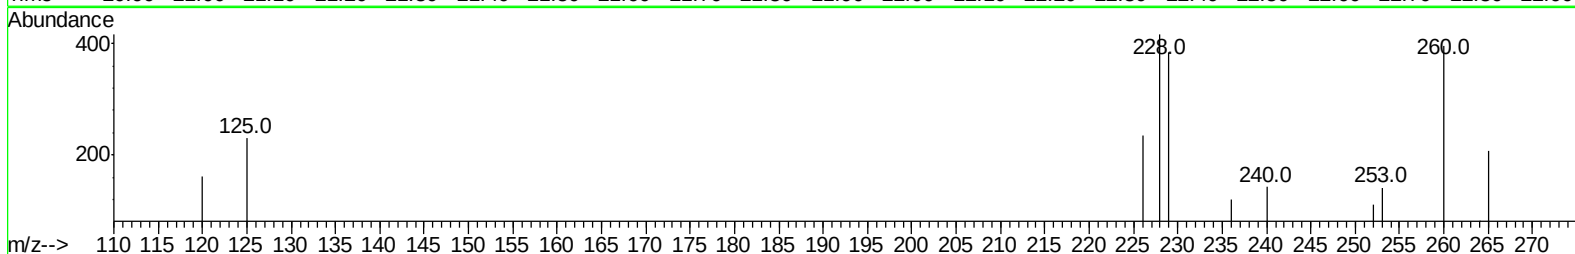


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\  
Data File : BE095892.D  
Acq On : 29 Mar 2018 00:17  
Operator : SJ/JU  
Sample : J2060-06  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 29 04:44:43 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 29 04:43:20 2018  
Response via : Initial Calibration

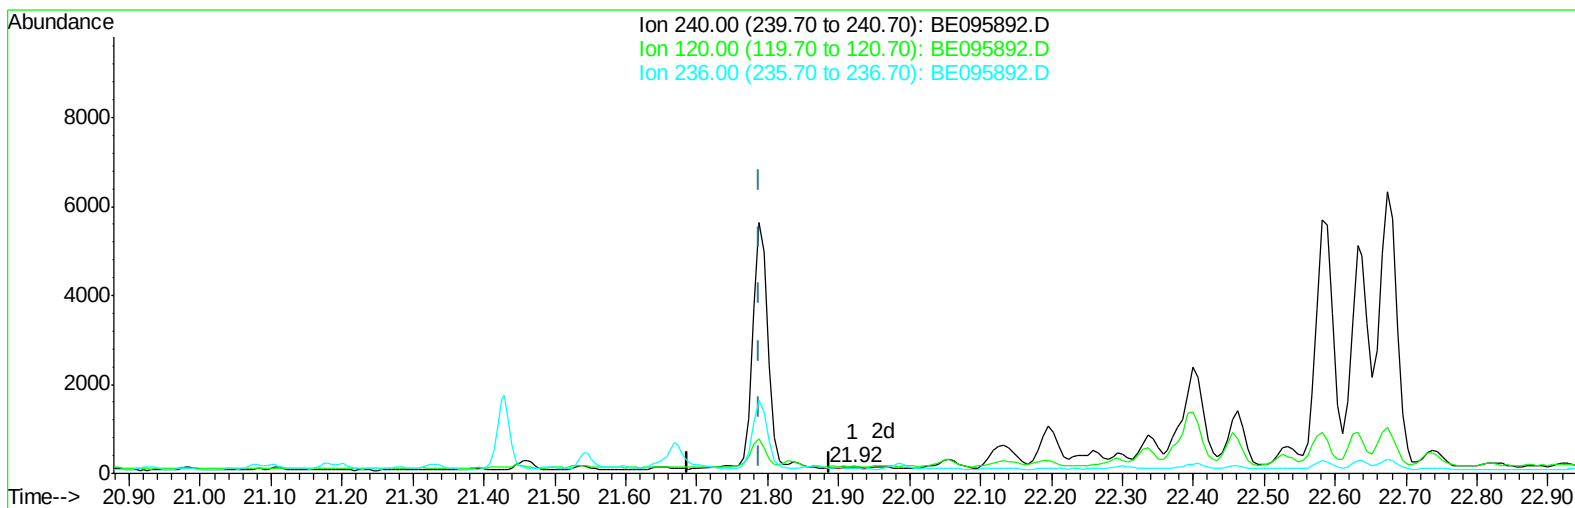

TIC: BE095892.D

(16) Chrysene-d12 (I)

21.921min (+0.133) 0.40ng/ul

response 75

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 240.00 | 100   | 100     |
| 120.00 | 20.60 | 113.99# |
| 236.00 | 34.90 | 84.62#  |
| 0.00   | 0.00  | 0.00    |