
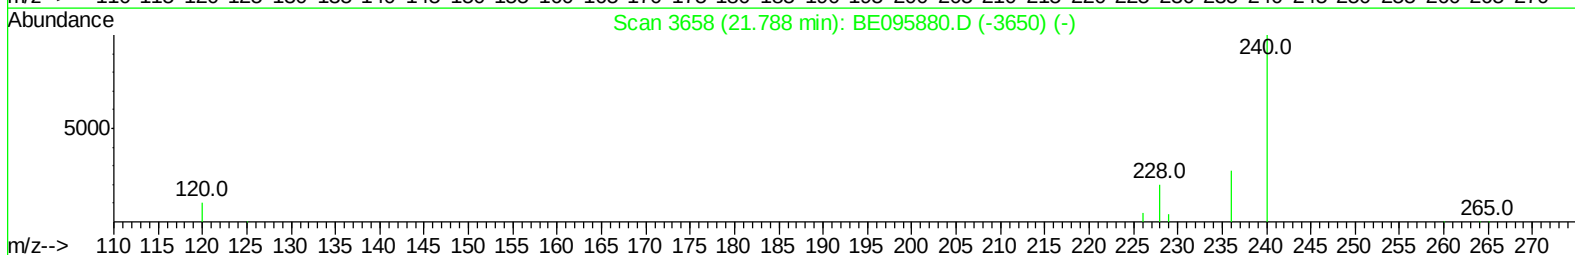
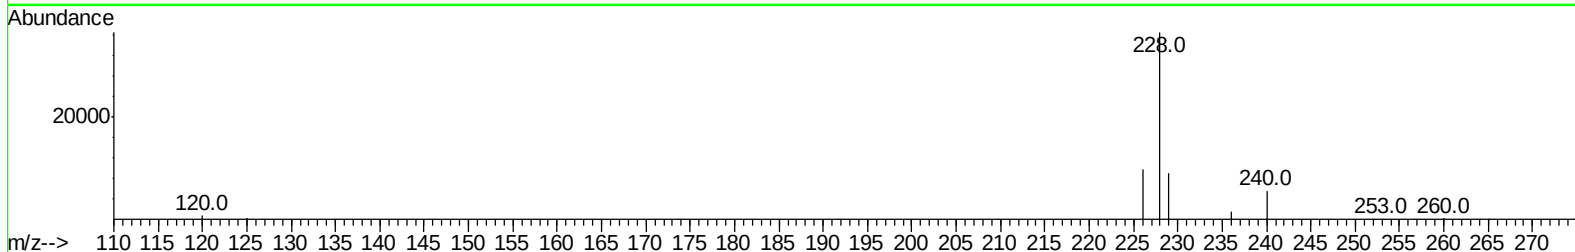


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095892.D
Acq On : 29 Mar 2018 00:17
Operator : SJ/JU
Sample : J2060-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 29 04:44:43 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 04:43:20 2018
Response via : Initial Calibration

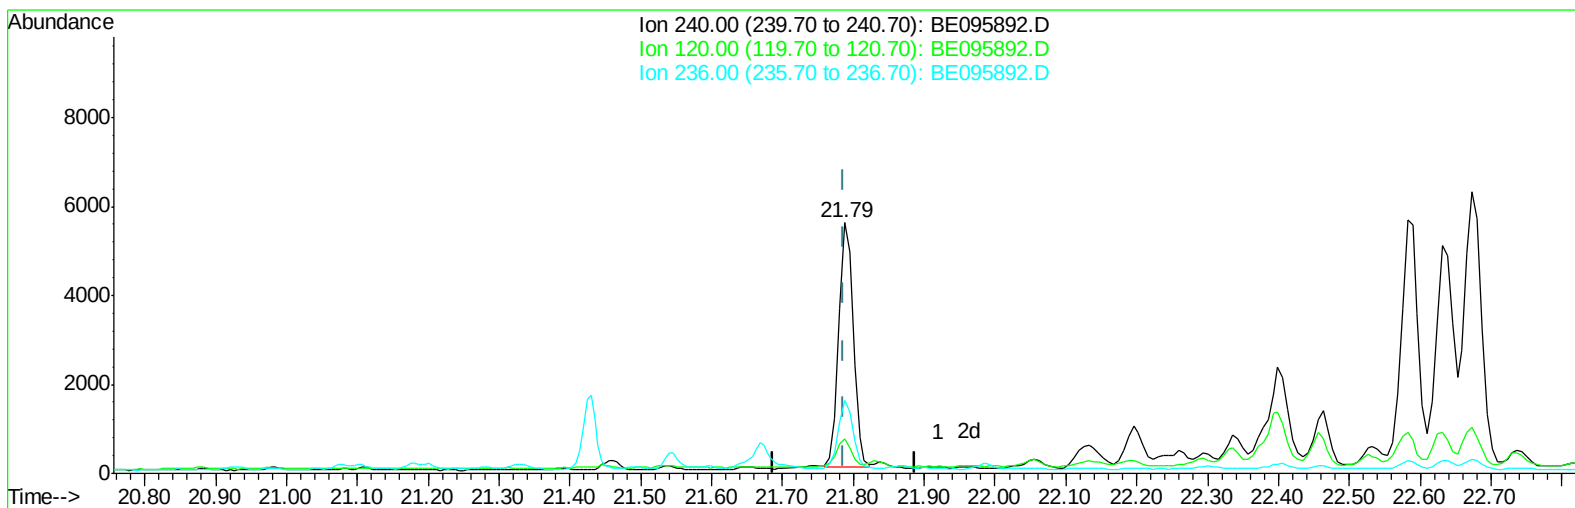

TIC: BE095892.D

(16) Chrysene-d12 (I)

21.788min (-0.000) 0.40ng/ul m

response 7707

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	13.72#
236.00	34.90	29.12
0.00	0.00	0.00