
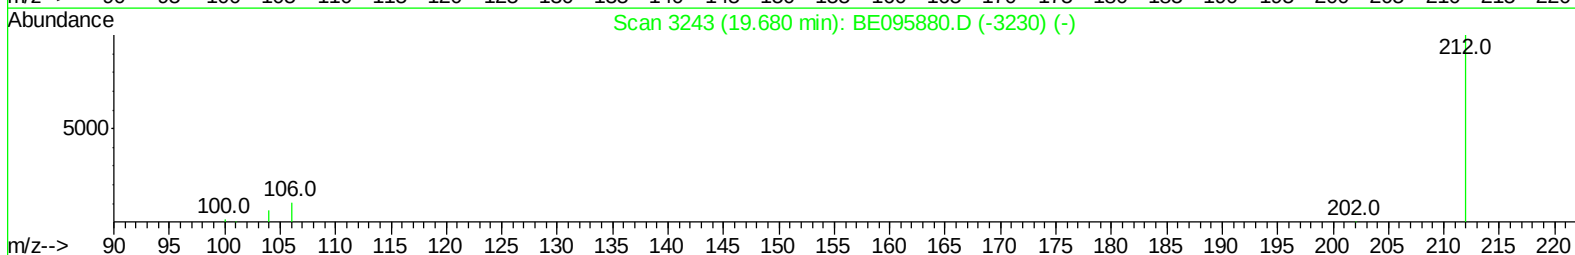
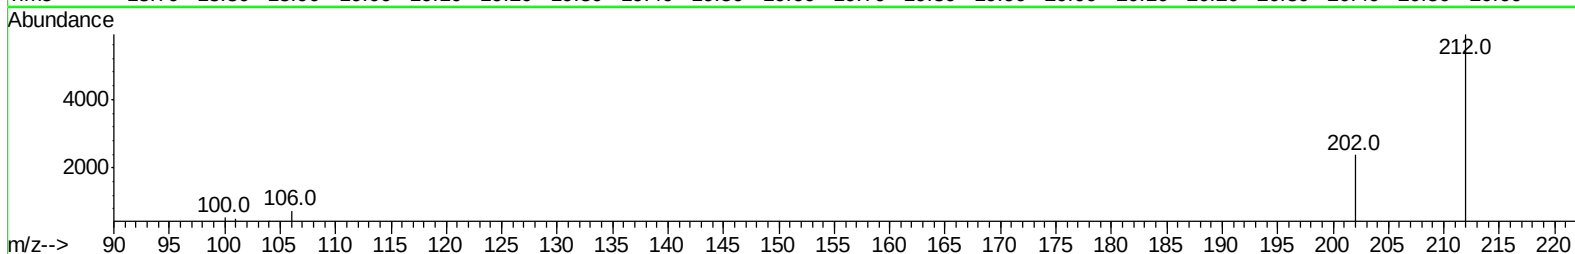


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095892.D
Acq On : 29 Mar 2018 00:17
Operator : SJ/JU
Sample : J2060-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 29 06:10:19 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 04:43:20 2018
Response via : Initial Calibration

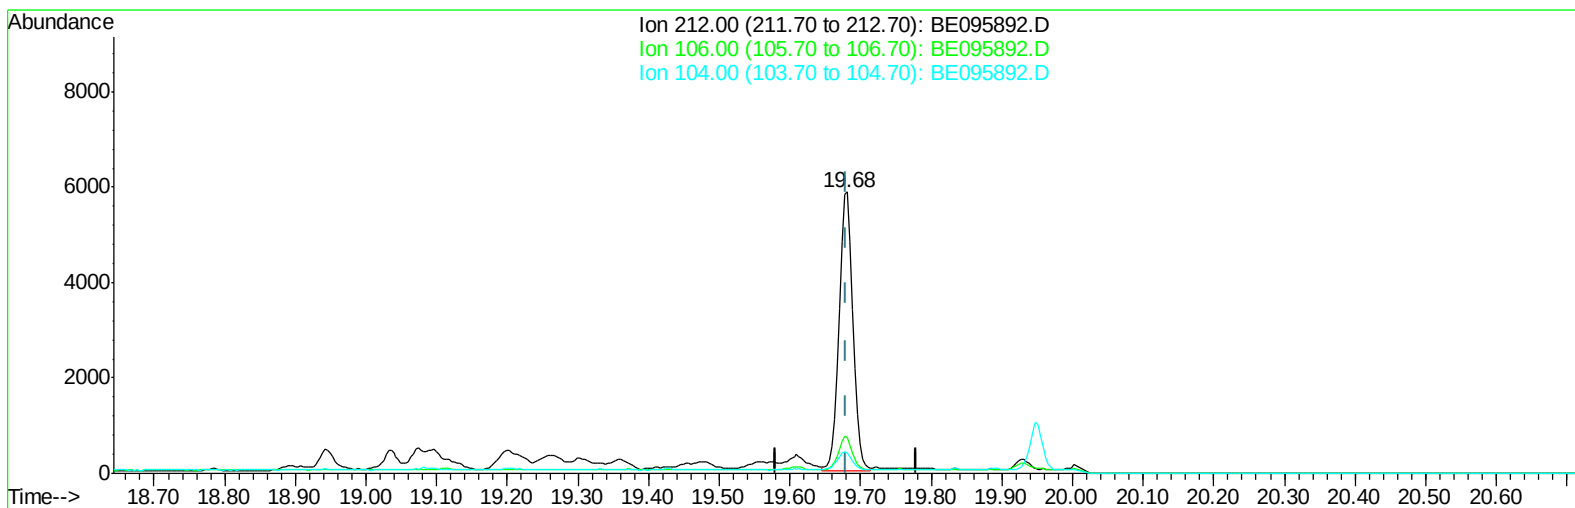

TIC: BE095892.D

(14) Fluoranthene-d10 (SURRE)

19.681min (+0.001) 0.32ng/ul m

response 7762

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00