
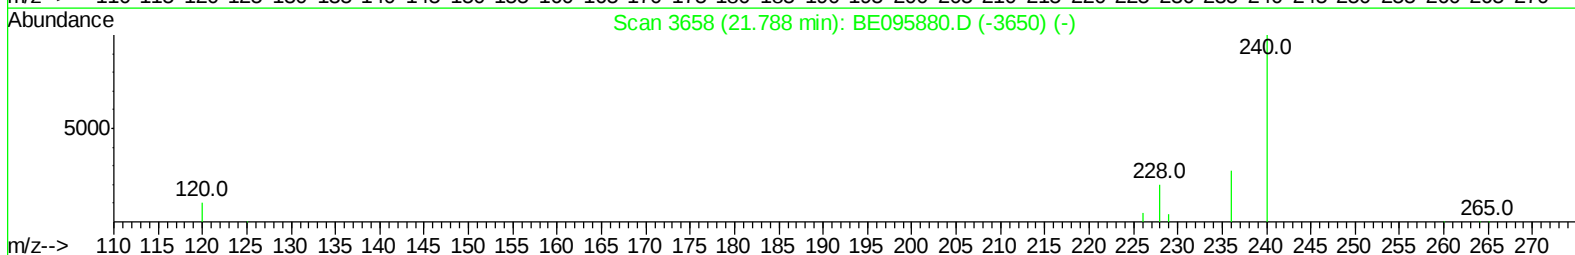
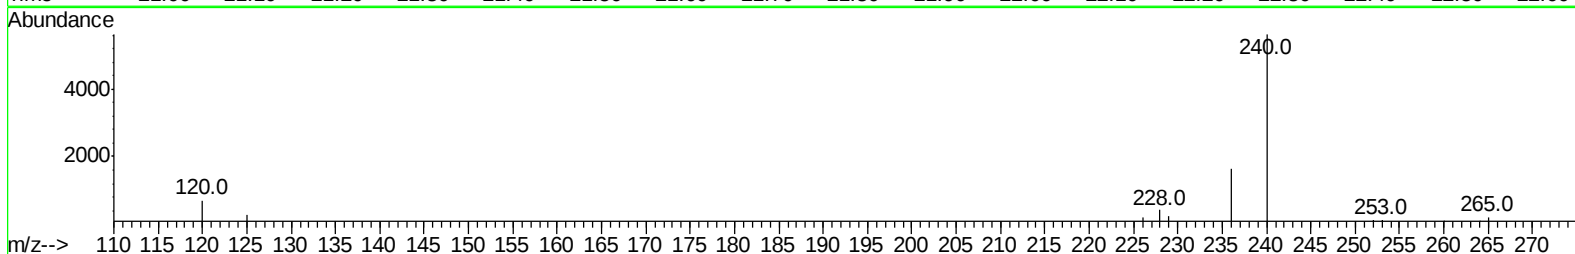


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\  
Data File : BE095893.D  
Acq On : 29 Mar 2018 00:53  
Operator : SJ/JU  
Sample : J2060-04  
Misc :  
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Mar 29 04:44:58 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 29 04:43:20 2018  
Response via : Initial Calibration

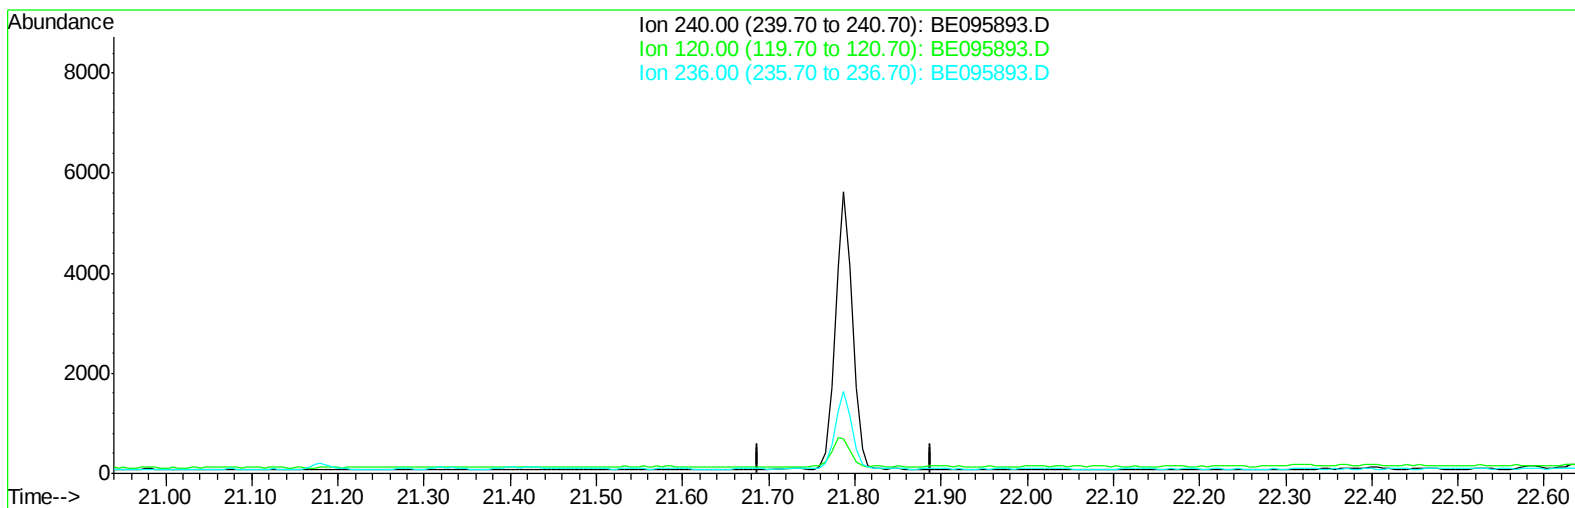

TIC: BE095893.D

(16) Chrysene-d12 (I)

21.788min (-21.788) 0.00ng/ul

response 0

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 240.00 | 100   | 0.00  |
| 120.00 | 20.60 | 0.00# |
| 236.00 | 34.90 | 0.00# |
| 0.00   | 0.00  | 0.00  |