
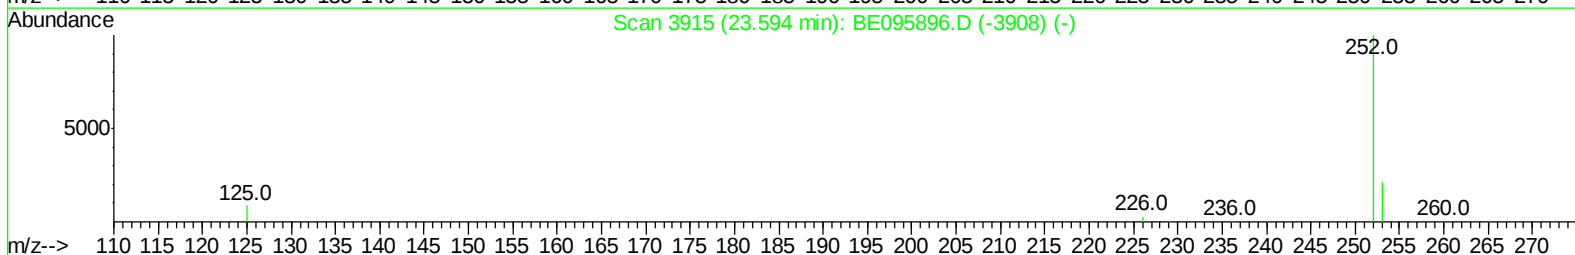
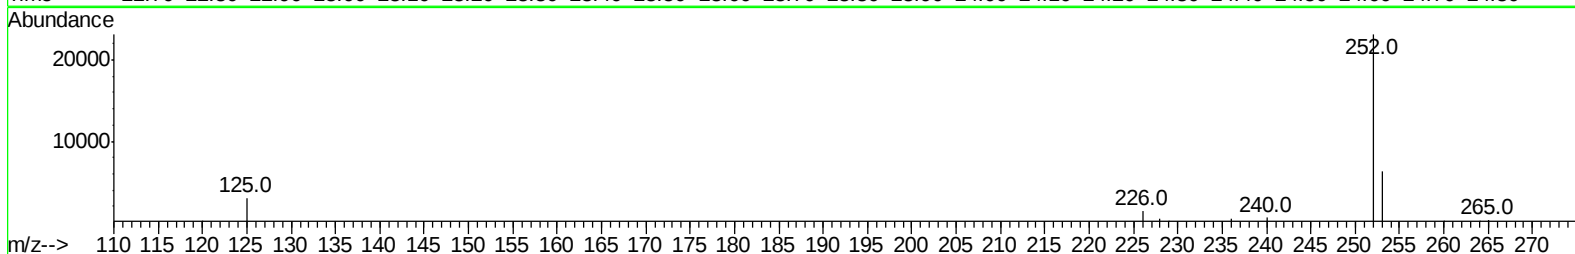


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\  
Data File : BE095897.D  
Acq On : 29 Mar 2018 3:16  
Operator : SJ/JU  
Sample : J2060-10  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Mar 29 07:12:11 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 29 07:00:08 2018  
Response via : Initial Calibration

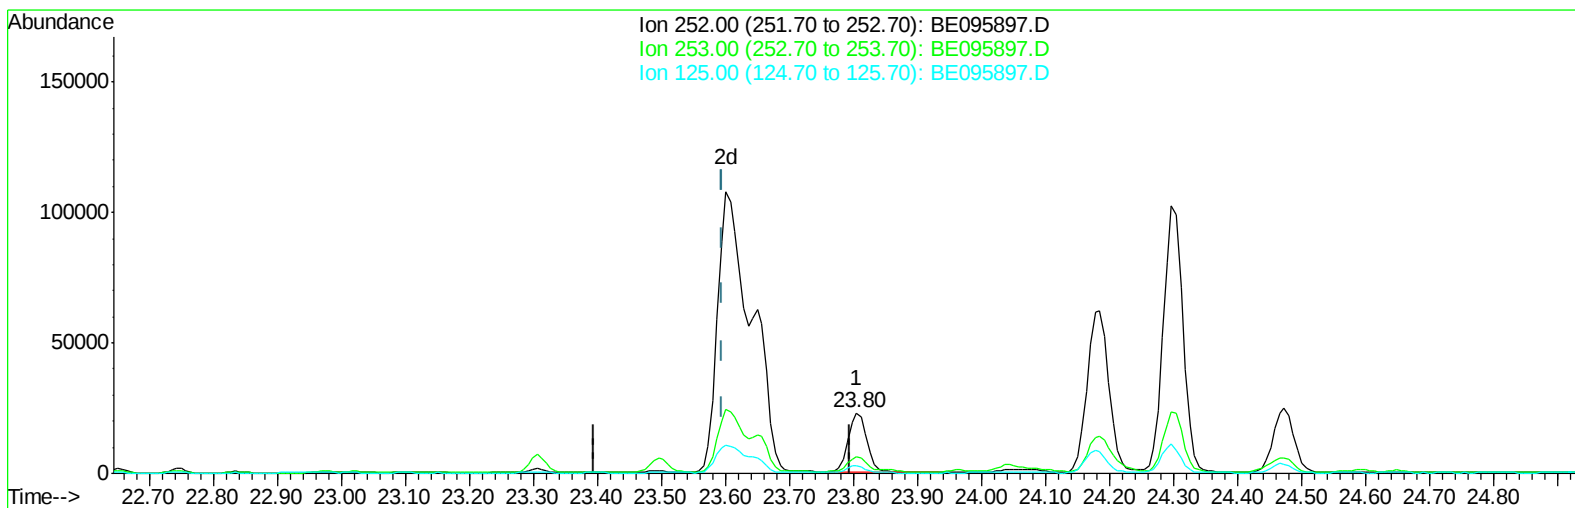

TIC: BE095897.D

(21) Benzo(b)fluoranthene

23.804min (+0.210) 1.43ng/ul

response 46842

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 100   |
| 253.00 | 32.10 | 27.02 |
| 125.00 | 17.50 | 12.96 |
| 0.00   | 0.00  | 0.00  |