
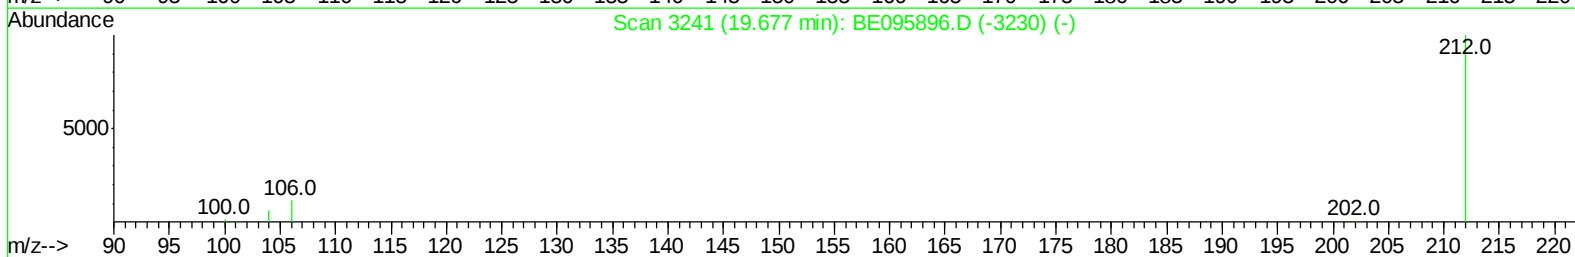
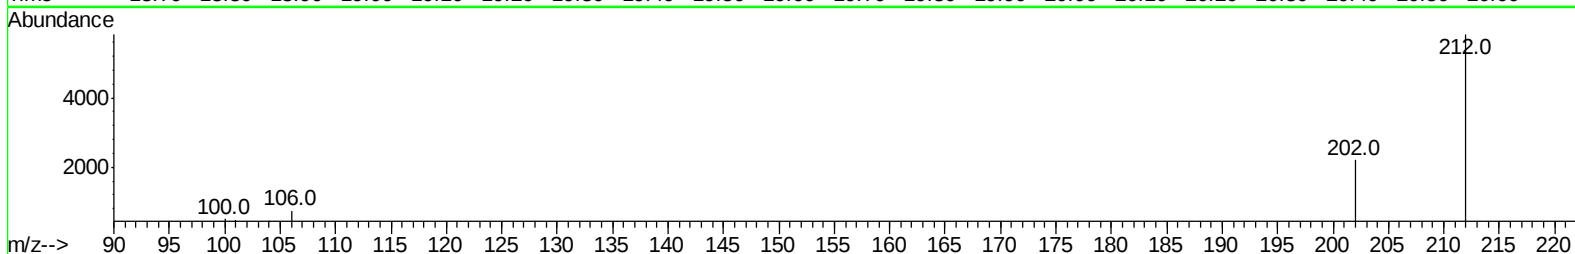


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095898.D
Acq On : 29 Mar 2018 3:52
Operator : SJ/JU
Sample : J1951-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Mar 29 07:17:18 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 07:00:13 2018
Response via : Initial Calibration

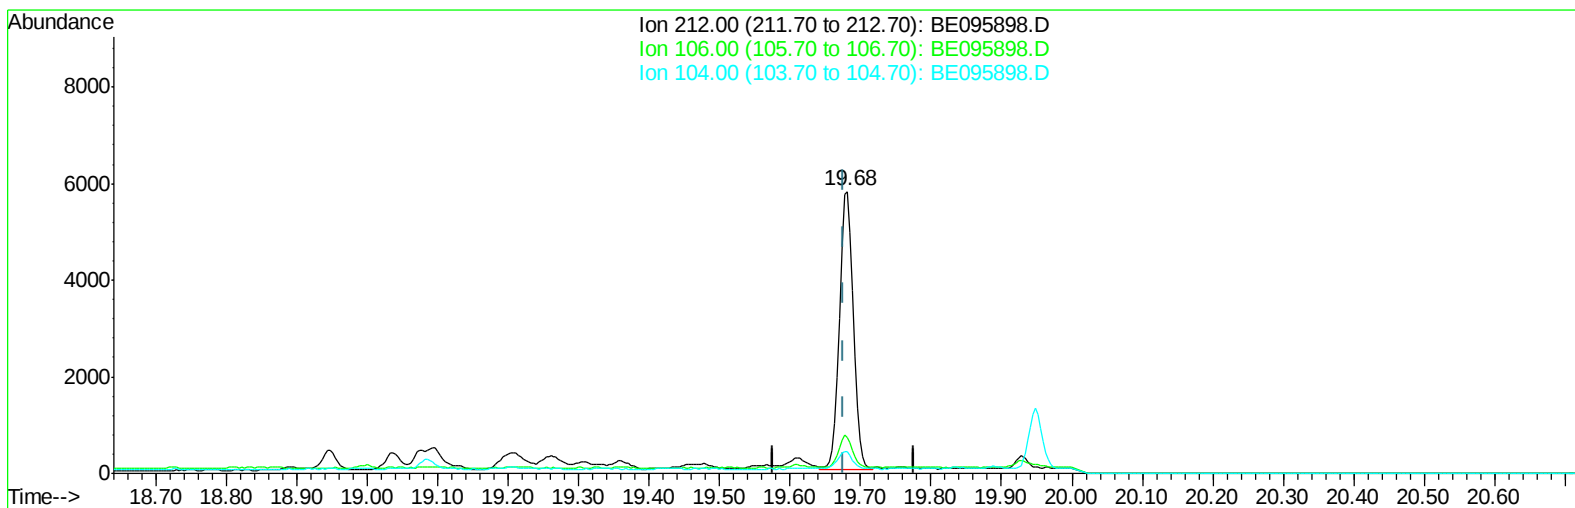

TIC: BE095898.D

(14) Fluoranthene-d10 (SURR)

19.681min (+0.004) 0.29ng/ul m

response 7723

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00