
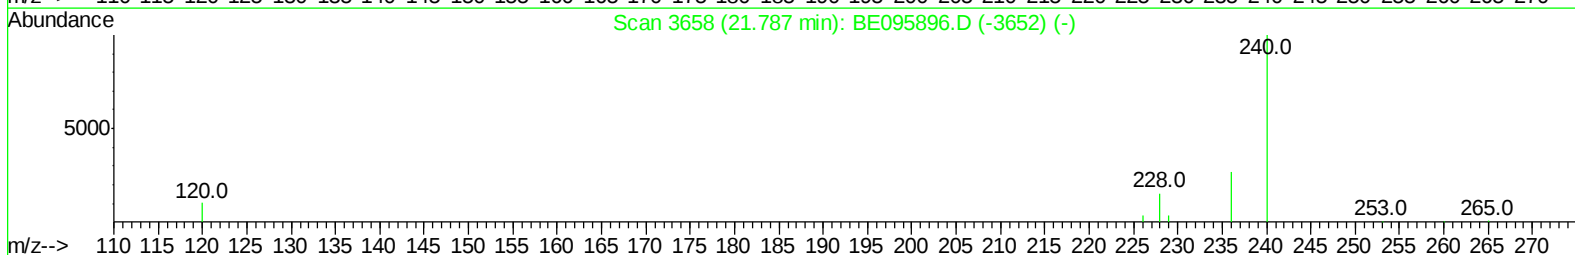
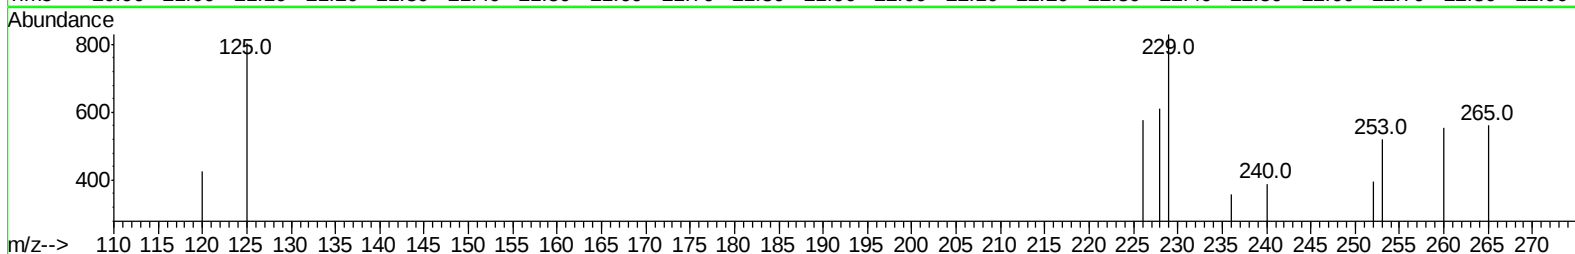


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095900.D
Acq On : 29 Mar 2018 5:03
Operator : SJ/JU
Sample : J1951-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Mar 29 07:01:24 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 07:00:13 2018
Response via : Initial Calibration

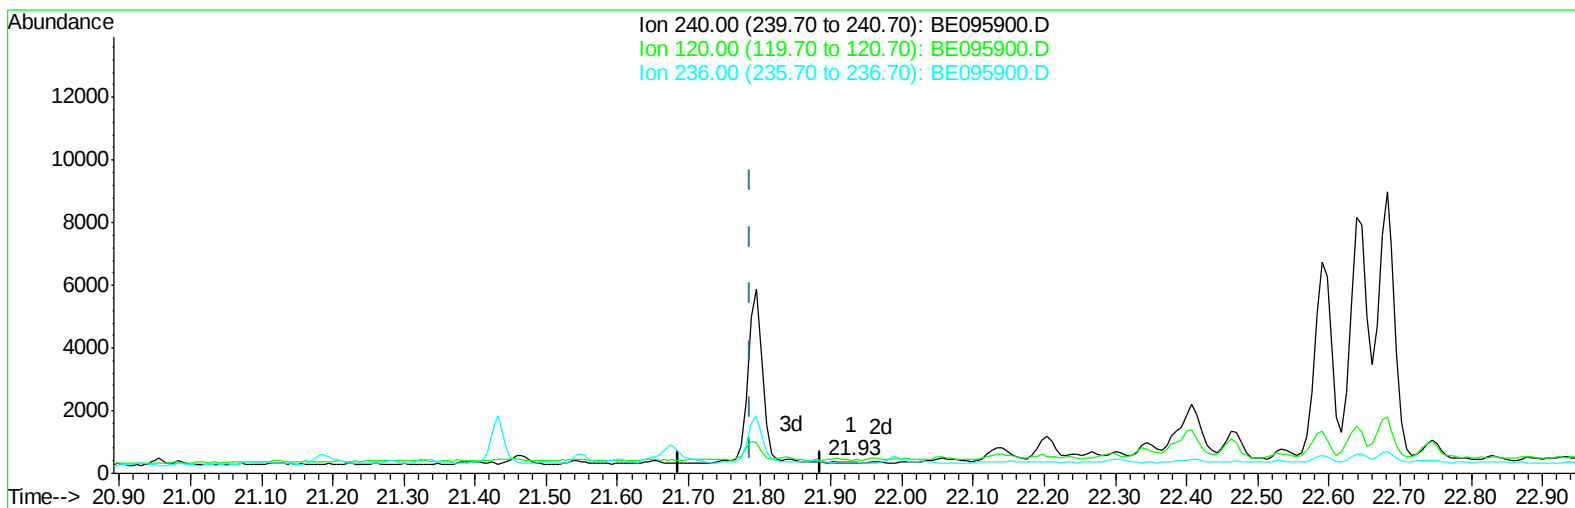

TIC: BE095900.D

(16) Chrysene-d12 (I)

21.929min (+0.142) 0.40ng/ul

response 112

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	110.05#
236.00	34.90	92.01#
0.00	0.00	0.00