
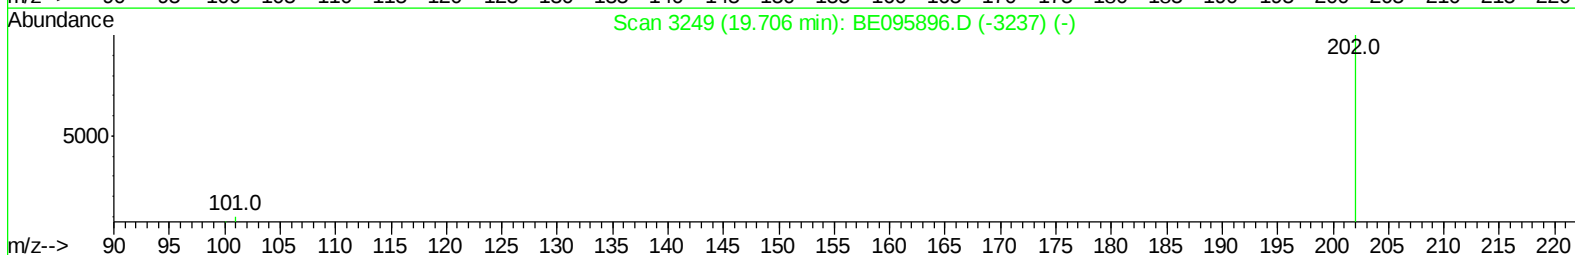
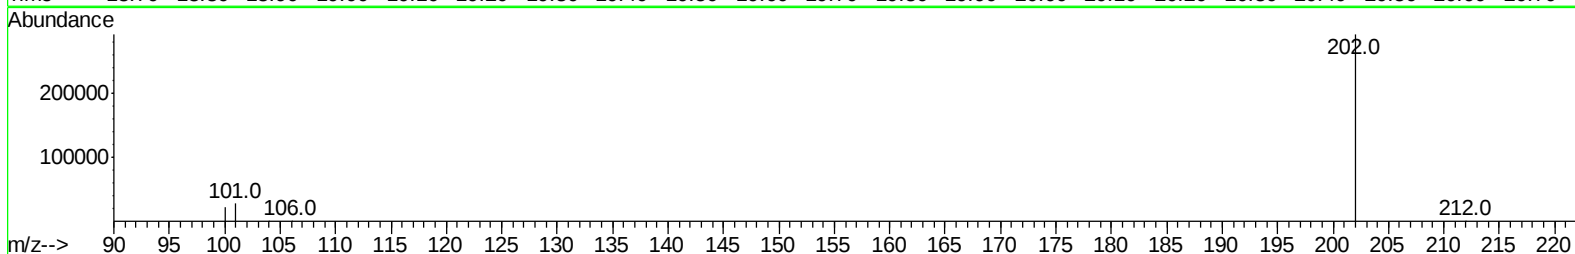


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\  
Data File : BE095900.D  
Acq On : 29 Mar 2018 5:03  
Operator : SJ/JU  
Sample : J1951-01  
Misc :  
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Mar 29 07:36:16 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 29 07:00:13 2018  
Response via : Initial Calibration

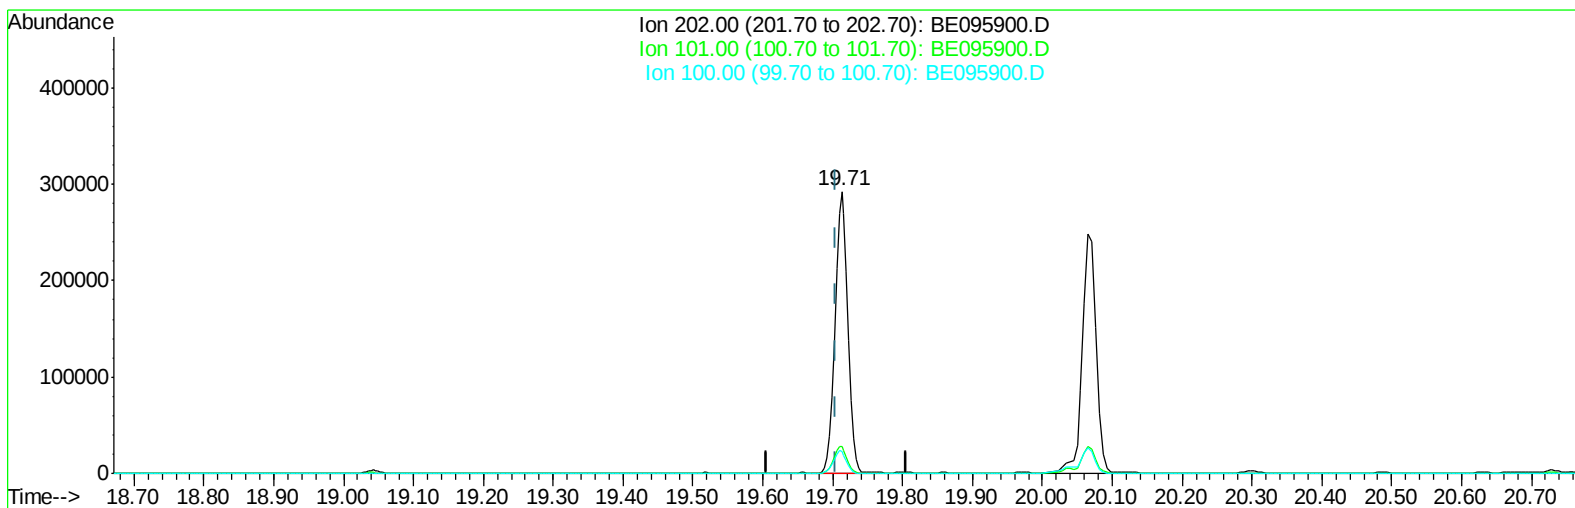

TIC: BE095900.D

(15) Fluoranthene (C)

19.713min (+0.007) 13.21ng/ul m

response 386954

| Ion    | Exp%  | Act% |
|--------|-------|------|
| 202.00 | 100   | 100  |
| 101.00 | 10.30 | 9.39 |
| 100.00 | 19.50 | 7.85 |
| 0.00   | 0.00  | 0.00 |