
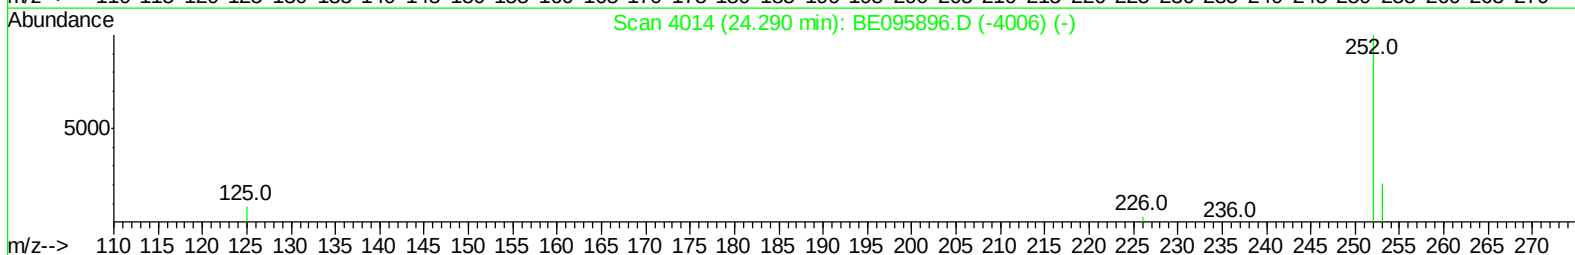
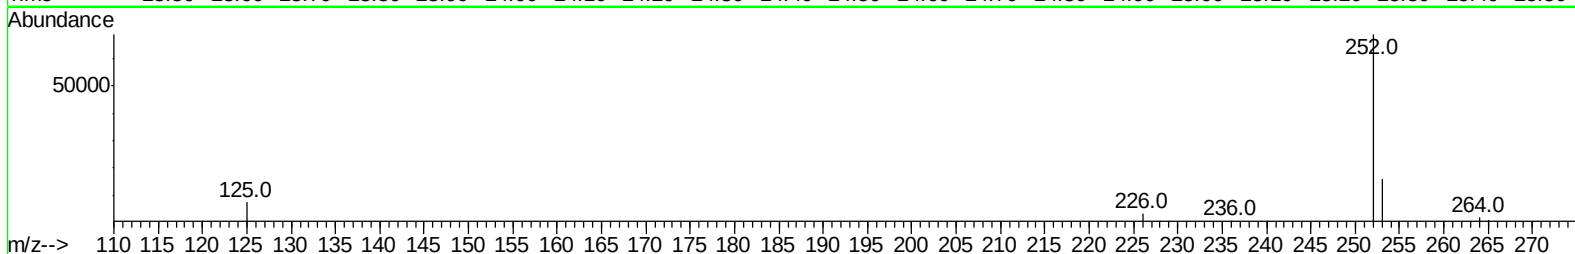


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095901.D
Acq On : 29 Mar 2018 5:39
Operator : SJ/JU
Sample : J2060-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Mar 29 07:50:14 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 07:00:13 2018
Response via : Initial Calibration

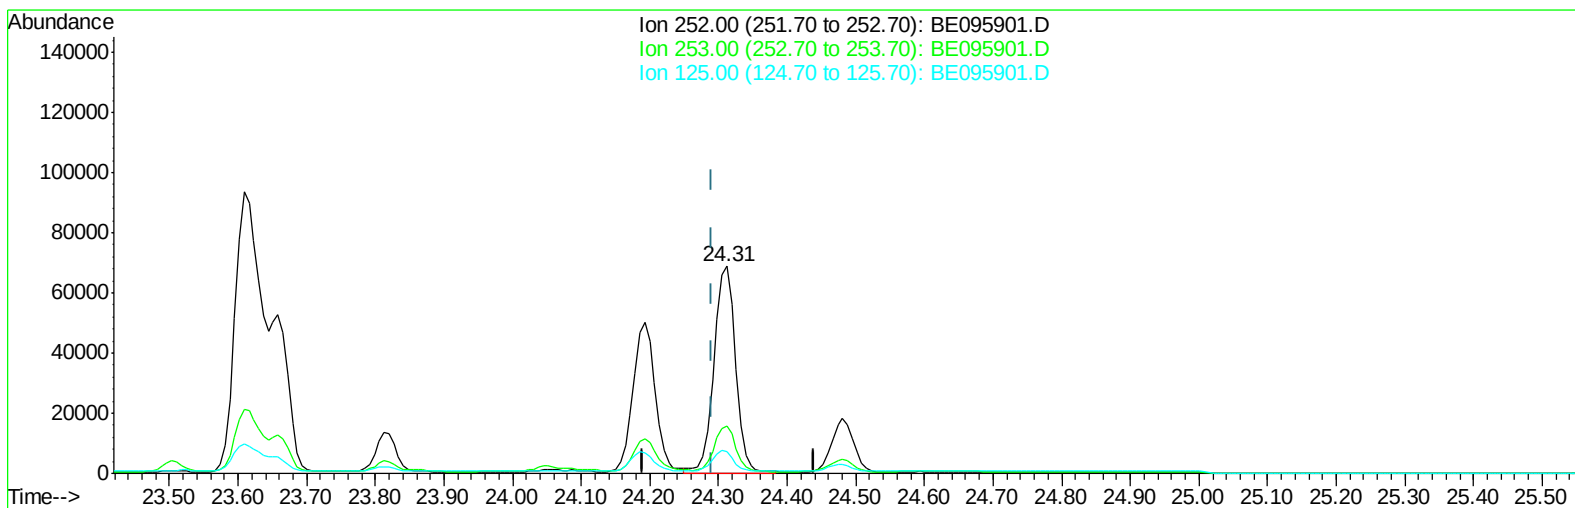

TIC: BE095901.D

(23) Benzo(a)pyrene (C)

24.312min (+0.022) 5.01ng/ul m

response 152574

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	23.08#
125.00	22.60	10.48#
0.00	0.00	0.00