
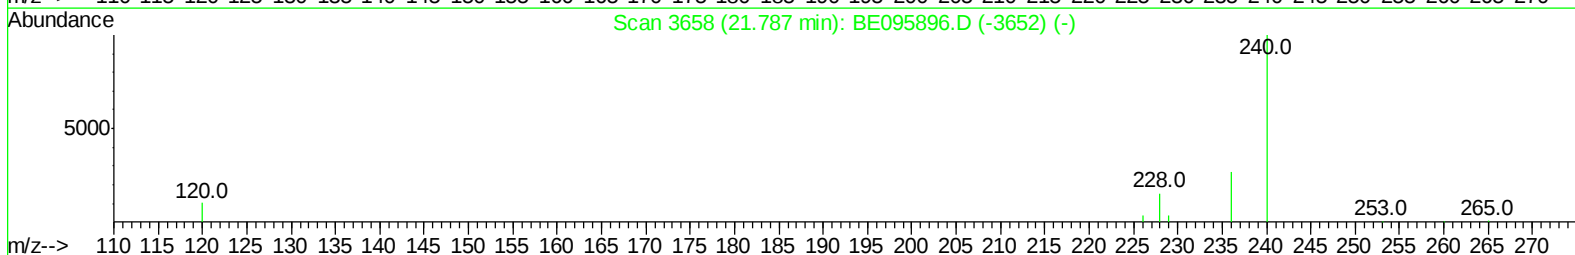
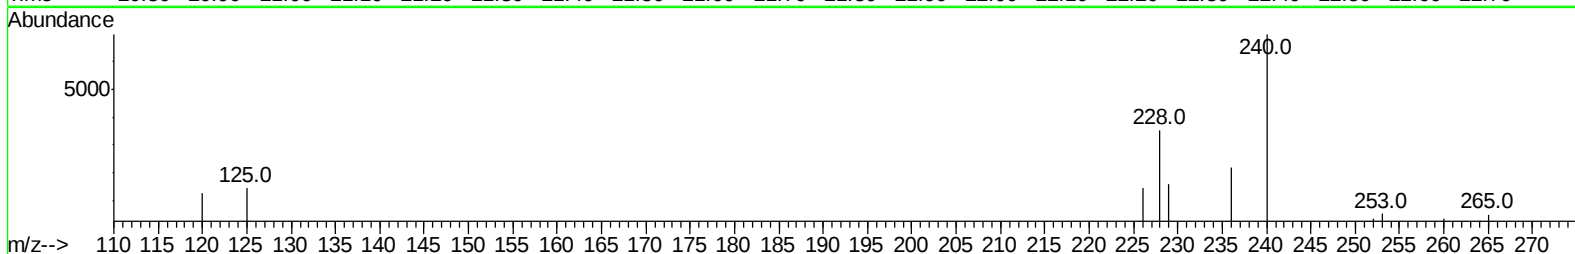


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095902.D
Acq On : 29 Mar 2018 6:15
Operator : SJ/JU
Sample : J2060-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Mar 29 07:01:48 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 07:00:13 2018
Response via : Initial Calibration

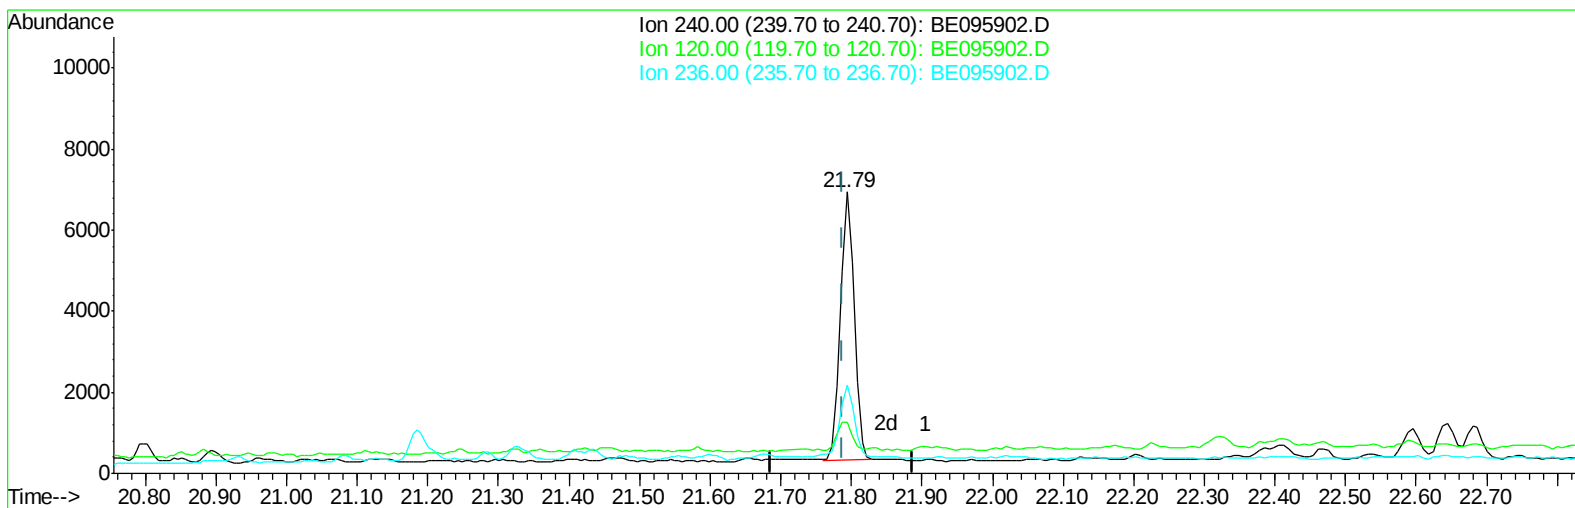

TIC: BE095902.D

(16) Chrysene-d12 (I)

21.794min (+0.007) 0.40ng/ul m

response 8776

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	18.34
236.00	34.90	31.45
0.00	0.00	0.00