
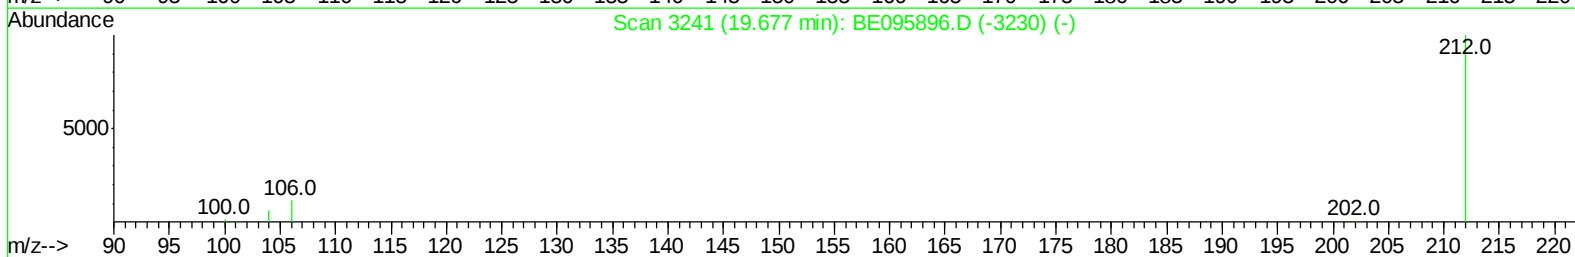
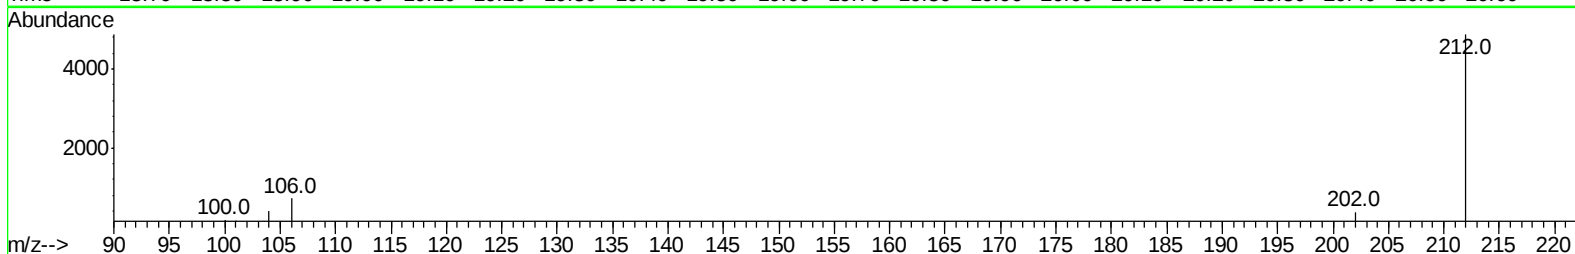


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095902.D
Acq On : 29 Mar 2018 6:15
Operator : SJ/JU
Sample : J2060-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Mar 29 07:53:31 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 07:00:13 2018
Response via : Initial Calibration

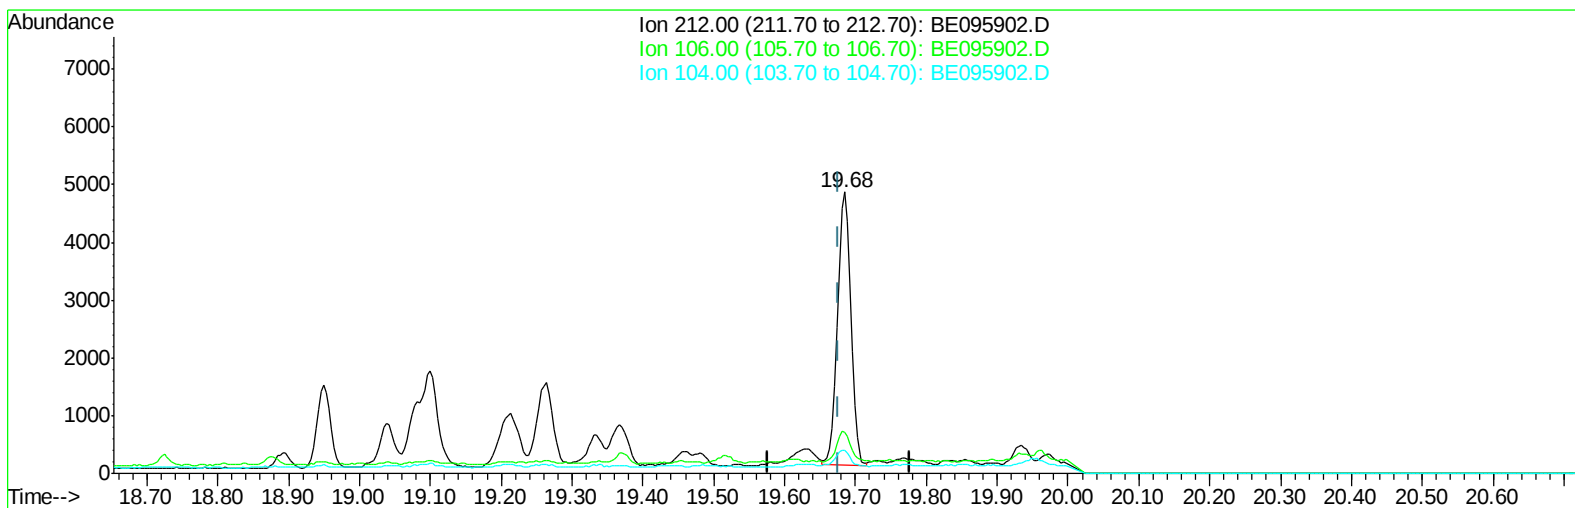

TIC: BE095902.D

(14) Fluoranthene-d10 (SURR)

19.684min (+0.007) 0.21ng/ul m

response 6113

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.31#
104.00	15.60	1.10#
0.00	0.00	0.00