
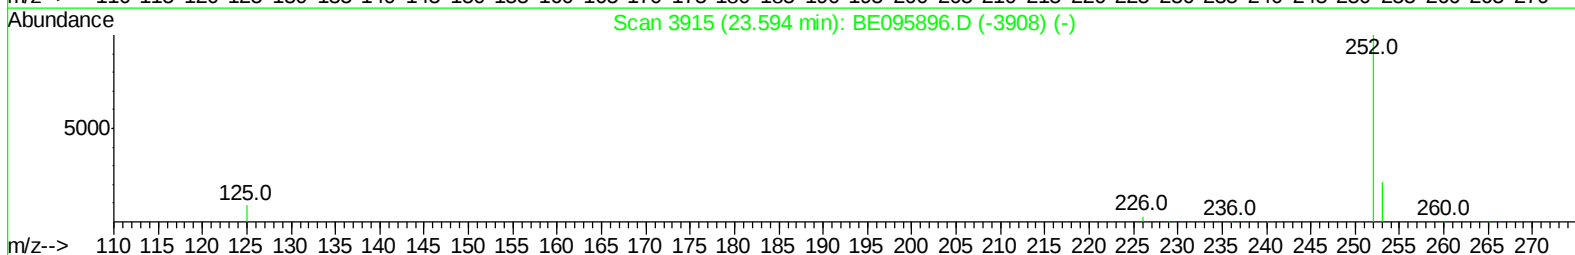
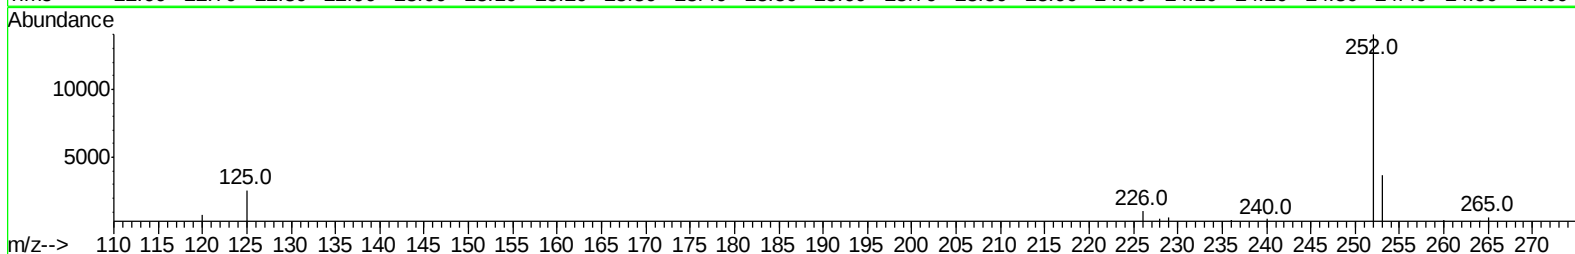


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095902.D
Acq On : 29 Mar 2018 6:15
Operator : SJ/JU
Sample : J2060-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Mar 29 07:53:31 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 07:00:13 2018
Response via : Initial Calibration

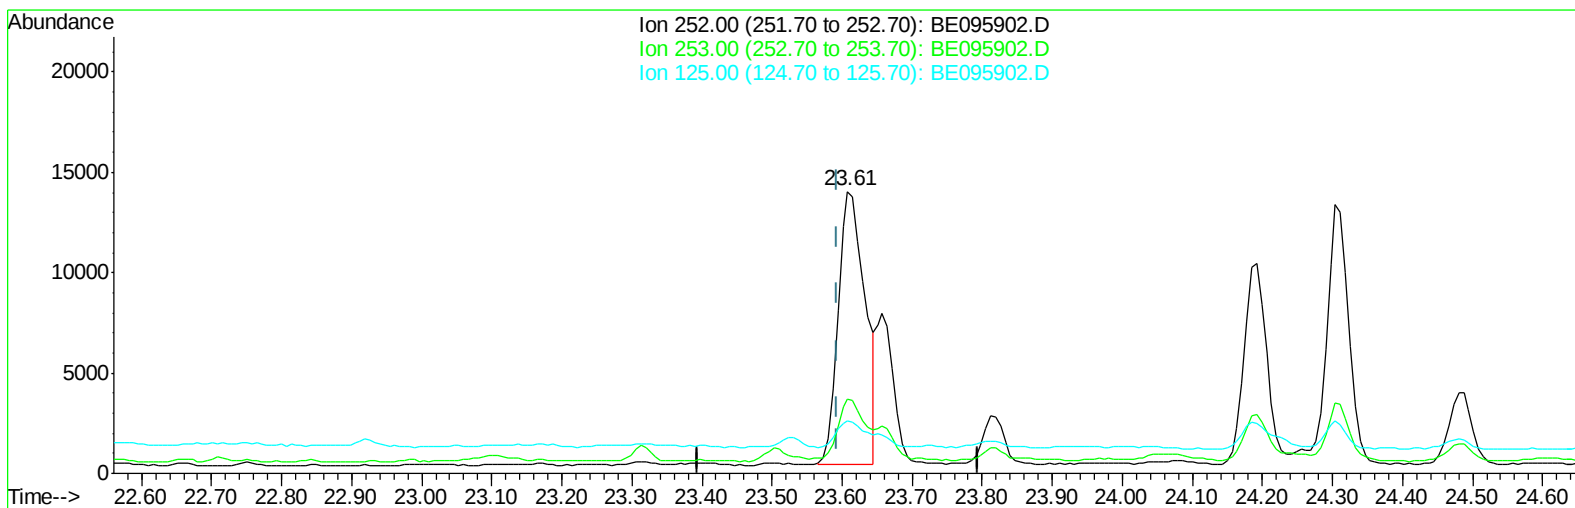

TIC: BE095902.D

(21) Benzo(b)fluoranthene

23.608min (+0.014) 1.09ng/ul m

response 36237

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	26.33
125.00	17.50	18.51
0.00	0.00	0.00