
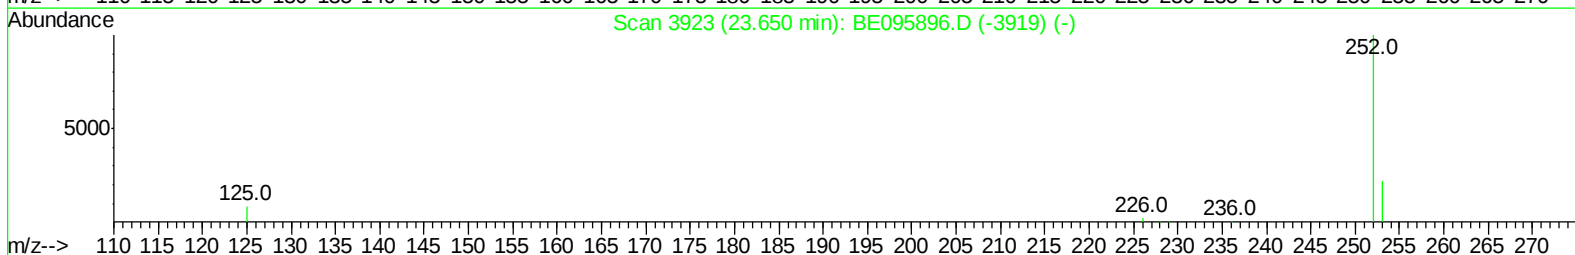
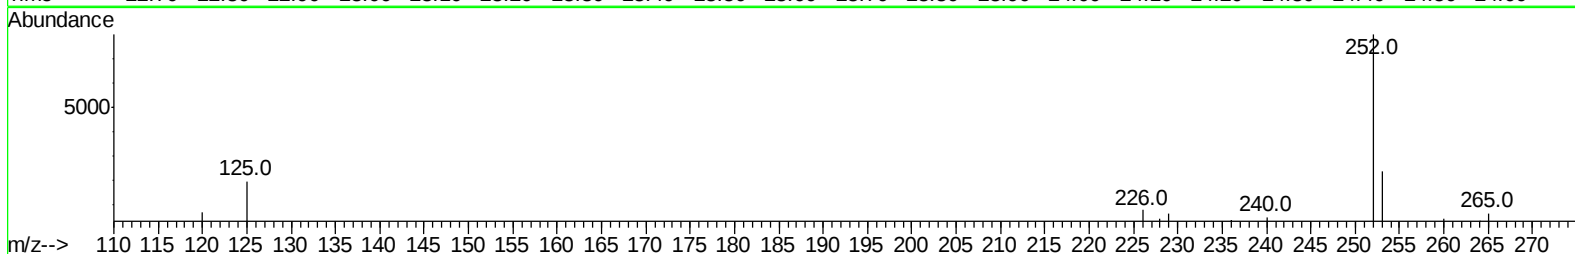


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095902.D
Acq On : 29 Mar 2018 6:15
Operator : SJ/JU
Sample : J2060-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Mar 29 07:53:31 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 07:00:13 2018
Response via : Initial Calibration

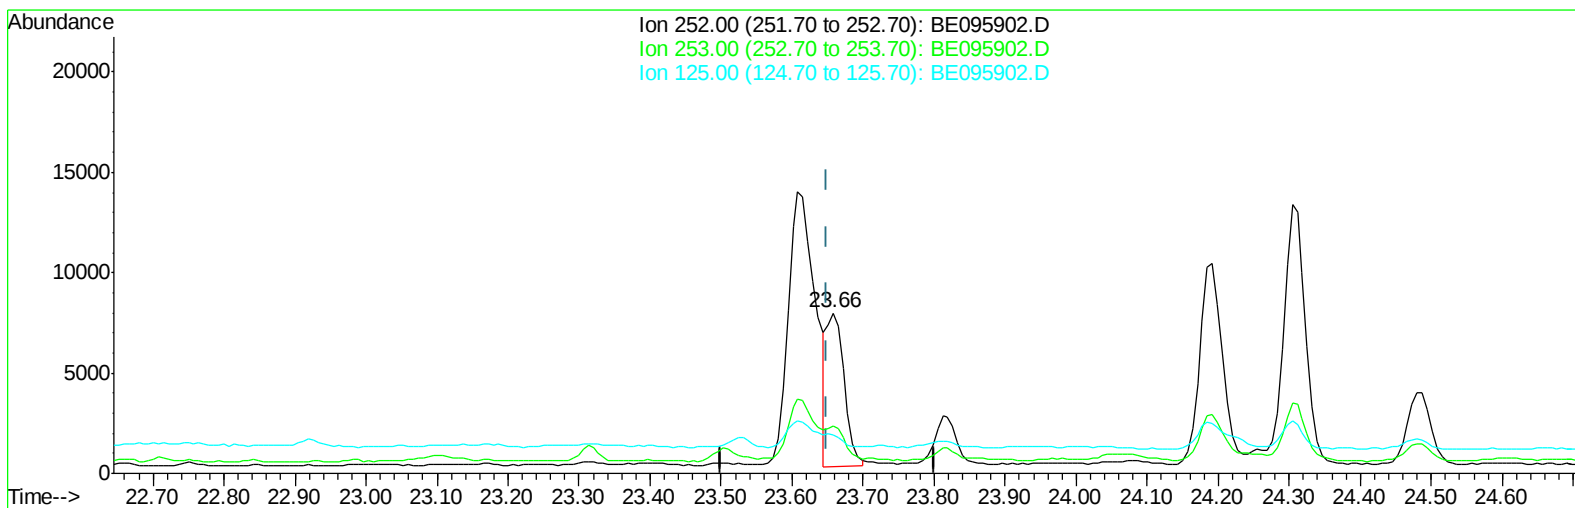

TIC: BE095902.D

(22) Benzo(k)fluoranthene

23.657min (+0.007) 0.41ng/ul m

response 13164

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	29.40
125.00	17.10	24.35#
0.00	0.00	0.00