
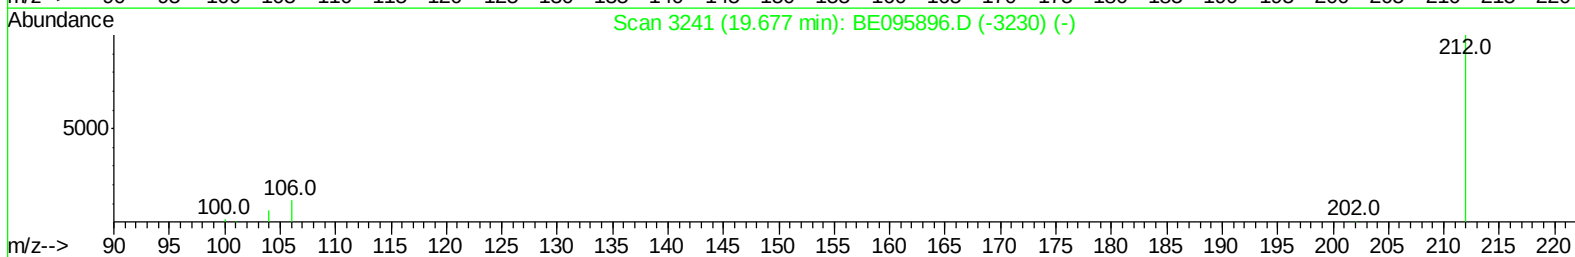
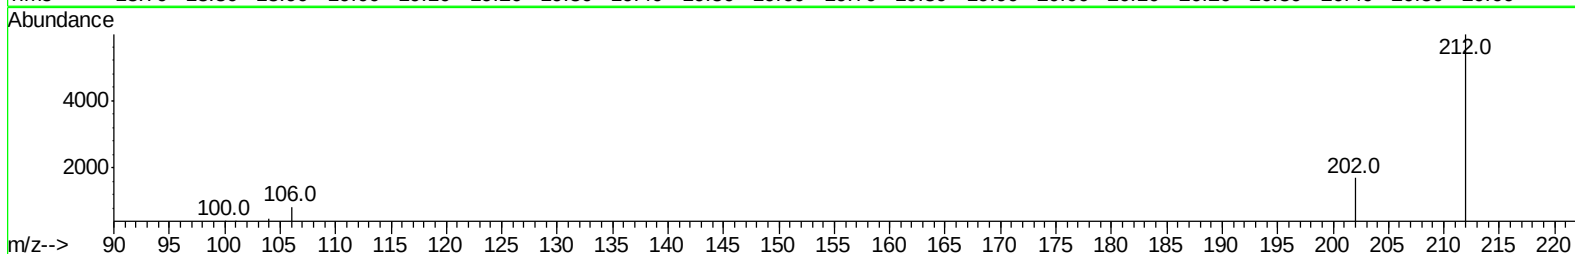


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\  
Data File : BE095903.D  
Acq On : 29 Mar 2018 6:51  
Operator : SJ/JU  
Sample : J2060-02  
Misc :  
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Mar 29 08:03:24 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 29 07:00:13 2018  
Response via : Initial Calibration

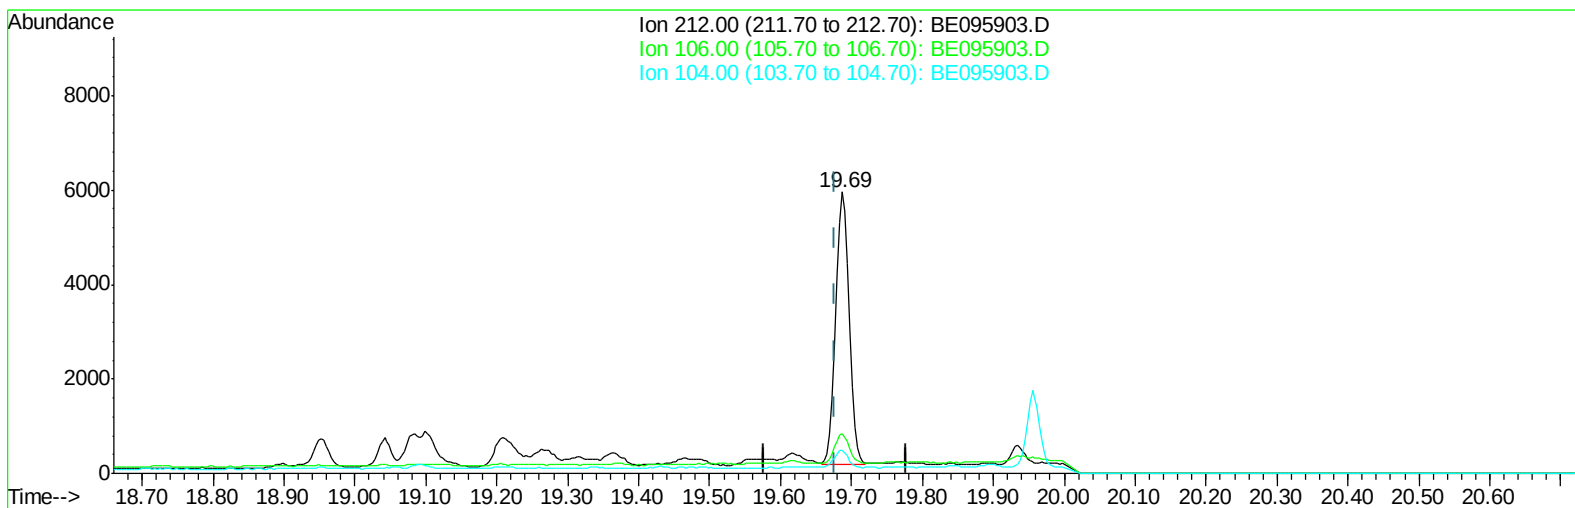

TIC: BE095903.D

(14) Fluoranthene-d10 (SURR)

19.687min (+0.010) 0.29ng/ul m

response 7592

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 212.00 | 100   | 100   |
| 106.00 | 18.30 | 0.00# |
| 104.00 | 15.60 | 0.00# |
| 0.00   | 0.00  | 0.00  |