
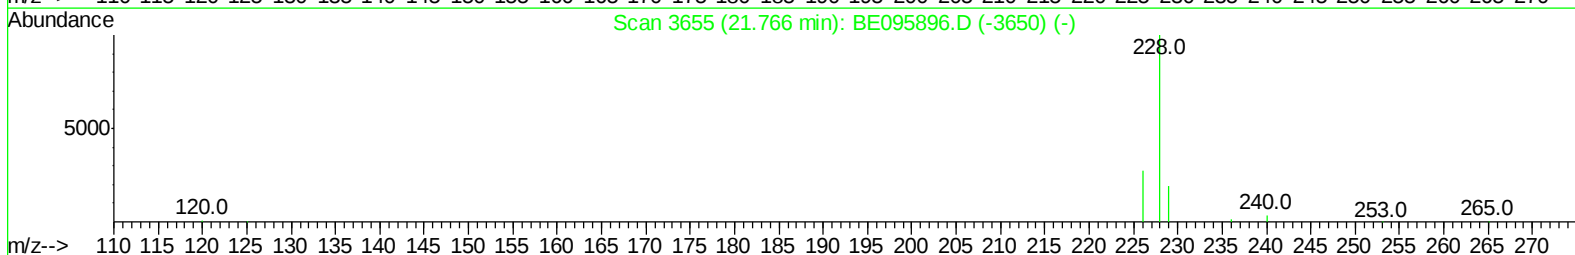
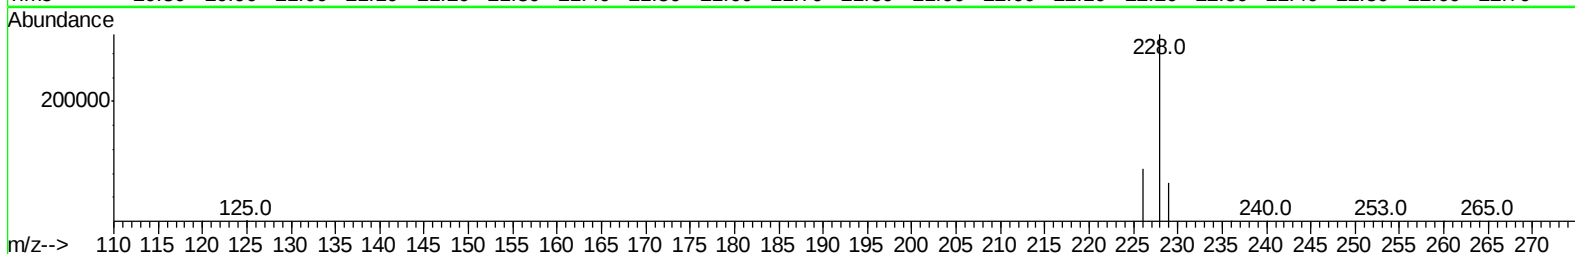


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095903.D
Acq On : 29 Mar 2018 6:51
Operator : SJ/JU
Sample : J2060-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Mar 29 08:03:24 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 07:00:13 2018
Response via : Initial Calibration

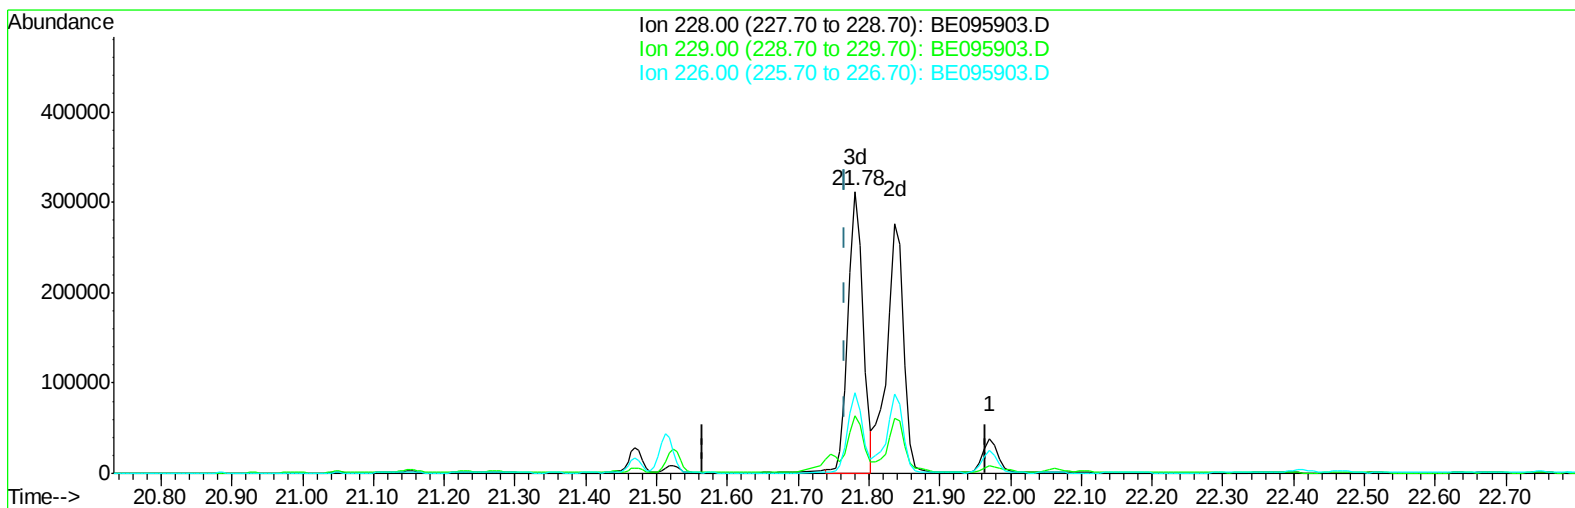

TIC: BE095903.D

(18) Benzo(a)anthracene

21.781min (+0.015) 18.29ng/ul m

response 451921

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	20.50#
226.00	21.30	28.50#
0.00	0.00	0.00