
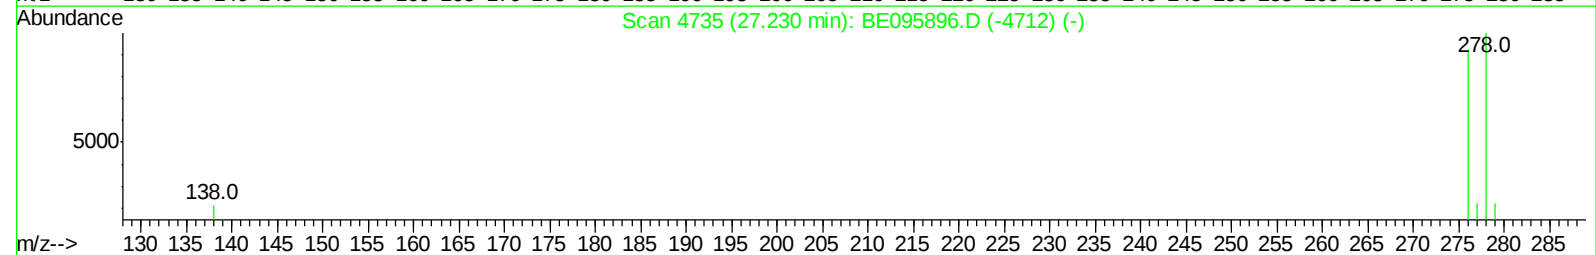
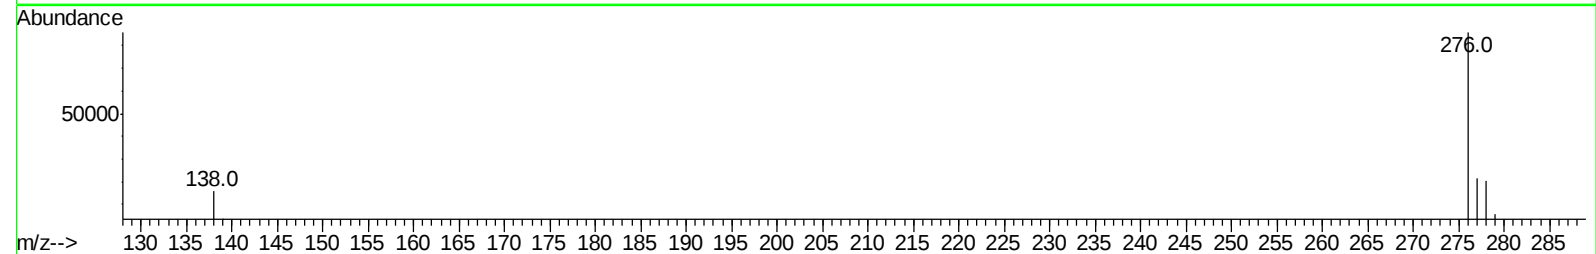


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095903.D
Acq On : 29 Mar 2018 6:51
Operator : SJ/JU
Sample : J2060-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Mar 29 08:03:24 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 07:00:13 2018
Response via : Initial Calibration

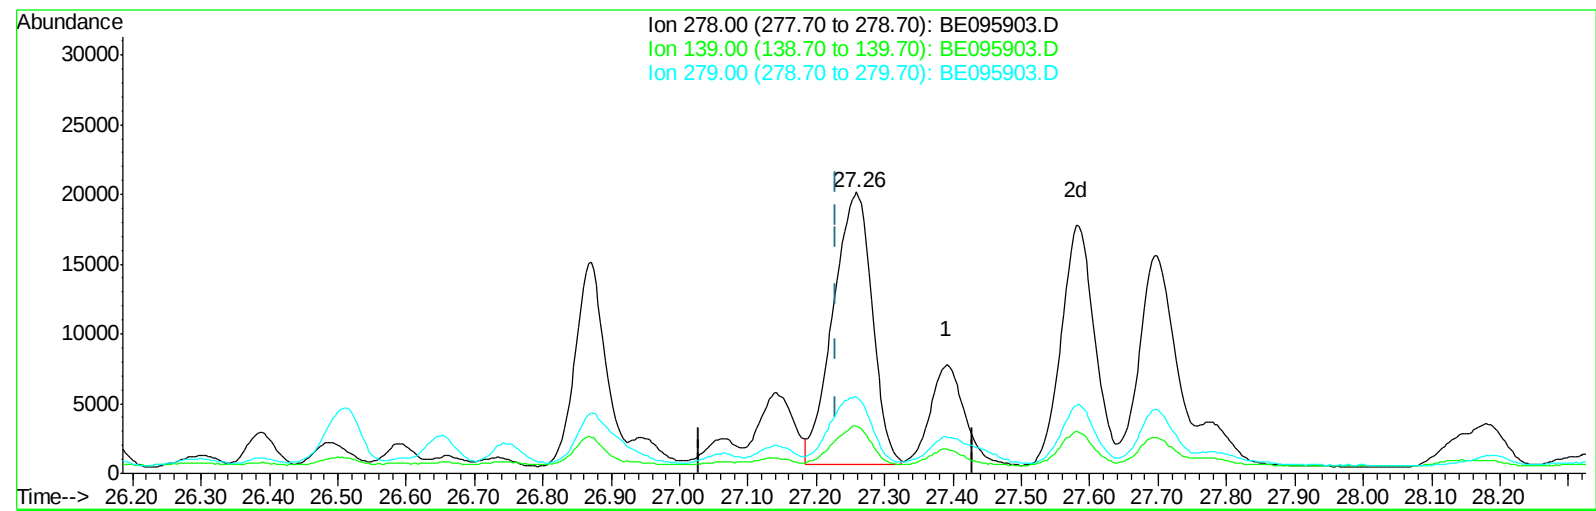

TIC: BE095903.D

(25) Dibenzo(a,h)anthracene

27.259min (+0.029) 2.86ng/ul m

response 77390

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	16.75#
279.00	32.40	27.17
0.00	0.00	0.00