

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
 Data File : BE095871.D
 Acq On : 28 Mar 2018 11:20
 Operator : SJ/JU
 Sample : PB107681BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Mar 28 16:25:53 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 16 02:40:12 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.42	152	1689	0.40	ng/ul	-0.03
2) Naphthalene-d8	11.24	136	4600	0.40	ng/ul	-0.04
6) Acenaphthene-d10	14.99	164	3067	0.40	ng/ul	-0.04
10) Phenanthrene-d10	17.80	188	568385	0.40	ng/ul	0.06
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.84
20) Perylene-d12	24.42	264	9802	0.40	ng/ul	-0.08
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.79	152	2773	0.36	ng/ul	-0.03
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.97	166	939	0.074	ng/ul#	23
23) Benzo(a)pyrene	24.25	252	2358	0.076	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095871.D
Acq On : 28 Mar 2018 11:20
Operator : SJ/JU
Sample : PB107681BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Mar 28 16:25:53 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 16 02:40:12 2018
Response via : Initial Calibration

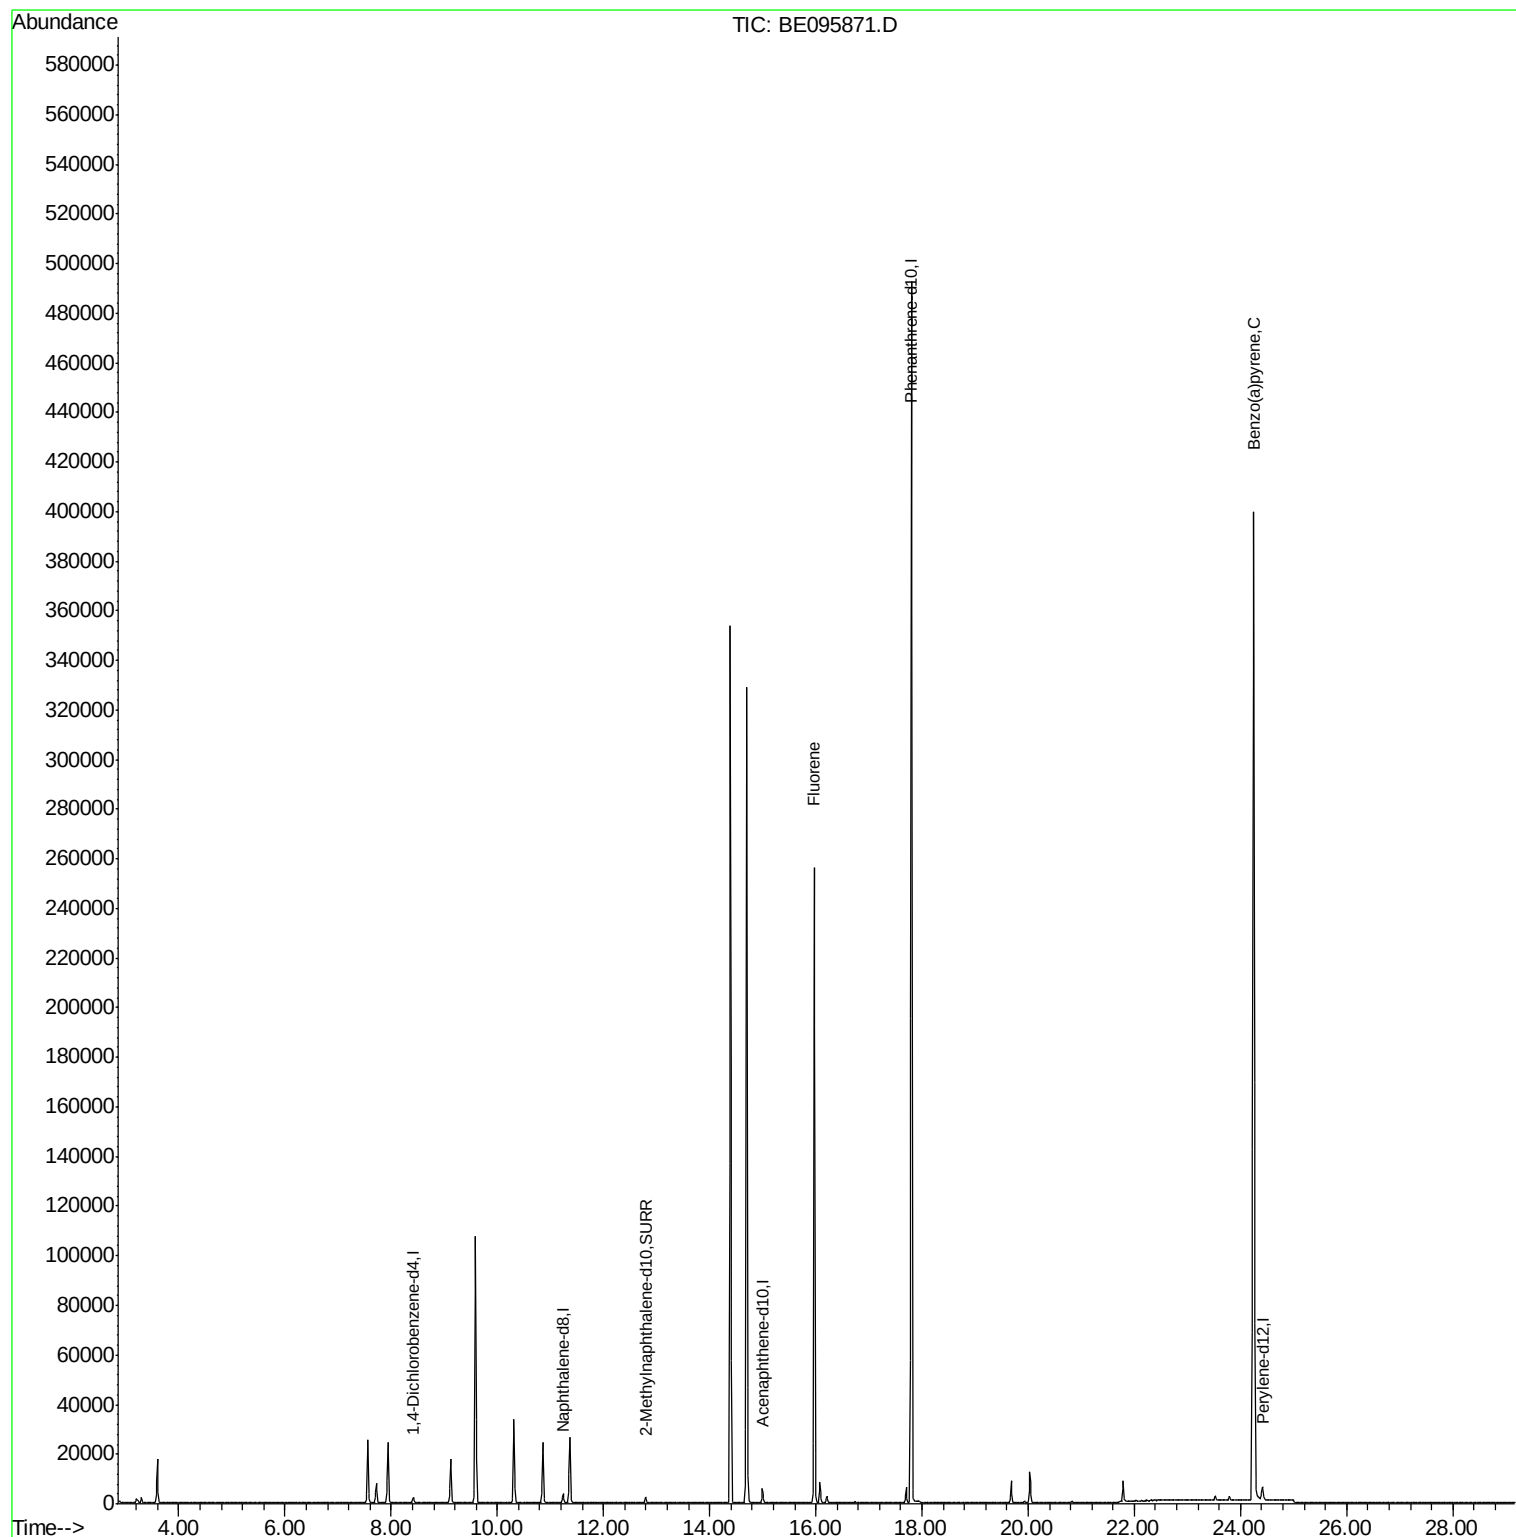

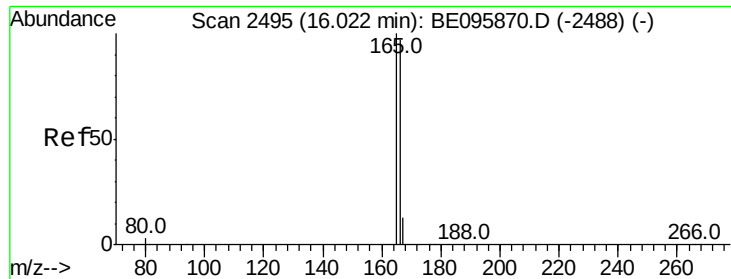

#9

Fluorene

Concen: 0.074 ng/ul

RT: 15.97 min Scan# 2489

Delta R.T. -0.09 min

Lab File: BE095871.D

Acq: 28 Mar 2018 11:20

Instrument :

BNA_E

ClientSampleId :





Tot Ion:166 Resp: 939

Ion Ratio Lower Upper

166 100

165 12.0 73.4 110.2#

167 36.6 14.6 22.0#

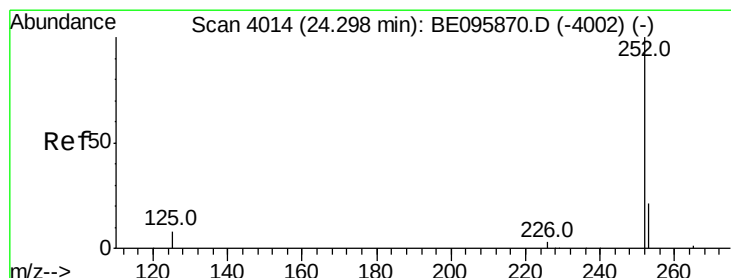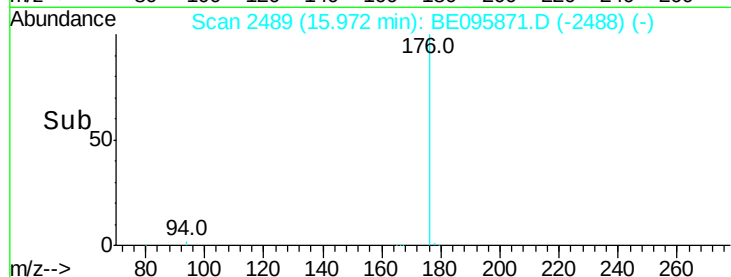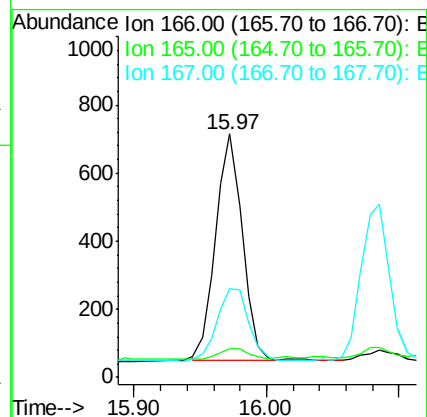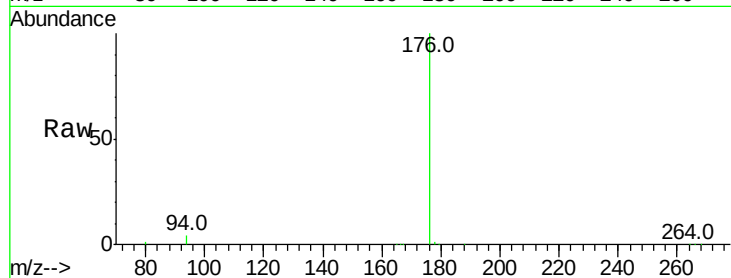

#23

Benzo(a)pyrene

Concen: 0.076 ng/ul

RT: 24.25 min Scan# 4009

Delta R.T. -0.13 min

Lab File: BE095871.D

Acq: 28 Mar 2018 11:20

Tgt Ion:252 Resp: 2358

Ion Ratio Lower Upper

252 100

253 42.0 28.5 42.7

125 36.4 18.1 27.1#

