

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\  
 Data File : BE095873.D  
 Acq On : 28 Mar 2018 12:59  
 Operator : SJ/JU  
 Sample : J2060-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :

Quant Time: Mar 28 16:26:13 2018  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Mar 28 16:25:04 2018  
 Response via : Initial Calibration


| Internal Standards          | R.T.  | QIon | Response | Conc  | Units  | Dev(Min) |
|-----------------------------|-------|------|----------|-------|--------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 8.42  | 152  | 1650     | 0.40  | ng/ul  | -0.03    |
| 2) Naphthalene-d8           | 11.24 | 136  | 4428     | 0.40  | ng/ul  | -0.04    |
| 6) Acenaphthene-d10         | 15.00 | 164  | 2945     | 0.40  | ng/ul  | -0.04    |
| 10) Phenanthrene-d10        | 17.80 | 188  | 518462   | 0.40  | ng/ul  | 0.06     |
| 16) Chrysene-d12            | 0.00  | 240  | 0        | 0.00  | ng/ul  | -21.84   |
| 20) Perylene-d12            | 24.41 | 264  | 9301     | 0.40  | ng/ul  | -0.09    |
| System Monitoring Compounds |       |      |          |       |        |          |
| 4) 2-Methylnaphthalene-d10  | 12.80 | 152  | 2622     | 0.35  | ng/ul  | -0.03    |
| 14) Fluoranthene-d10        | 0.00  | 212  | 0        | 0.00  | ng/ul  |          |
| Target Compounds            |       |      |          |       |        |          |
| 21) Benzo(b)fluoranthene    | 23.60 | 252  | 1262     | 0.039 | ng/ul# | 56       |
| 22) Benzo(k)fluoranthene    | 23.60 | 252  | 1252     | 0.041 | ng/ul# | 53       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\  
Data File : BE095873.D  
Acq On : 28 Mar 2018 12:59  
Operator : SJ/JU  
Sample : J2060-07  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :

Quant Time: Mar 28 16:26:13 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 28 16:25:04 2018  
Response via : Initial Calibration

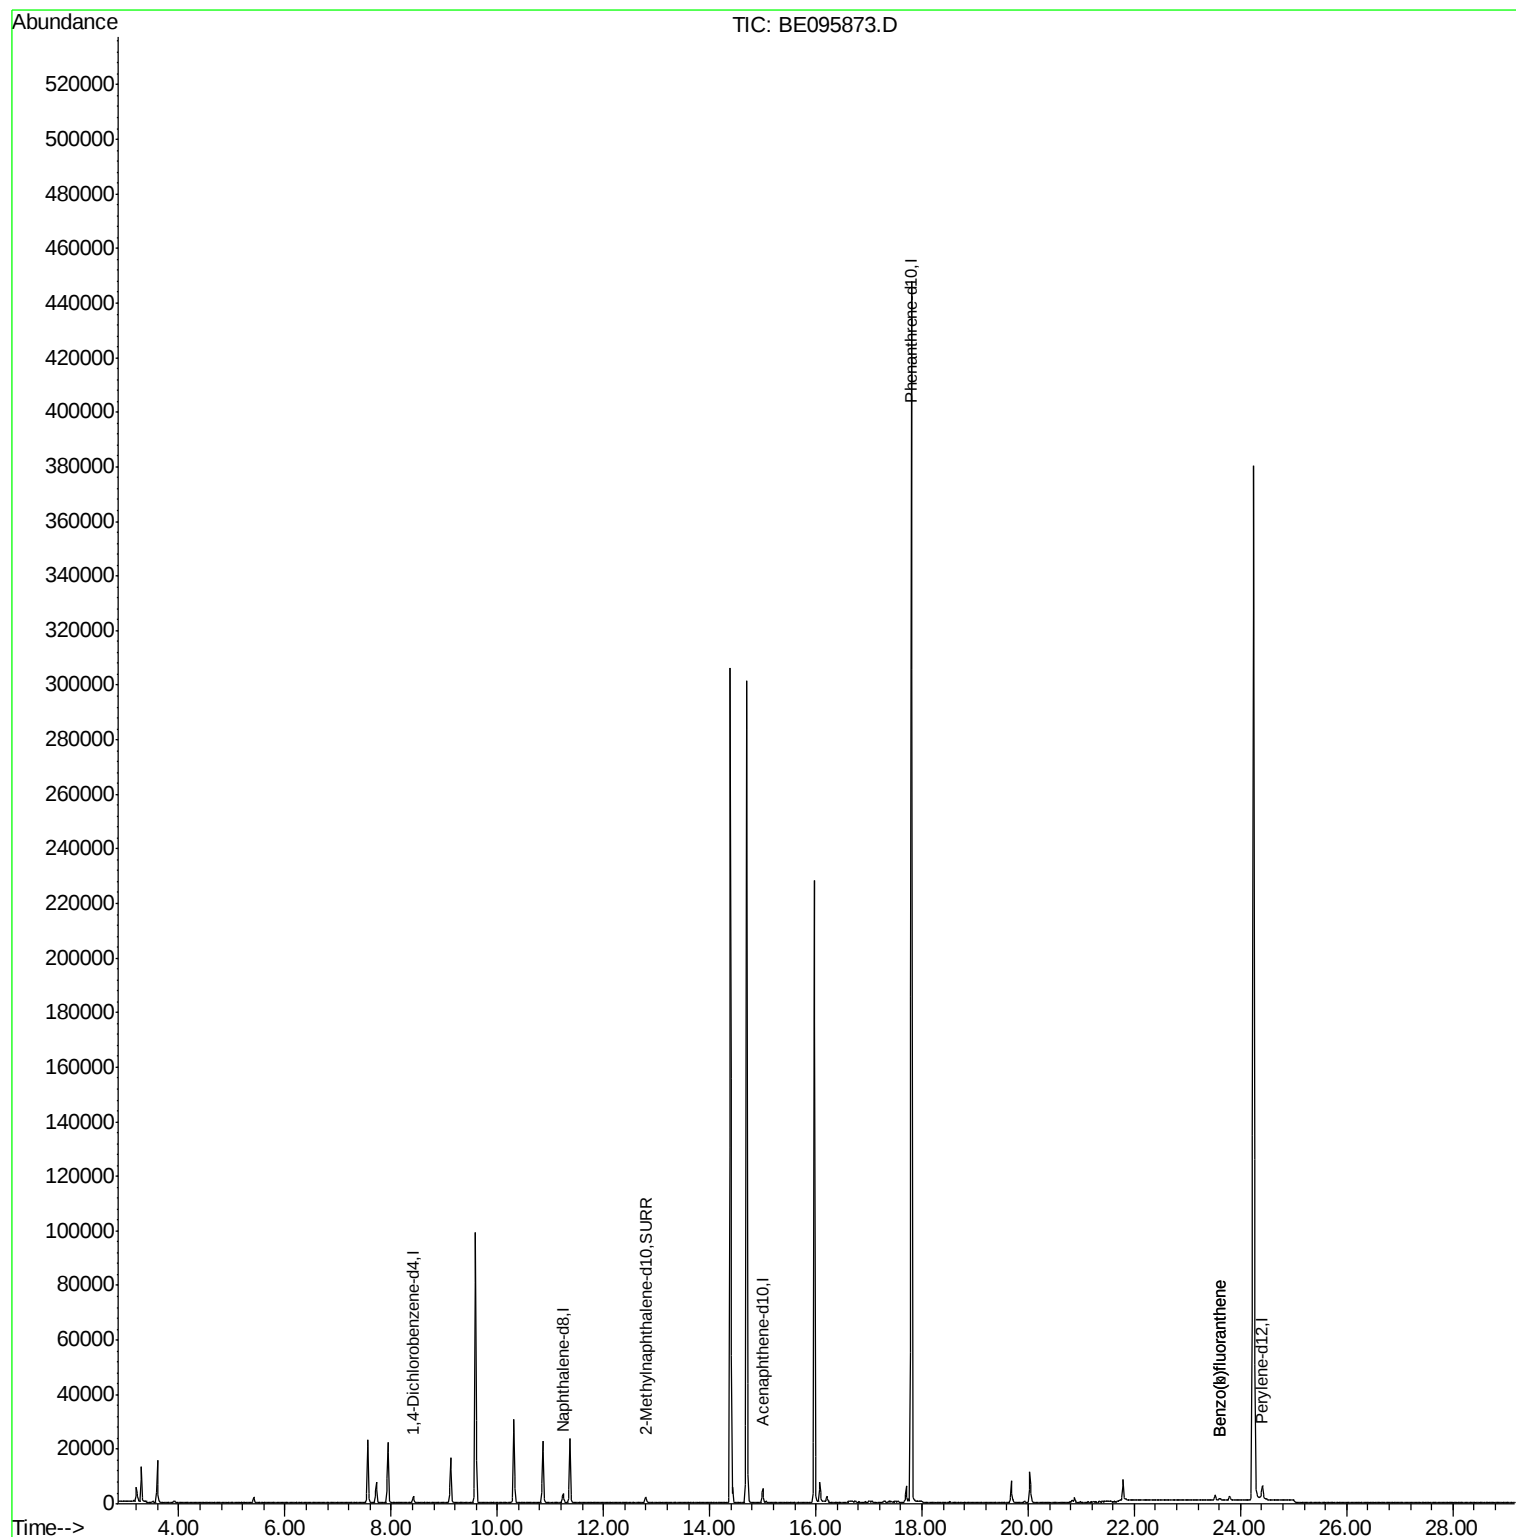

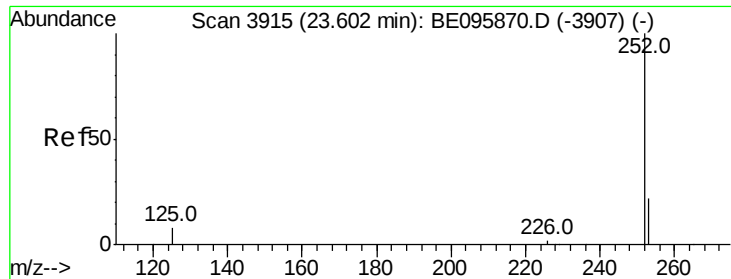

#21

Benzo(b)fluoranthene

Concen: 0.039 ng/ul

RT: 23.60 min Scan# 3917

Delta R.T. -0.07 min

Lab File: BE095873.D

Acq: 28 Mar 2018 12:59

Instrument :

BNA\_E

ClientSampleId :


Tot Ion:252 Resp: 1262

Ion Ratio Lower Upper

252 100

253 49.4 0.0 64.2



125 47.1 0.0 35.0#

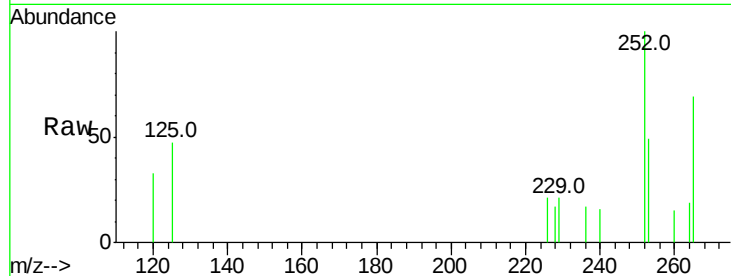

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

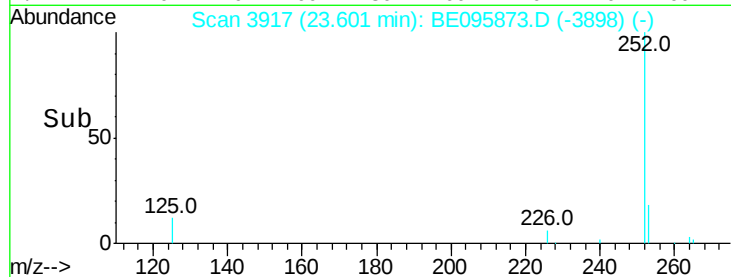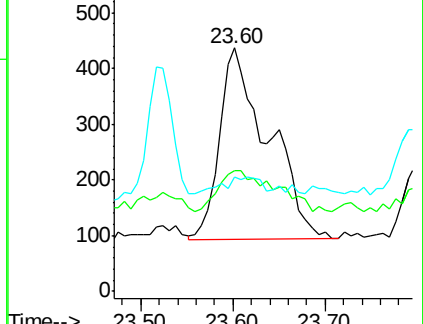

#22

Benzo(k)fluoranthene

Concen: 0.041 ng/ul

RT: 23.60 min Scan# 3917

Delta R.T. -0.12 min

Lab File: BE095873.D

Acq: 28 Mar 2018 12:59



Tgt Ion:252 Resp: 1252

Ion Ratio Lower Upper

252 100

253 49.4 24.5 36.7#

125 47.1 13.7 20.5#

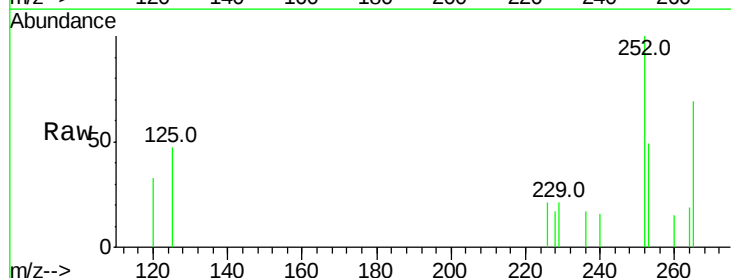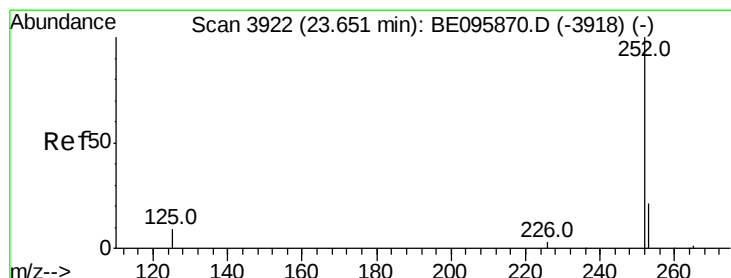

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

