

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
 Data File : BE095876.D
 Acq On : 28 Mar 2018 14:46
 Operator : SJ/JU
 Sample : J1950-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Mar 28 16:27:03 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 28 16:25:04 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.41	152	1643	0.40	ng/ul	-0.04
2) Naphthalene-d8	11.24	136	4416	0.40	ng/ul	-0.04
6) Acenaphthene-d10	15.00	164	2957	0.40	ng/ul	-0.04
10) Phenanthrene-d10	17.80	188	500620	0.40	ng/ul	0.06
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.84
20) Perylene-d12	24.42	264	8942	0.40	ng/ul	-0.08
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.79	152	2478	0.33	ng/ul	-0.04
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
26) Benzo(a,h,i)perylene	28.09	276	559	0.021	ng/ul#	Ovalue 51




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095876.D
Acq On : 28 Mar 2018 14:46
Operator : SJ/JU
Sample : J1950-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Mar 28 16:27:03 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 16:25:04 2018
Response via : Initial Calibration

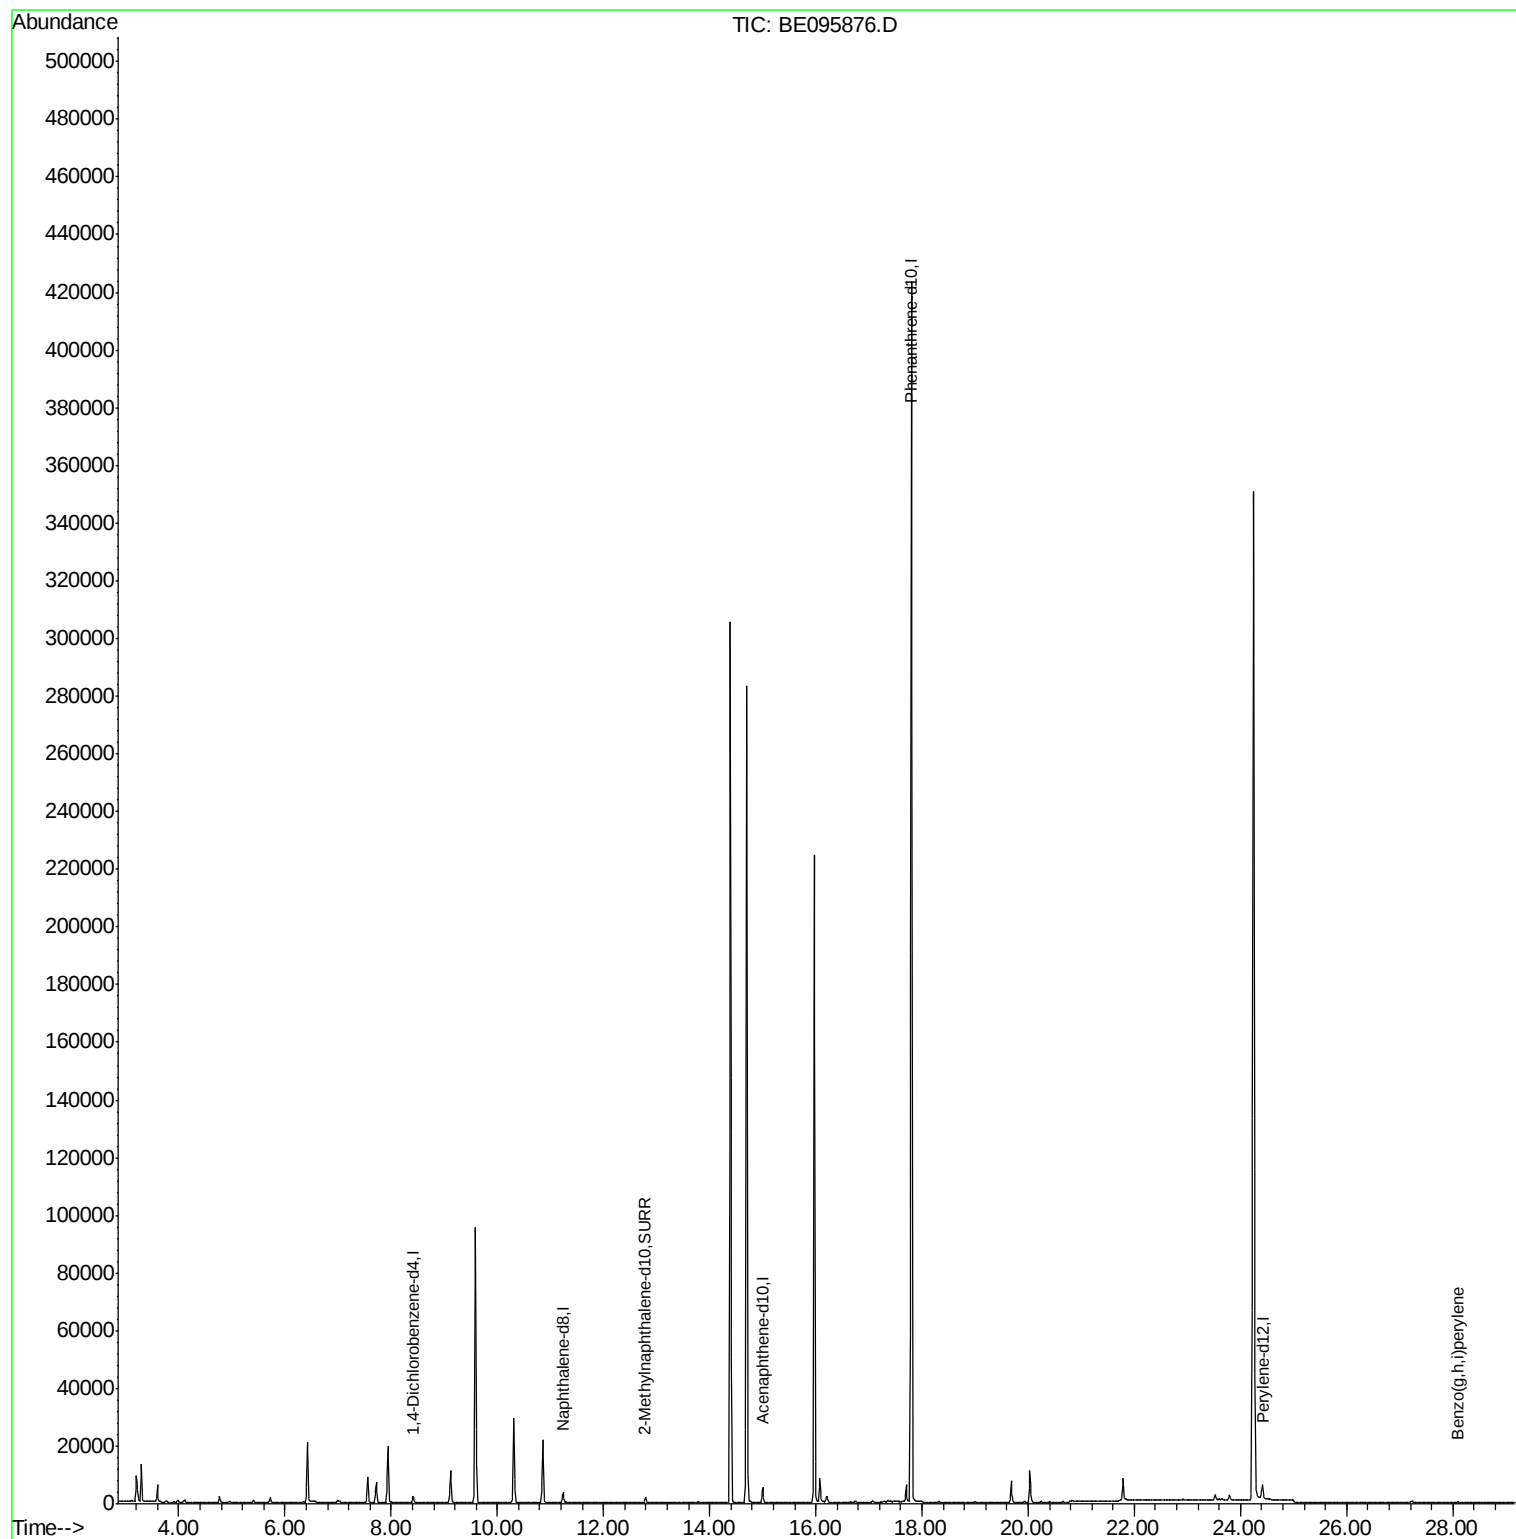

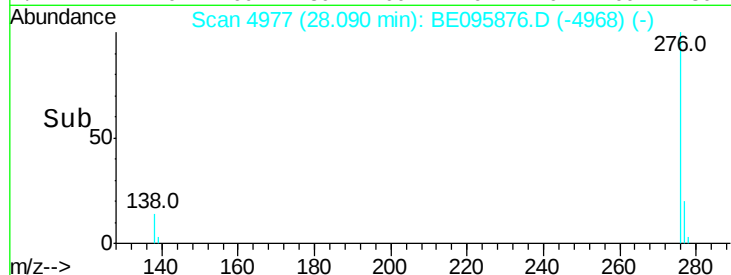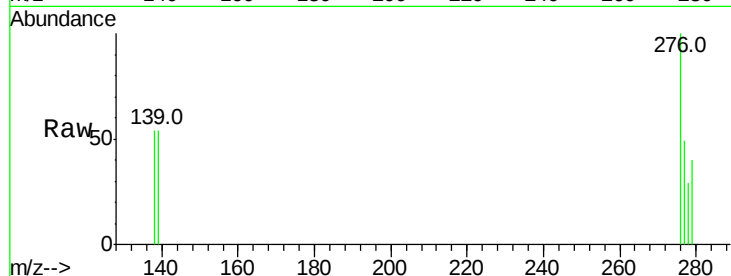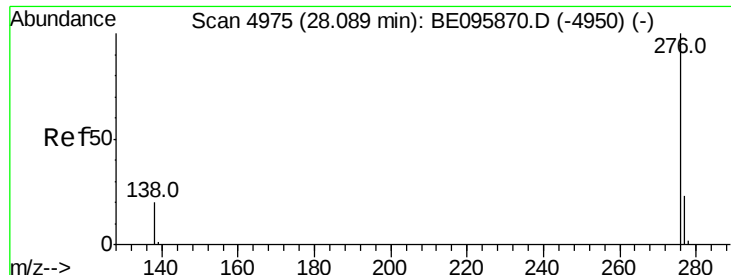

#26

Benzo(a,h,i)perylene

Concen: 0.021 ng/ul

RT: 28.09 min Scan# 4977

Delta R.T. -0.17 min

Lab File: BE095876.D

Acq: 28 Mar 2018 14:46

Instrument :

BNA_E

ClientSampleId :

Tot Ion:276 Resp: 559

Ion Ratio Lower Upper

276 100

138 54.2 21.8 32.8#

277 48.6 20.5 30.7#

