

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
 Data File : BE095886.D
 Acq On : 28 Mar 2018 20:42
 Operator : SJ/JU
 Sample : J1951-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Mar 29 04:44:03 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 29 04:43:20 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.41	152	1677	0.40	ng/ul	0.00
2) Naphthalene-d8	11.23	136	4581	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.99	164	2963	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.80	188	279788	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.79
20) Perylene-d12	24.41	264	7916	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.79	152	1532	0.20	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds				Ovalue		
3) Naphthalene	11.29	128	1163	0.091	ng/ul#	81
5) 2-Methylnaphthalene	12.87	142	354	0.040	ng/ul	97
8) Acenaphthene	15.06	153	1039	0.092	ng/ul	93
9) Fluorene	16.02	166	765	0.063	ng/ul	91
21) Benzo(b)fluoranthene	23.60	252	26642	0.972	ng/ul	86
22) Benzo(k)fluoranthene	23.60	252	26642	1.022	ng/ul#	88
23) Benzo(a)pyrene	24.29	252	15244	0.609	ng/ul#	81
24) Indeno(1,2,3-cd)pyrene	27.21	276	9157	0.330	ng/ul#	75
25) Dibenzo(a,h)anthracene	27.22	278	2474	0.111	ng/ul#	96
26) Benzo(g,h,i)perylene	28.09	276	8351	0.350	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095886.D
Acq On : 28 Mar 2018 20:42
Operator : SJ/JU
Sample : J1951-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Mar 29 04:44:03 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 04:43:20 2018
Response via : Initial Calibration

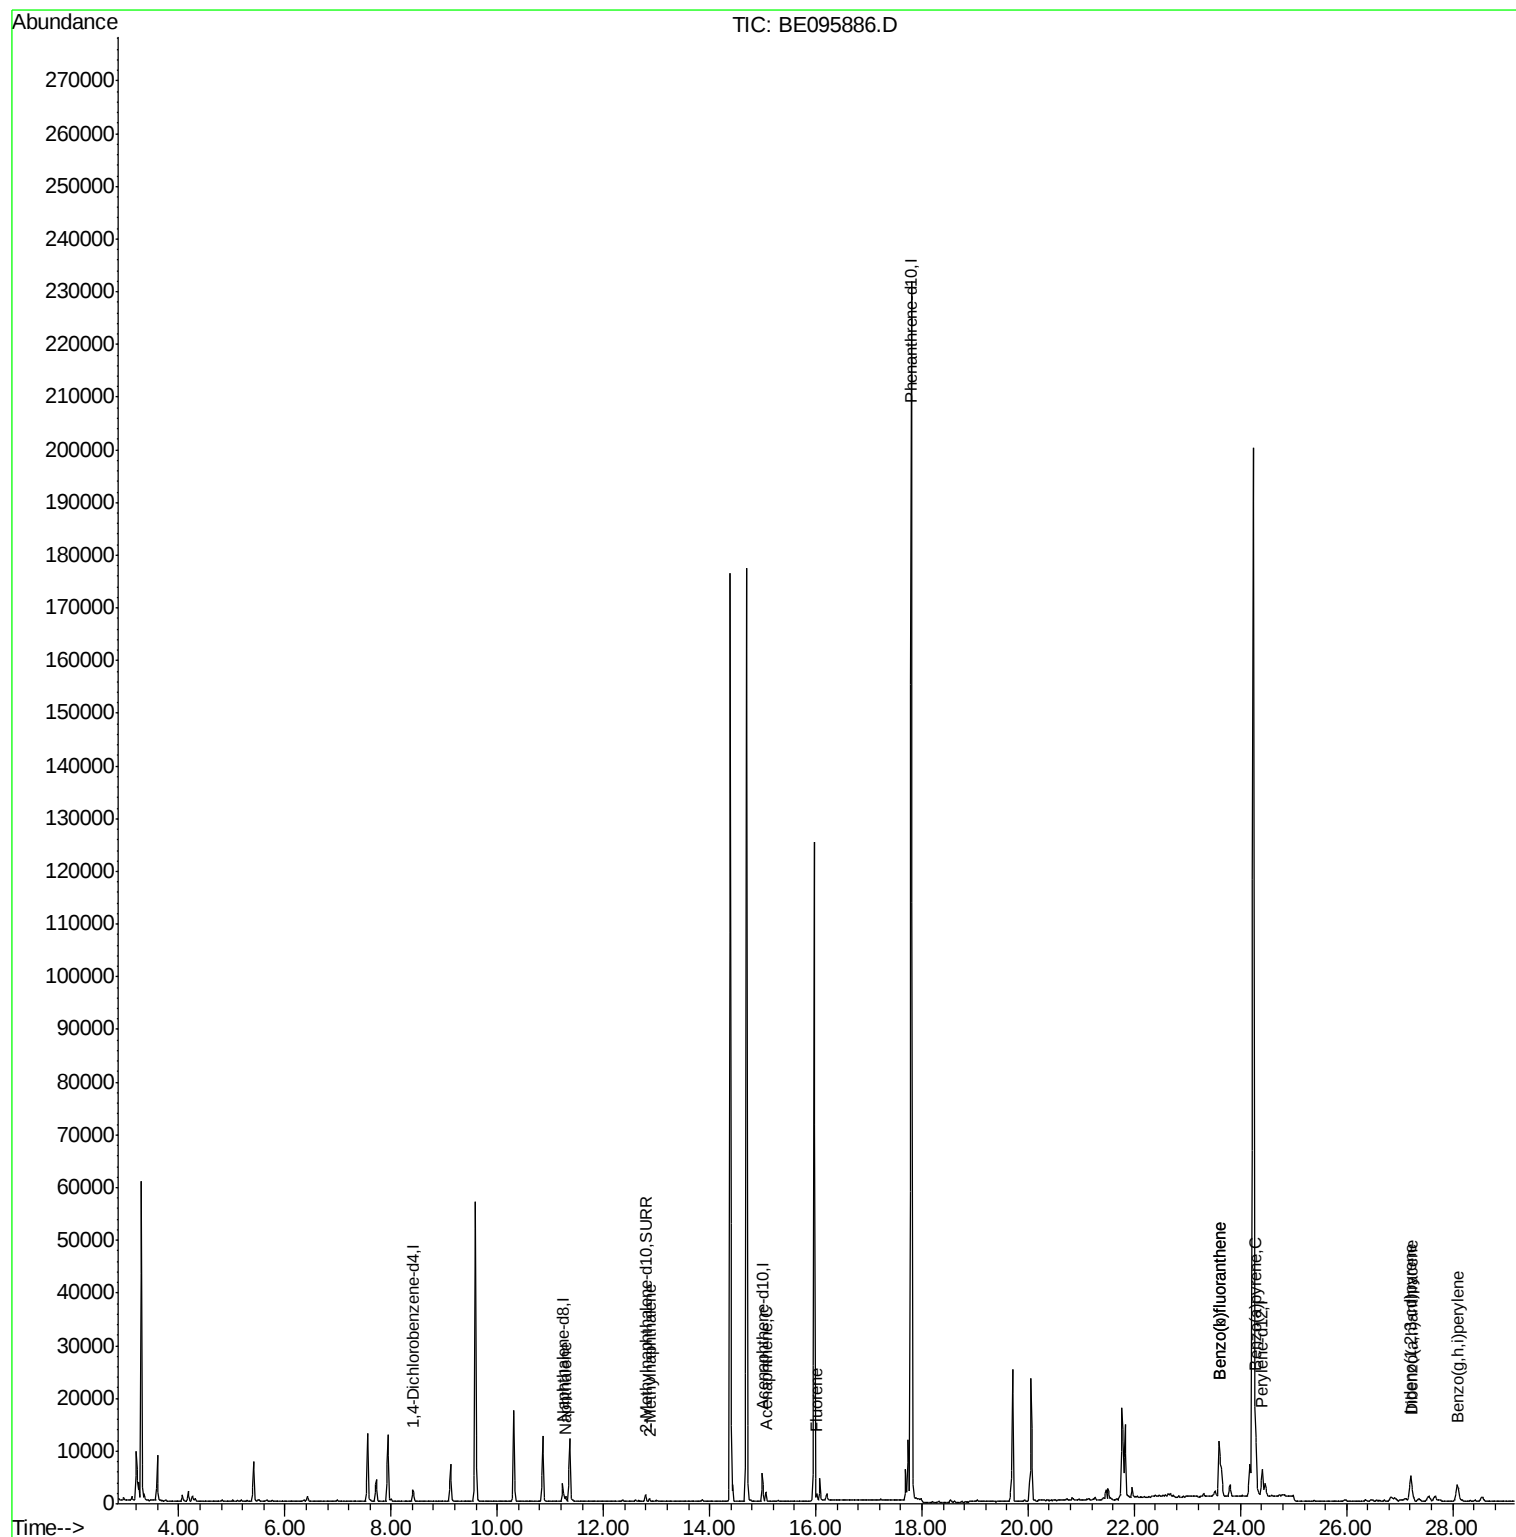

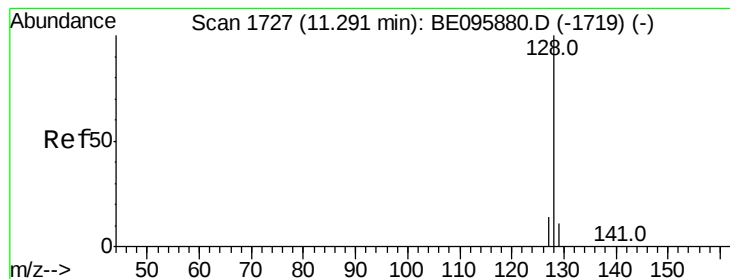

#3

Naphthalene

Concen: 0.091 ng/ul

RT: 11.29 min Scan# 1727

Delta R.T. -0.01 min

Lab File: BE095886.D

Acq: 28 Mar 2018 20:42

Instrument :

BNA_E

ClientSampled :


Tot Ion:128 Resp: 1163

Ion Ratio Lower Upper

128 100

129 18.3 11.3 16.9#




127 19.1 4.0 6.0#

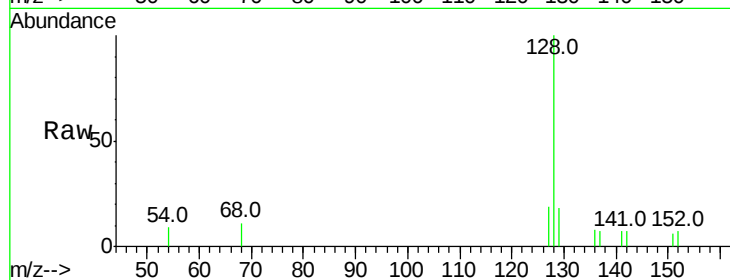

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

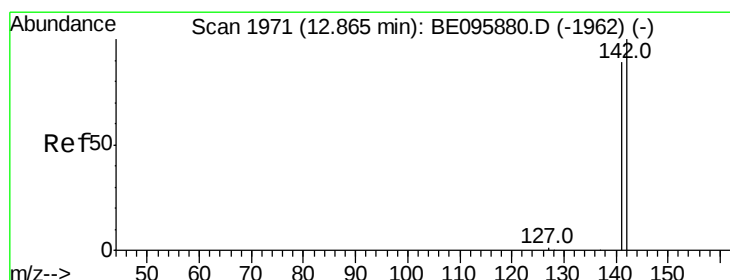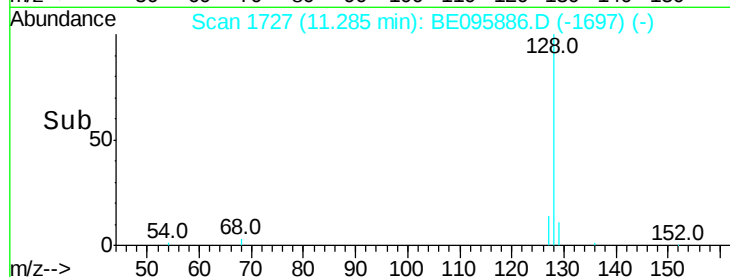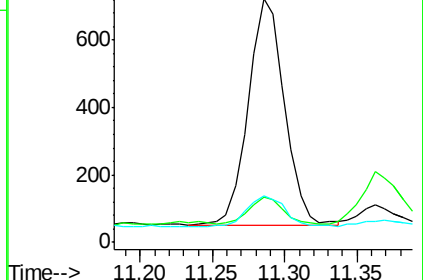

#5

2-Methylnaphthalene

Concen: 0.040 ng/ul

RT: 12.87 min Scan# 1972

Delta R.T. 0.00 min

Lab File: BE095886.D


Acq: 28 Mar 2018 20:42

Tgt Ion:142 Resp: 354

Ion Ratio Lower Upper



142 100


141 93.5 72.6 108.8

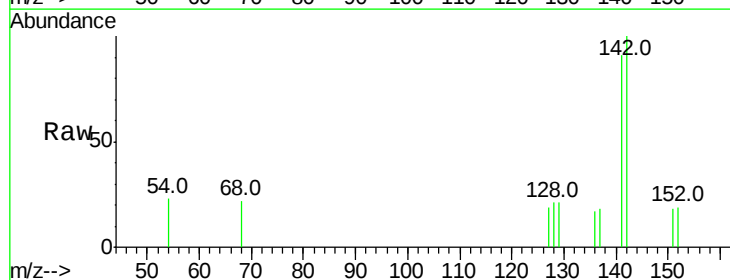

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

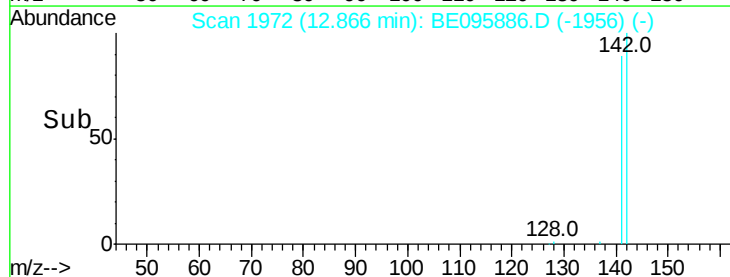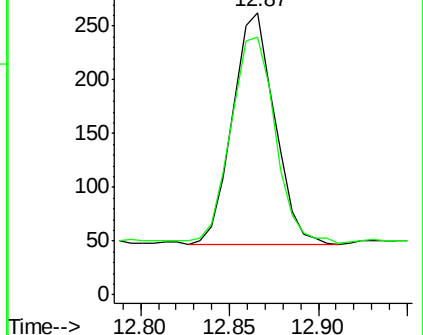

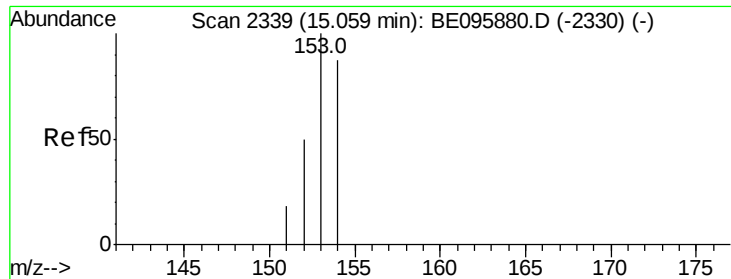

#8

Acenaphthene

Concen: 0.092 ng/ul

RT: 15.06 min Scan# 2339

Delta R.T. -0.00 min

Lab File: BE095886.D

Acq: 28 Mar 2018 20:42

Instrument :

BNA_E

ClientSampleId :


Tot Ion:153 Resp: 1039

Ion Ratio Lower Upper

153 100

152 53.1 36.0 54.0




154 85.4 72.0 108.0

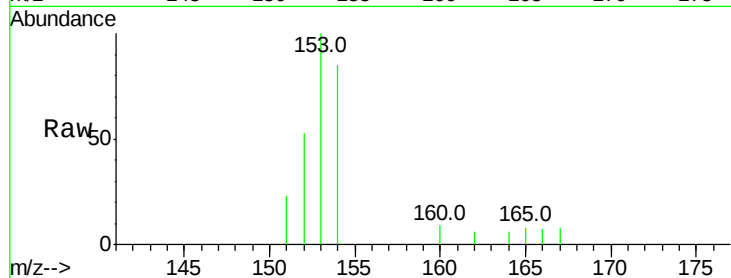

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

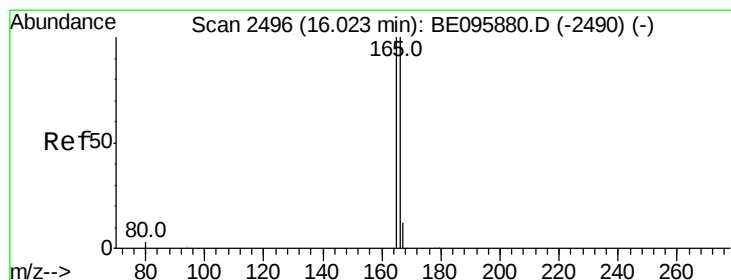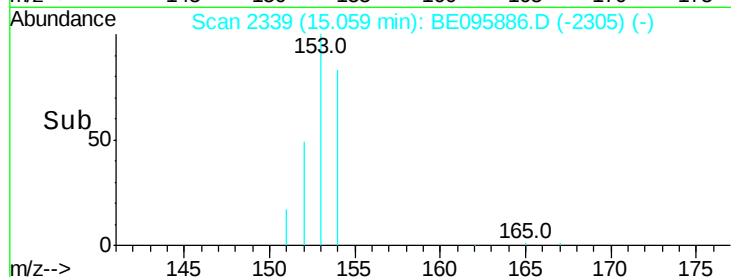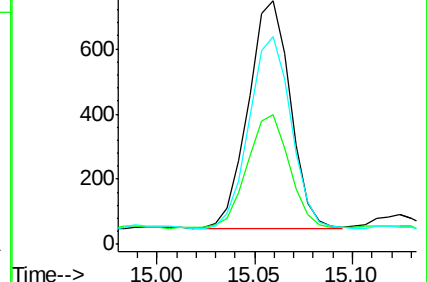

#9

Fluorene

Concen: 0.063 ng/ul

RT: 16.02 min Scan# 2496

Delta R.T. -0.00 min

Lab File: BE095886.D

Acq: 28 Mar 2018 20:42


Tgt Ion:166 Resp: 765

Ion Ratio Lower Upper

166 100

165 101.3 73.4 110.2



167 19.9 14.6 22.0

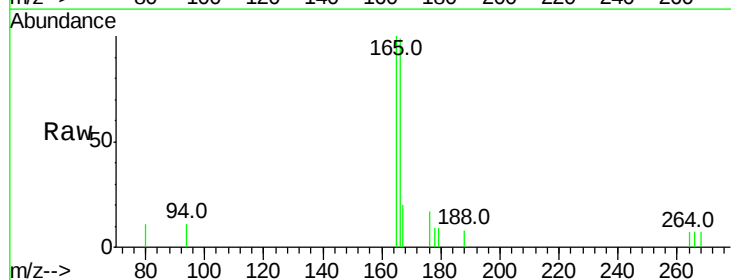


Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

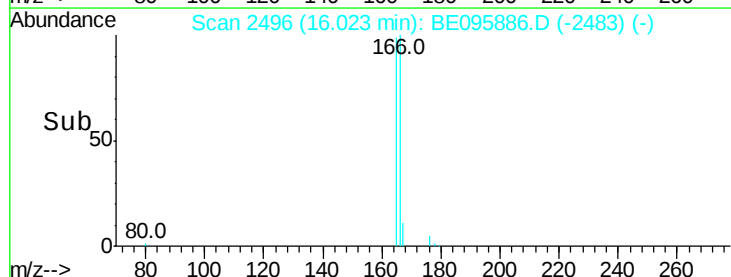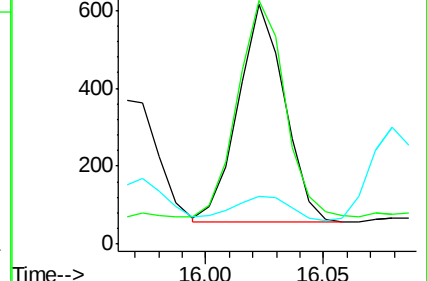

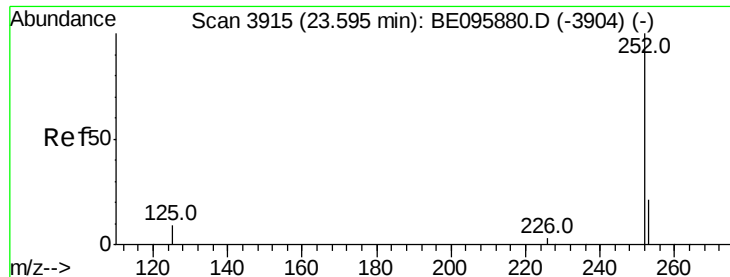

#21

Benzo(b)fluoranthene

Concen: 0.972 ng/ul

RT: 23.60 min Scan# 3916

Delta R.T. 0.01 min

Lab File: BE095886.D

Acq: 28 Mar 2018 20:42

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 26642

Ion Ratio Lower Upper

252 100

253 24.0 0.0 64.2




125 11.8 0.0 35.0

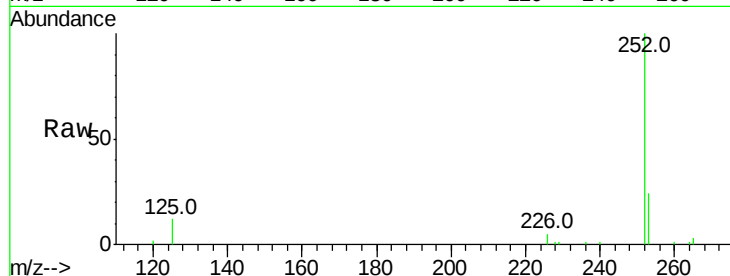

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

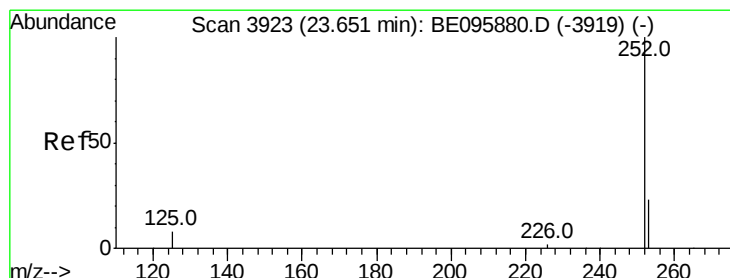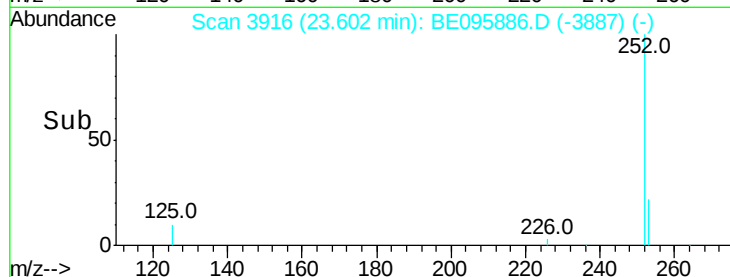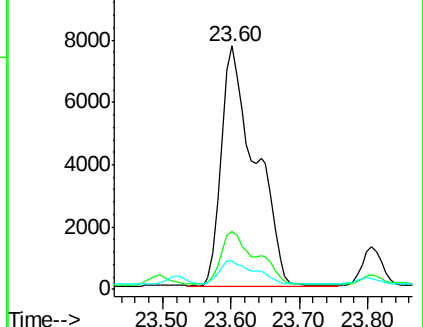

#22

Benzo(k)fluoranthene

Concen: 1.022 ng/ul

RT: 23.60 min Scan# 3916

Delta R.T. -0.05 min

Lab File: BE095886.D

Acq: 28 Mar 2018 20:42


Tgt Ion:252 Resp: 26642

Ion Ratio Lower Upper

252 100

253 24.0 24.5 36.7#



125 11.8 13.7 20.5#

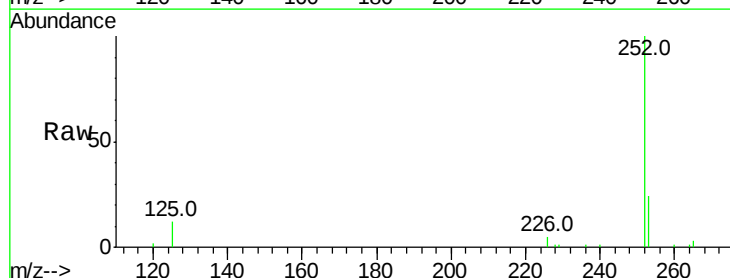


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

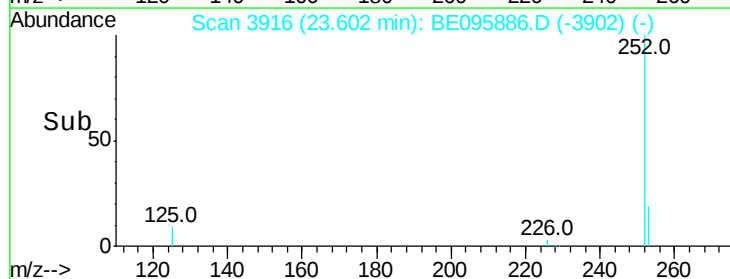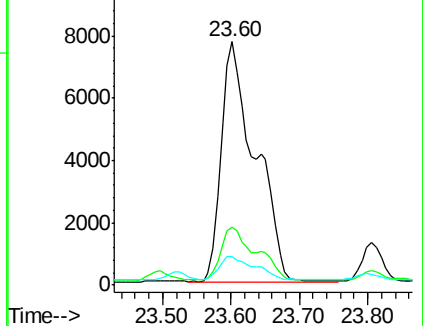

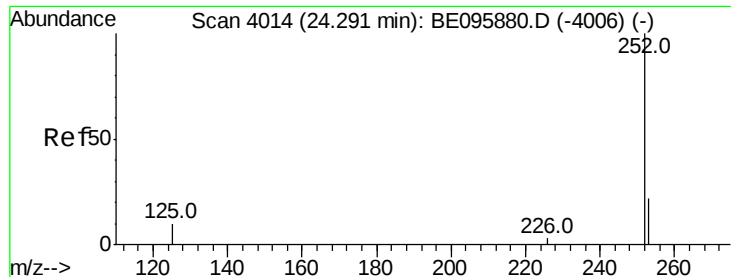

#23

Benzo(a)pyrene

Concen: 0.609 ng/ul

RT: 24.29 min Scan# 4014

Delta R.T. -0.00 min

Lab File: BE095886.D

Acq: 28 Mar 2018 20:42

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 15244

Ion Ratio Lower Upper

252 100

253 24.7 28.5 42.7#




125 13.1 18.1 27.1#

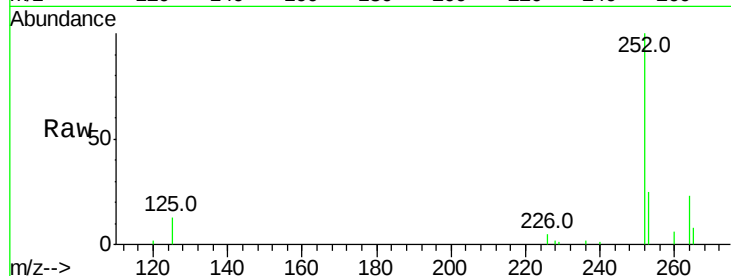

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

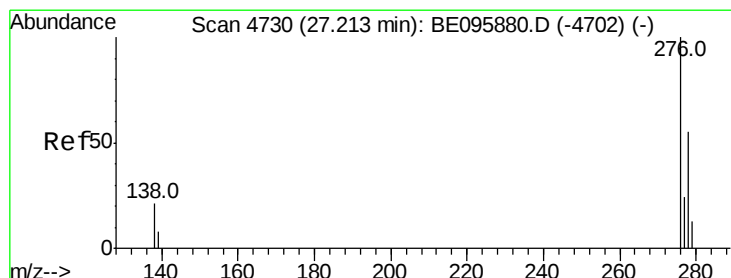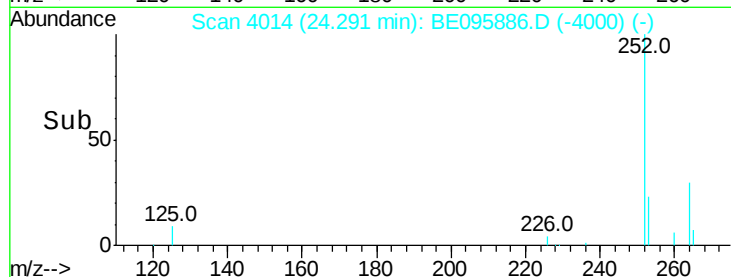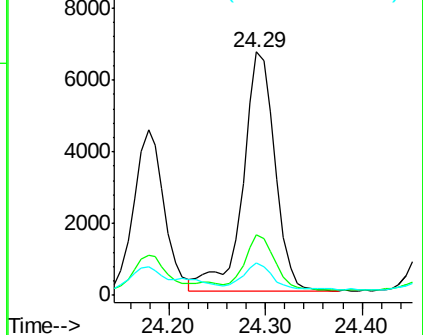

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.330 ng/ul

RT: 27.21 min Scan# 4730

Delta R.T. -0.00 min

Lab File: BE095886.D

Acq: 28 Mar 2018 20:42


Tgt Ion:276 Resp: 9157

Ion Ratio Lower Upper

276 100

138 20.5 28.0 42.0#



227 0.0 8.0 12.0#

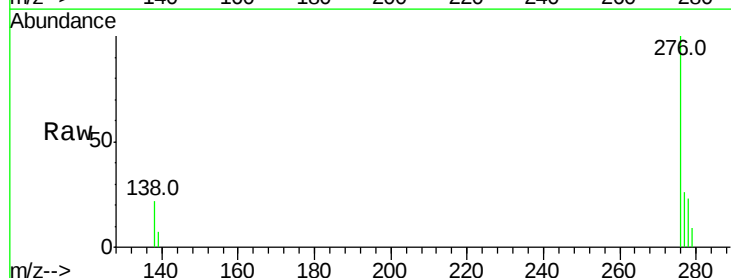


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

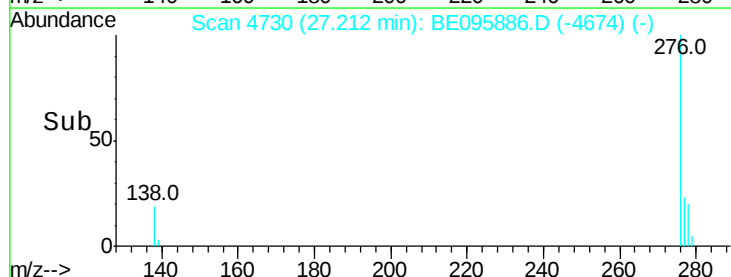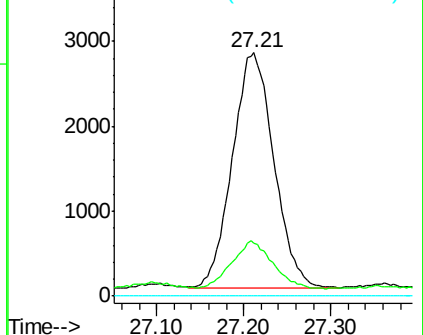

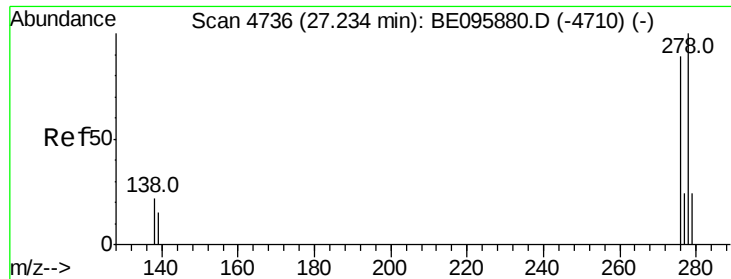

#25

Dibenzo(a,h)anthracene

Concen: 0.111 ng/ul

RT: 27.22 min Scan# 4733

Delta R.T. -0.01 min

Lab File: BE095886.D

Acq: 28 Mar 2018 20:42

Instrument :

BNA_E

ClientSampleId :





Tot Ion:278 Resp: 2474

Ion Ratio Lower Upper

278 100

139 26.5 17.4 26.0#

279 32.4 25.9 38.9

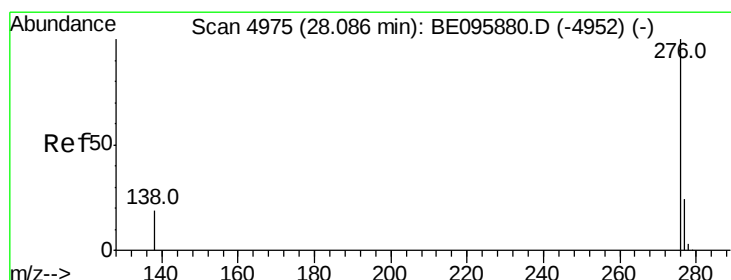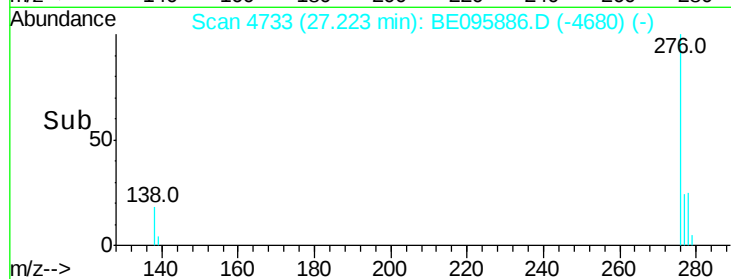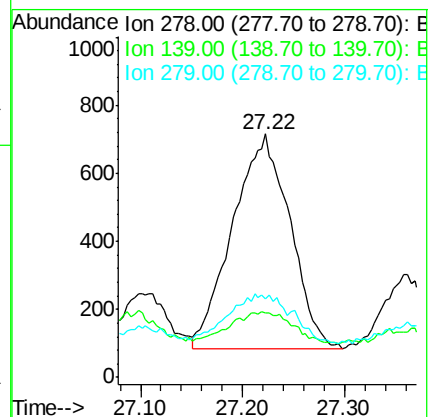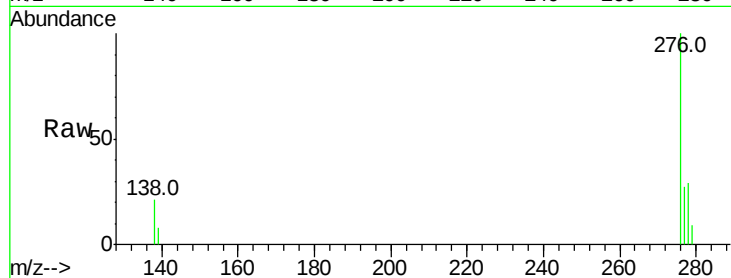

#26

Benzo(g,h,i)perylene

Concen: 0.350 ng/ul

RT: 28.09 min Scan# 4976

Delta R.T. 0.00 min

Lab File: BE095886.D

Acq: 28 Mar 2018 20:42

Tgt Ion:276 Resp: 8351

Ion Ratio Lower Upper

276 100

138 22.3 21.8 32.8

277 26.7 20.5 30.7

