

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
 Data File : BE095891.D
 Acq On : 28 Mar 2018 23:41
 Operator : SJ/JU
 Sample : J2059-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Mar 29 04:44:38 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 29 04:43:20 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.41	152	1704	0.40	ng/ul	0.00
2) Naphthalene-d8	11.24	136	5264	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.00	164	3322	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.80	188	676263	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.79
20) Perylene-d12	24.25	264	539109	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.79	152	3443	0.39	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
8) Acenaphthene	15.05	153	662	0.052	ng/ul#	30
9) Fluorene	15.97	166	1097	0.080	ng/ul#	21


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095891.D
Acq On : 28 Mar 2018 23:41
Operator : SJ/JU
Sample : J2059-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Mar 29 04:44:38 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 04:43:20 2018
Response via : Initial Calibration

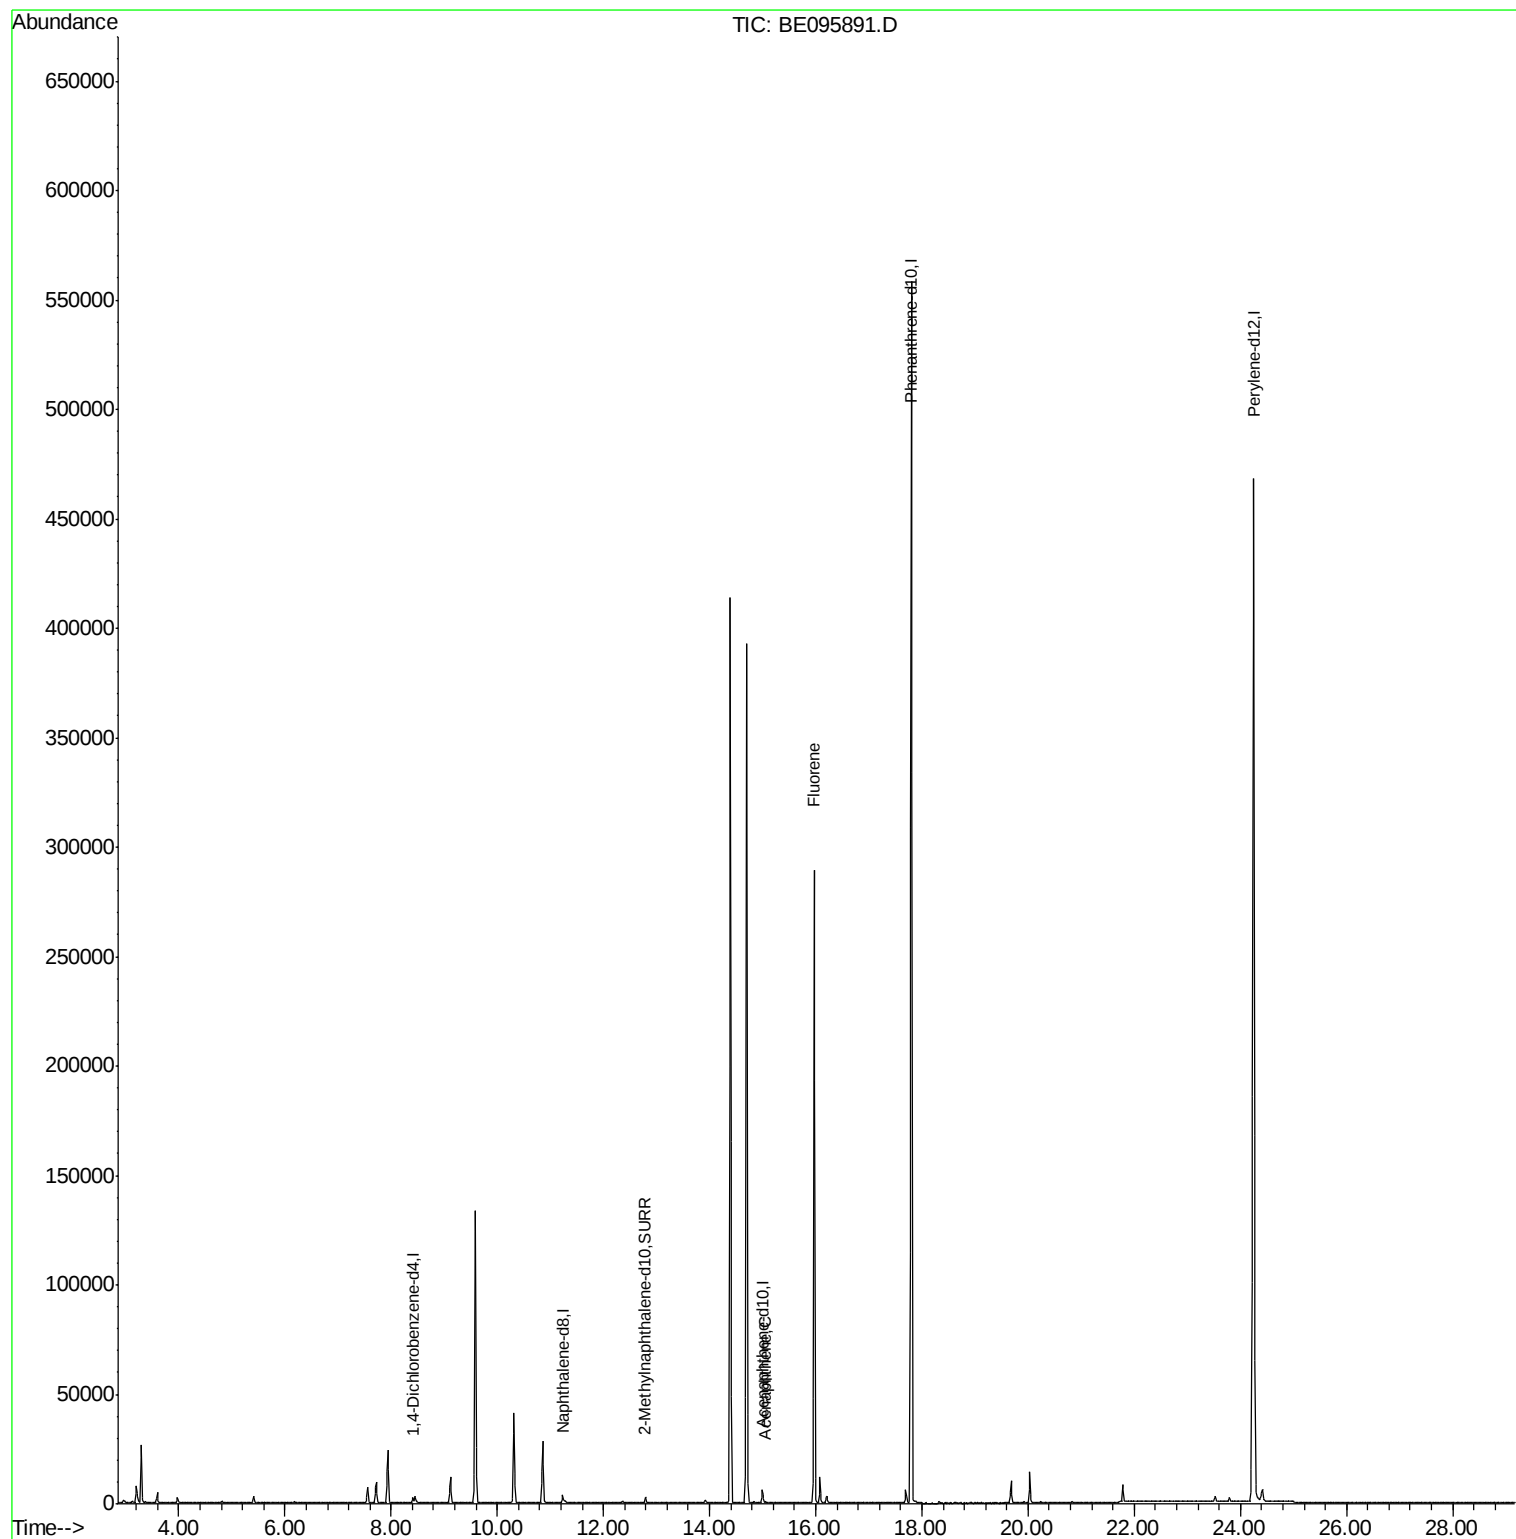

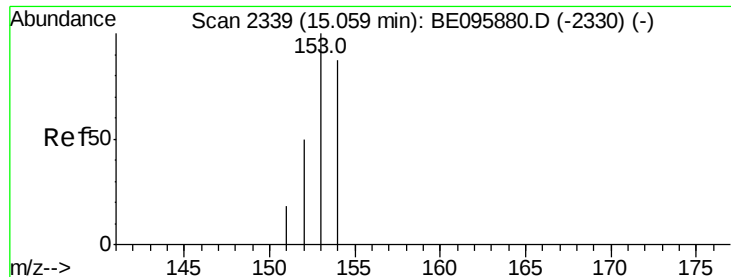

#8

Acenaphthene

Concen: 0.052 ng/ul

RT: 15.05 min Scan# 2337

Delta R.T. -0.01 min

Lab File: BE095891.D

Acq: 28 Mar 2018 23:41

Instrument :

BNA_E

ClientSampleId :


Tot Ion:153 Resp: 662

Ion Ratio Lower Upper

153 100

152 10.4 36.0 54.0#




154 16.4 72.0 108.0#

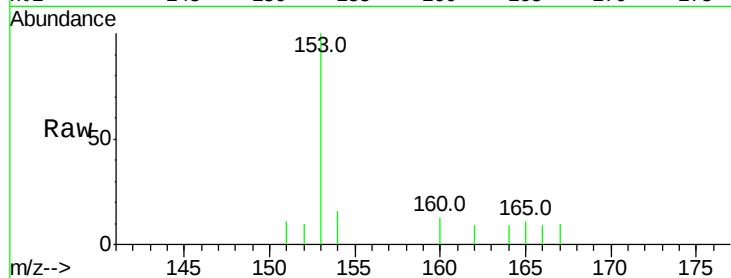

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

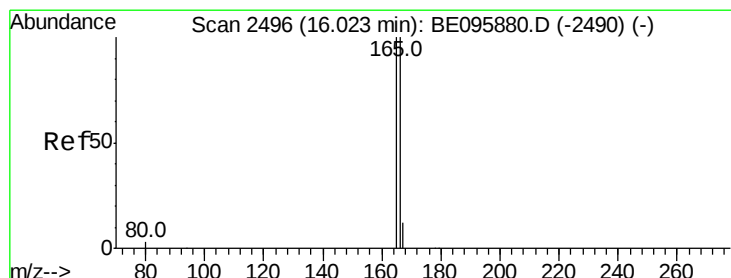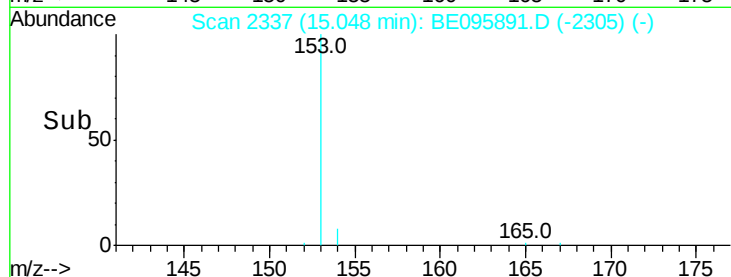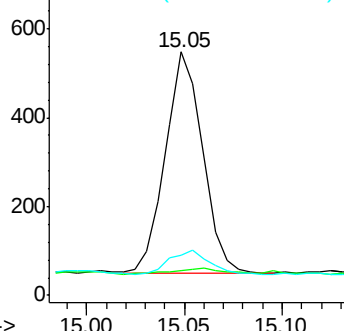

#9

Fluorene

Concen: 0.080 ng/ul

RT: 15.97 min Scan# 2489

Delta R.T. -0.05 min

Lab File: BE095891.D

Acq: 28 Mar 2018 23:41


Tgt Ion:166 Resp: 1097

Ion Ratio Lower Upper

166 100

165 11.1 73.4 110.2#

167 41.5 14.6 22.0#

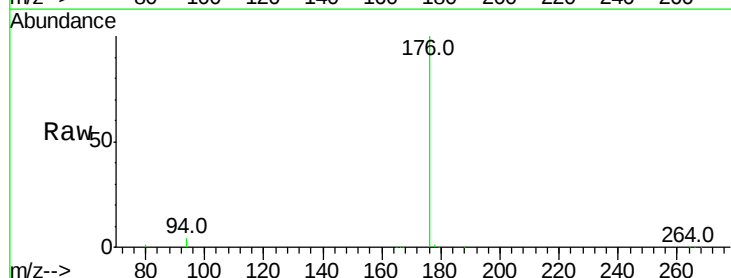

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

