

Data Path : Z:\HPCHEM1\BNA E\Data\BE032818\
Data File : BE095884.D
Acq On : 28 Mar 2018 19:30
Operator : SJ/JU
Sample : PB107777BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Mar 29 05:19:01 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 04:43:20 2018
Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :


SBLK77

Manual Integrations

APPROVED

Sohil

3/29/2018 5:47:07 PM

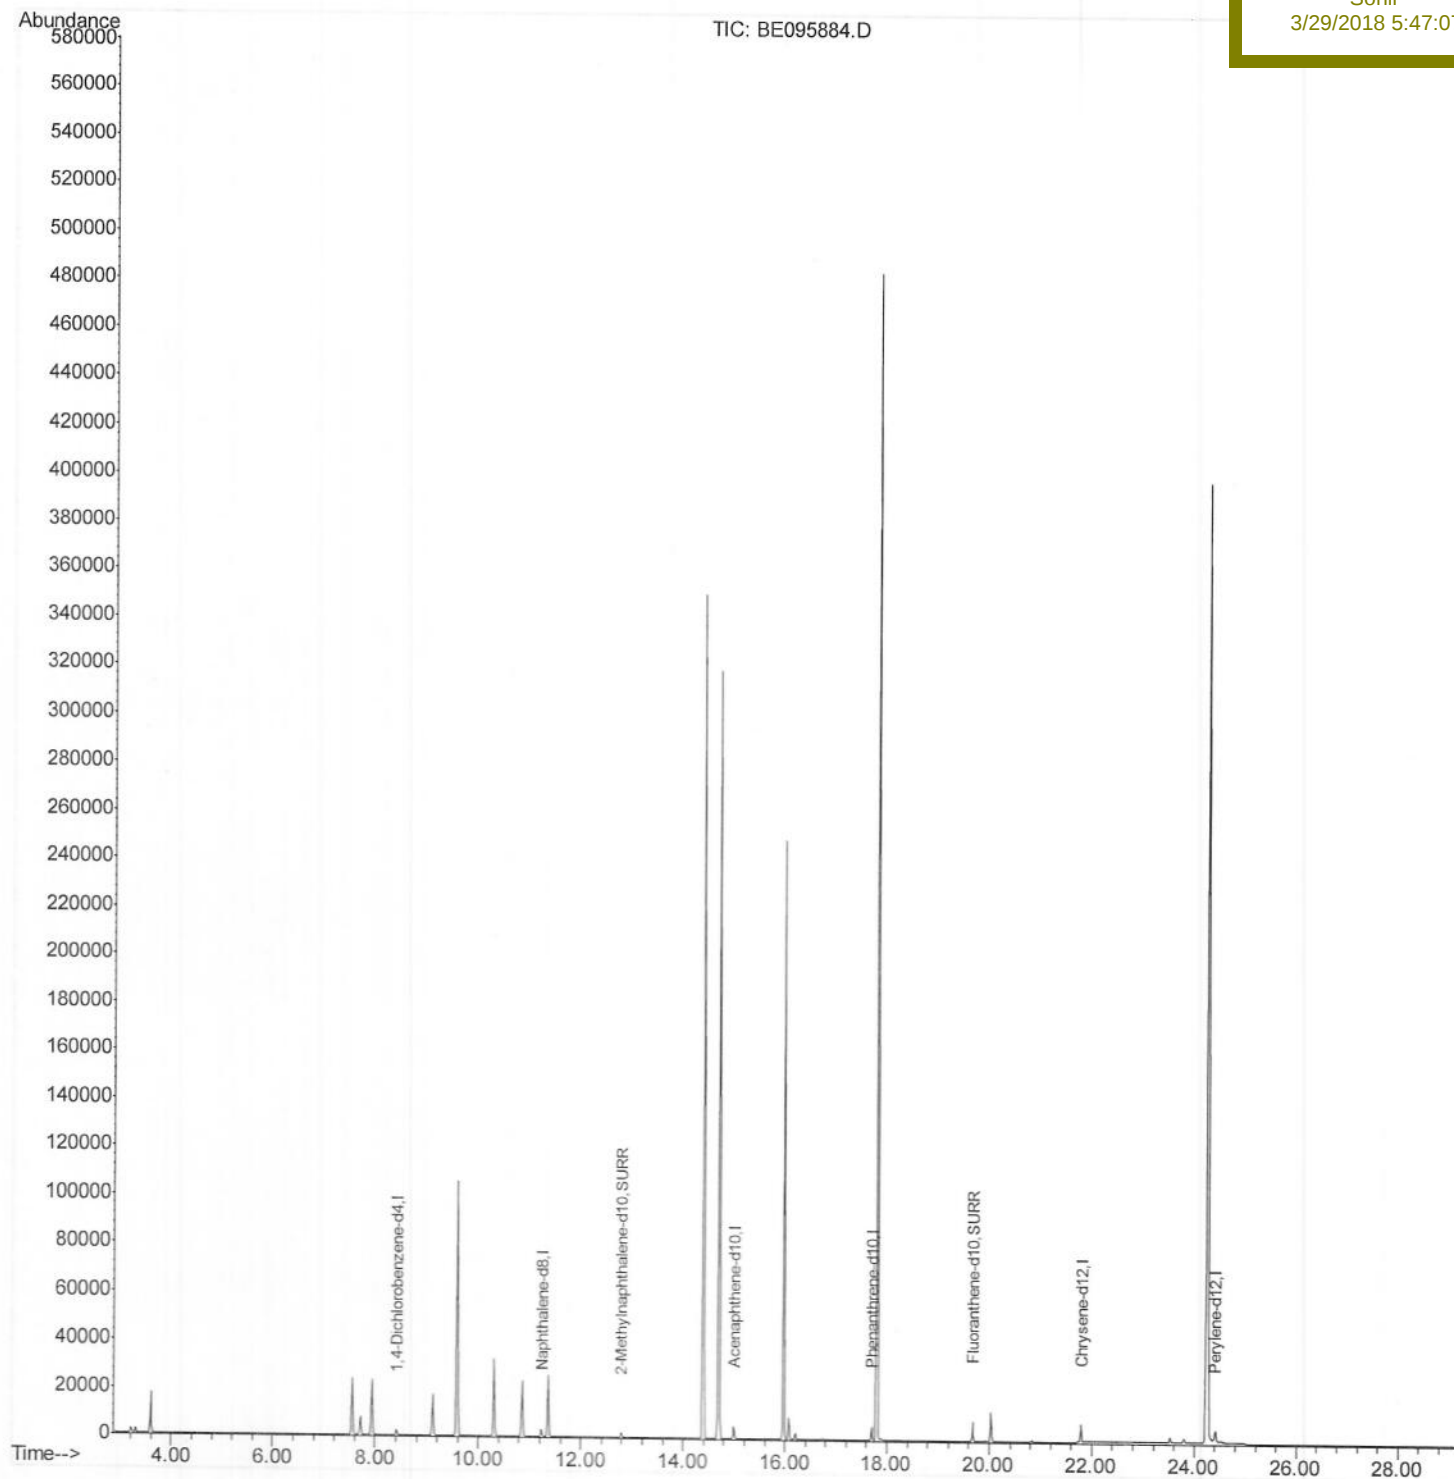


Data Path : Z:\HPCHEM1\BNA E\Data\BE032818\
Data File : BE095884.D
Acq On : 28 Mar 2018 19:30
Operator : SJ/JU
Sample : PB107777BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Apr 02 02:33:07 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 16:32:29 2018
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
SBLK77

Manual Integrations
APPROVED

Sohil
3/29/2018 5:47:07 PM

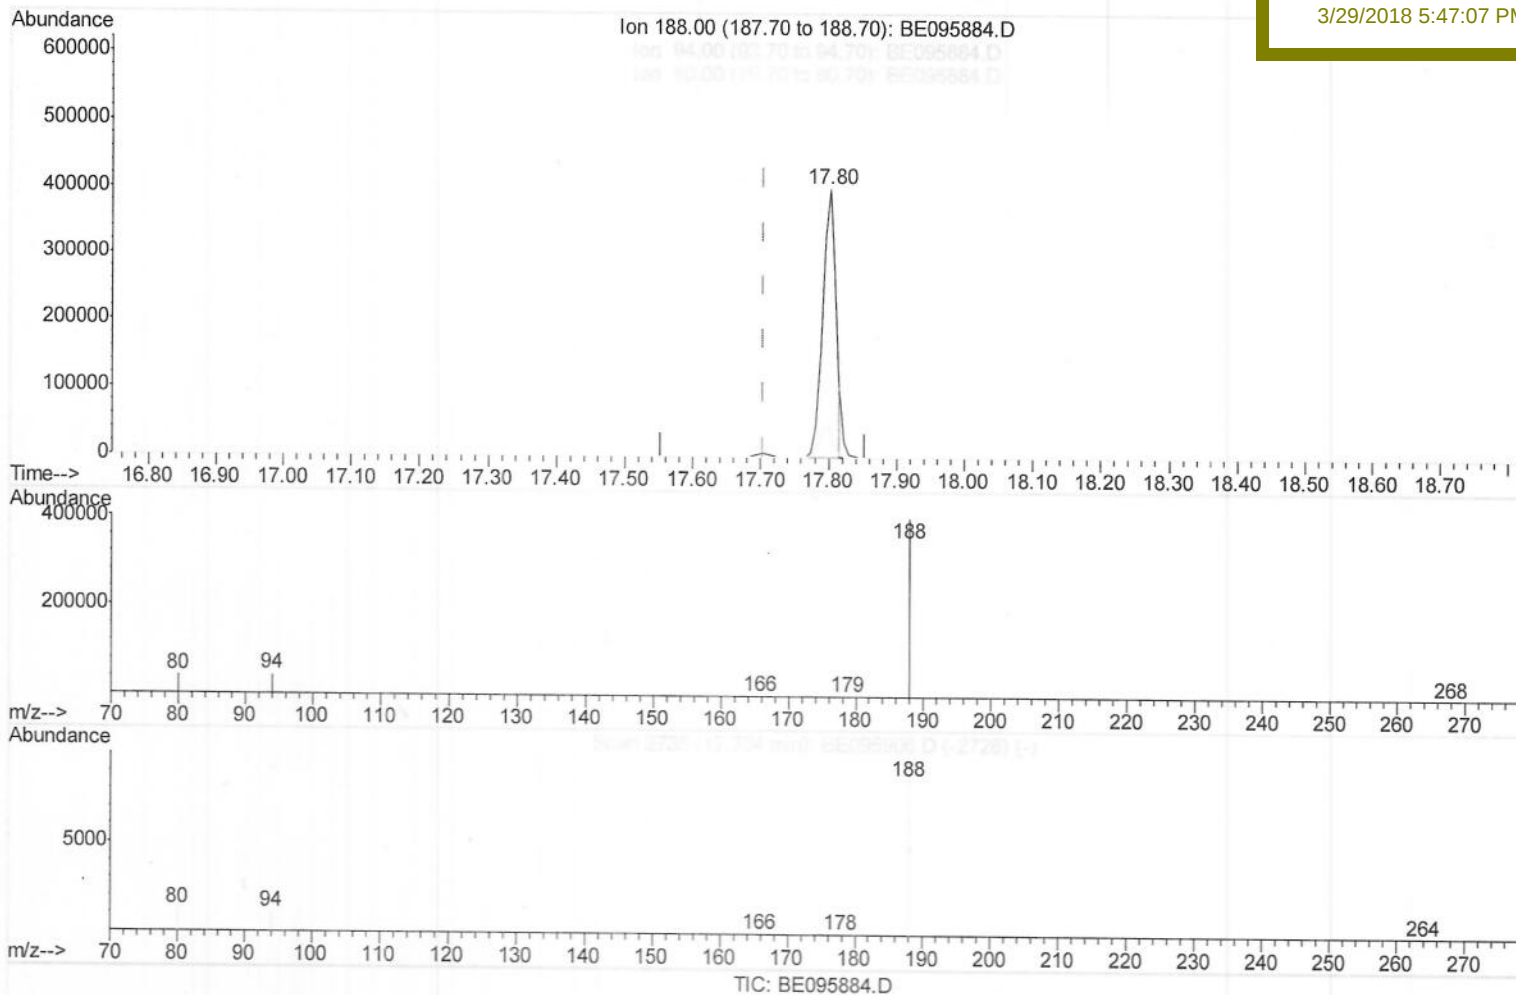

(10) Phenanthrene-d10 (I)

17.802min (+0.098) 0.40ng/ul

response 557128

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.48
80.00	11.80	10.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE032818\
Data File : BE095884.D
Acq On : 28 Mar 2018 19:30
Operator : SJ/JU
Sample : PB107777BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Mar 29 05:19:01 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 04:43:20 2018
Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :




SBLK77

Manual Integrations

APPROVED

Sohil

3/29/2018 5:47:07 PM

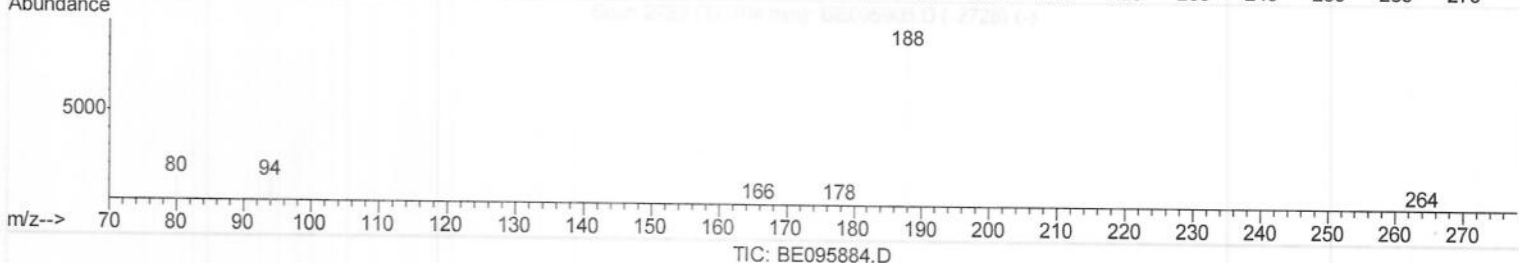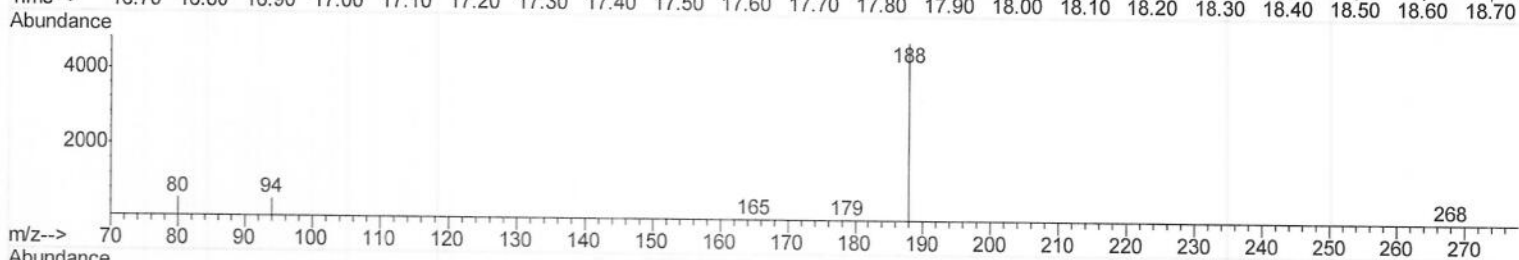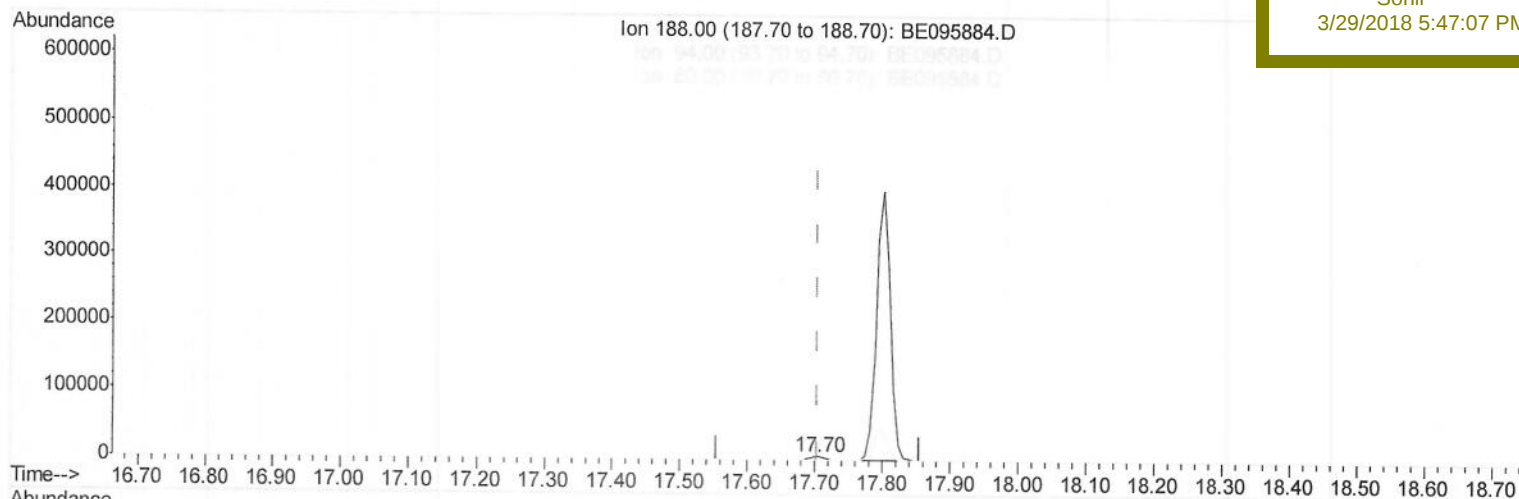

(10) Phenanthrene-d10 (I)

17.703min (-0.001) 0.40ng/ul m) JU 3130118

response 6962

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.46
80.00	11.80	10.81
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE032818\

Data File : BE095884.D

Acq On : 28 Mar 2018 19:30

Operator : SJ/JU

Sample : PB107777BL

Misc :

ALS Vial : 15 Sample Multiplier: 1

Quant Time: Apr 02 02:33:07 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Mar 29 16:32:29 2018

Response via : Initial Calibration

Instrument :

BNA_E




ClientSampleId :

SBLK77

Manual Integrations
APPROVED

Sohil

3/29/2018 5:47:07 PM

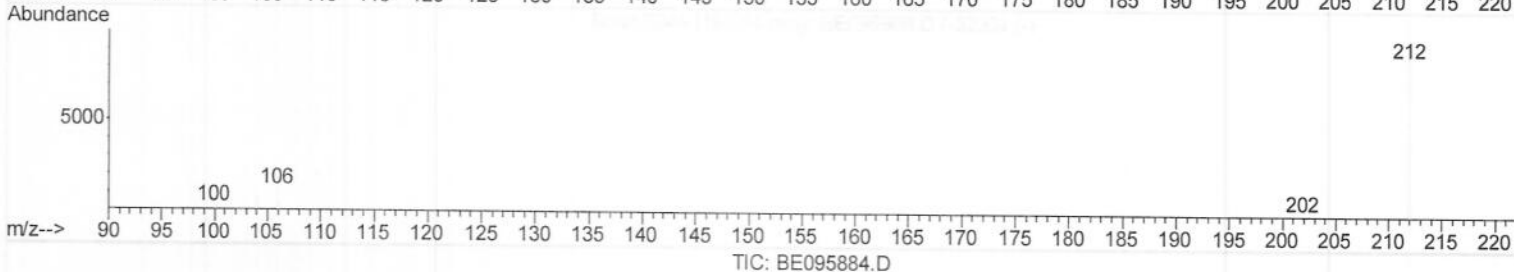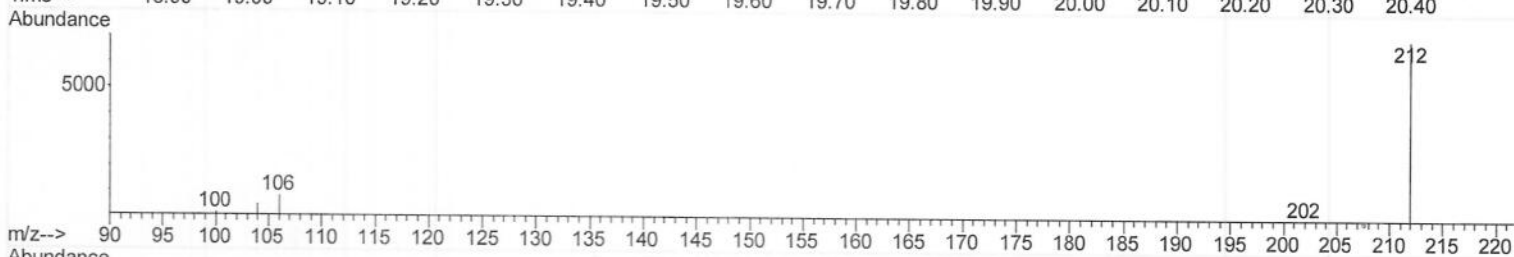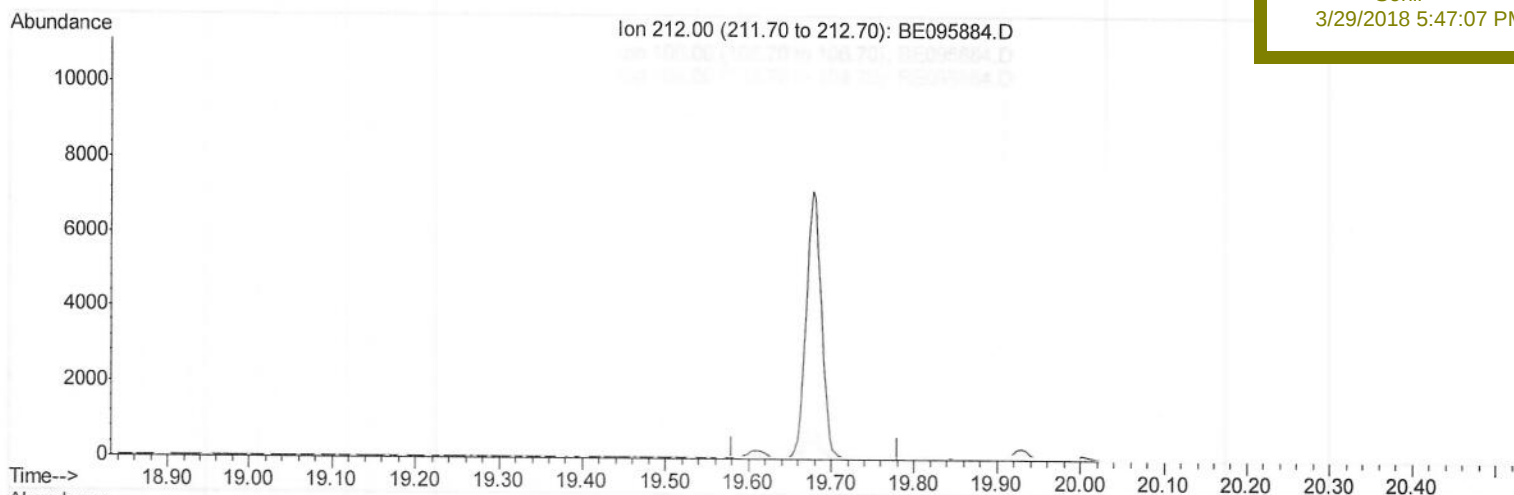

(14) Fluoranthene-d10 (SURR)

19.681min (-19.681) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE032818\

Data File : BE095884.D

Acq On : 28 Mar 2018 19:30

Operator : SJ/JU

Sample : PB107777BL

Misc :

ALS Vial : 15 Sample Multiplier: 1

Quant Time: Mar 29 05:19:01 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Mar 29 04:43:20 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :


SBLK77

Manual Integrations

APPROVED

Sohil

3/29/2018 5:47:07 PM

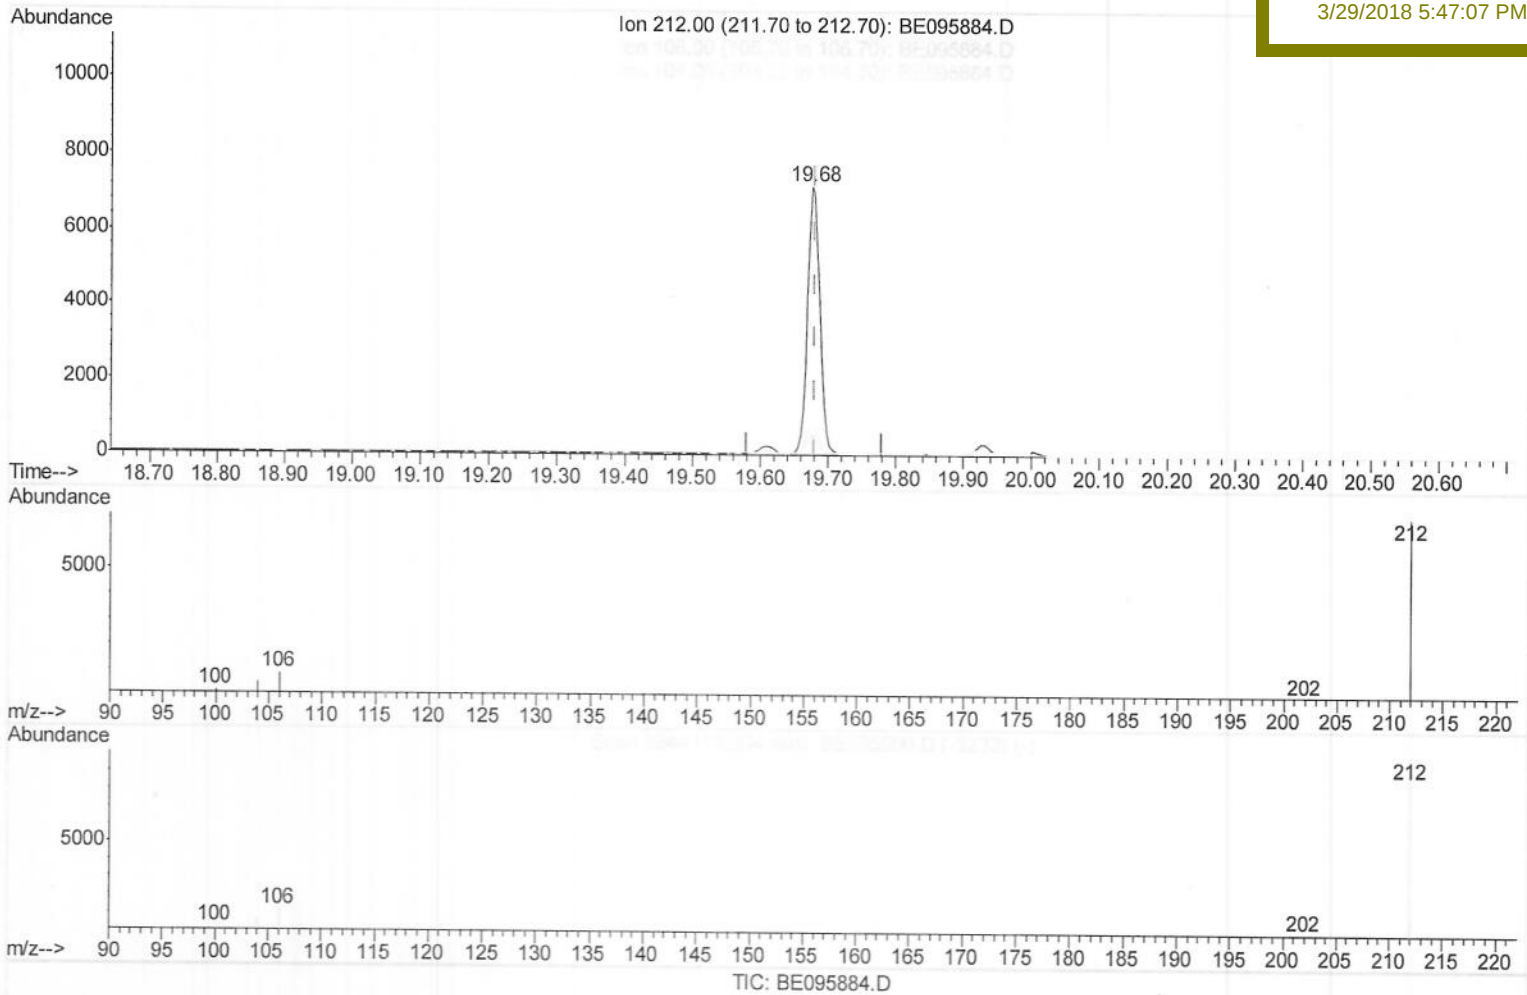

(14) Fluoranthene-d10 (SURR)

19.677min (-0.003) 0.41ng/ul m 503130118

response 9112

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE032818\

Data File : BE095884.D

Acq On : 28 Mar 2018 19:30

Operator : SJ/JU

Sample : PB107777BL

Misc :

ALS Vial : 15 Sample Multiplier: 1

Quant Time: Apr 02 02:33:07 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Mar 29 16:32:29 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :


SBLK77

Manual Integrations

APPROVED

Sohil

3/29/2018 5:47:07 PM

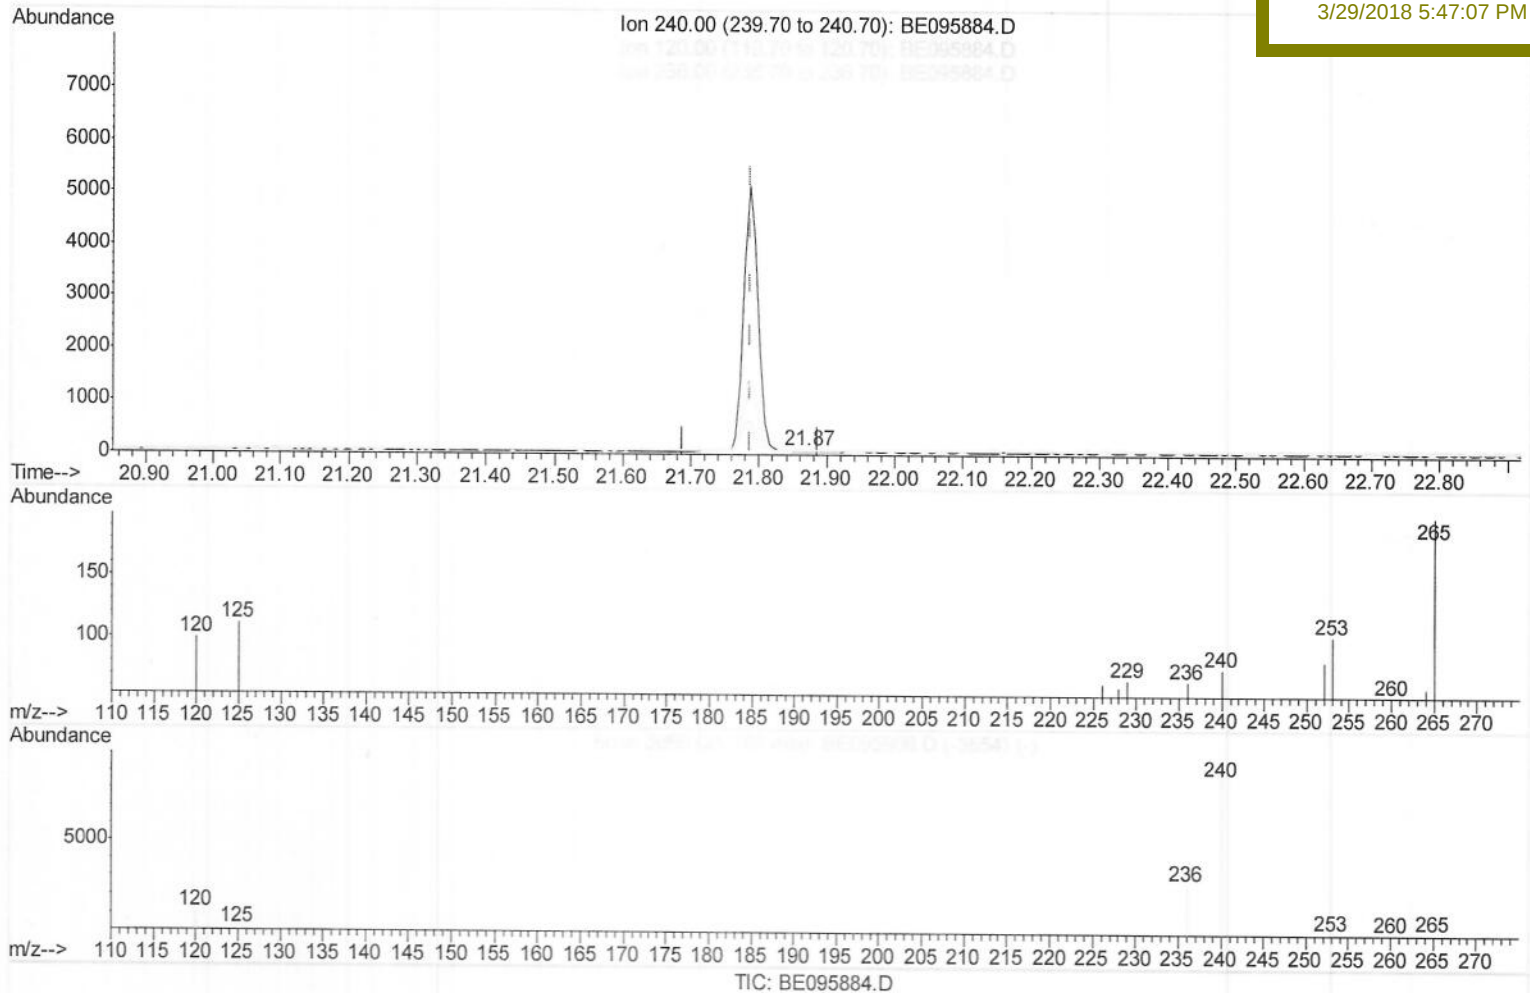

(16) Chrysene-d12 (I)

21.871min (+0.084) 0.40ng/ul

response 38

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	130.26#
236.00	34.90	86.84#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE032818\

Data File : BE095884.D

Acq On : 28 Mar 2018 19:30

Operator : SJ/JU

Sample : PB107777BL

Misc :

ALS Vial : 15 Sample Multiplier: 1

Quant Time: Mar 29 05:19:01 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Mar 29 04:43:20 2018




Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

SBLK77

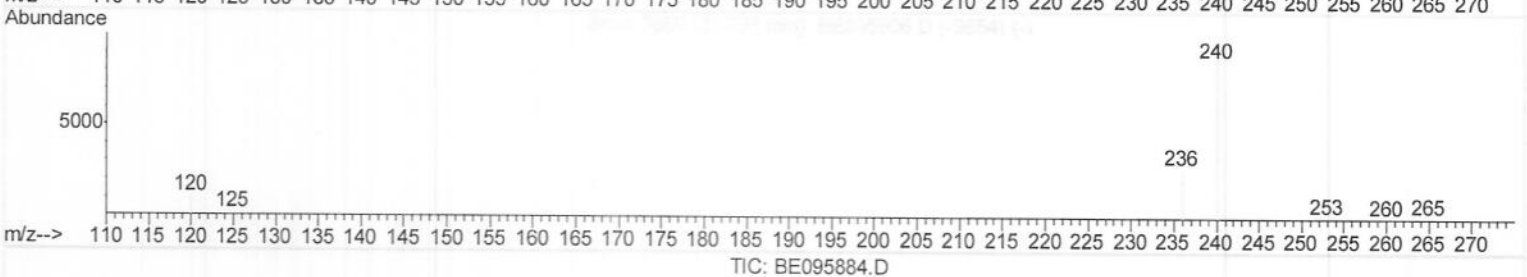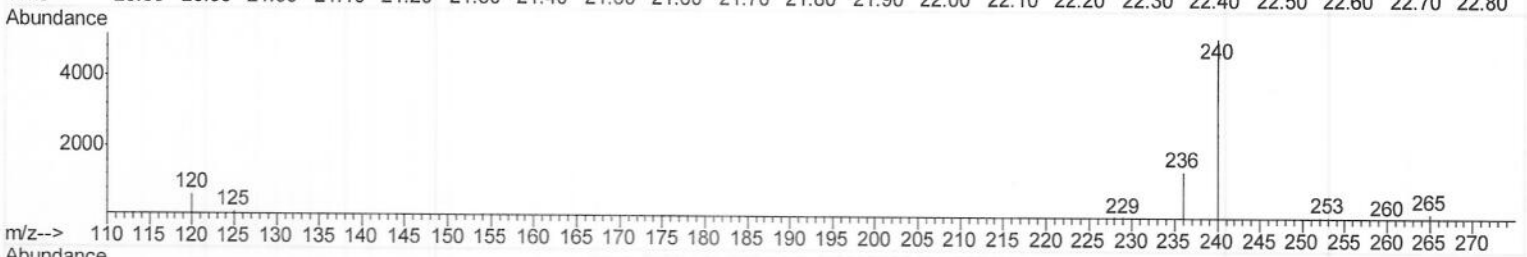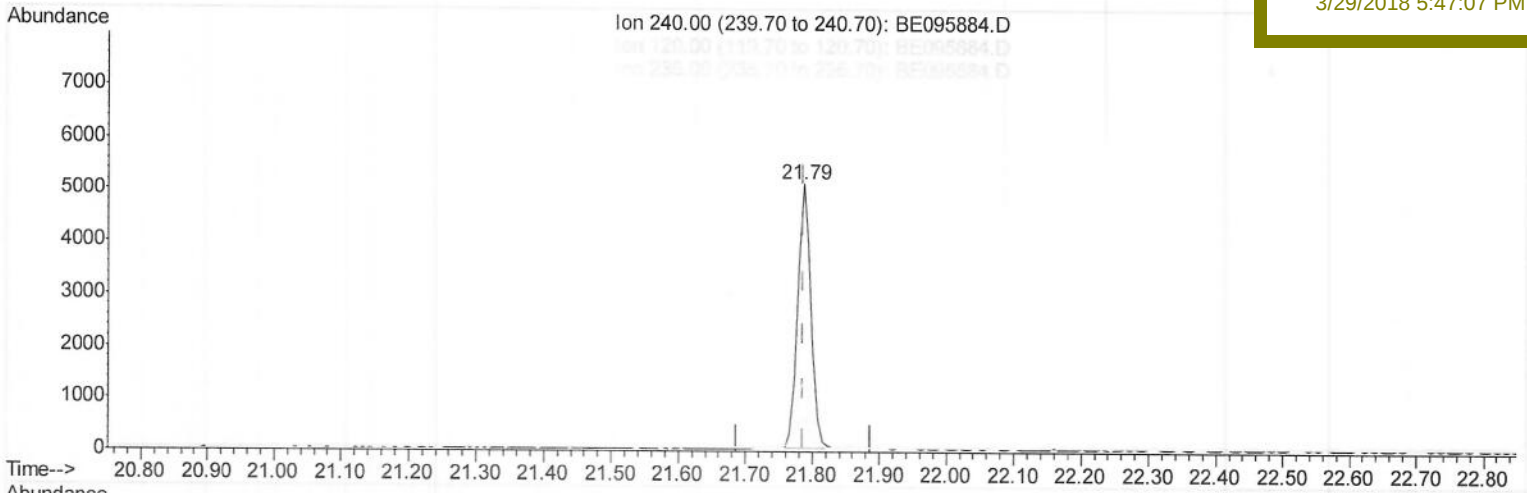Manual Integrations
APPROVEDSohil
3/29/2018 5:47:07 PM

(16) Chrysene-d12 (I)

21.787min (-0.001) 0.40ng/ul m) JU3/30/18

response 7169

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	12.08#
236.00	34.90	26.89#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE032818\
Data File : BE095884.D
Acq On : 28 Mar 2018 19:30
Operator : SJ/JU
Sample : PB107777BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Mar 29 05:19:01 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 04:43:20 2018
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
SBLK77

Manual Integrations
APPROVED

Sohil
3/29/2018 5:47:07 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.41	152	1615	0.40	ng/ul	0.00
2) Naphthalene-d8	11.24	136	4339	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.99	164	2871	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.70	188	6962m)	0.40	ng/ul	0.00
16) Chrysene-d12	21.79	240	7169m)	0.40	ng/ul	0.00
20) Perylene-d12	24.41	264	8875	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.79	152	2781	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.68	212	9112m)	0.41	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

} JU 3/30/18