

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
 Data File : BE095878.D
 Acq On : 28 Mar 2018 15:58
 Operator : SJ/JU
 Sample : J1950-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AK4

Manual Integrations
 APPROVED

Sohil
 3/29/2018 5:17:48 PM

Quant Time: Mar 29 11:38:37 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 28 16:31:37 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.41	152	1654	0.40	ng/ul	0.00
2) Naphthalene-d8	11.24	136	4489	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.00	164	2975	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.70	188	7100m	0.40	ng/ul	0.00
16) Chrysene-d12	21.79	240	7731m	0.40	ng/ul	0.00
20) Perylene-d12	24.42	264	7241m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.80	152	2446	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.68	212	8308m	0.37	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.29	128	780	0.062	ng/ul#	73
17) Pyrene	20.07	202	912m	0.031	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095878.D
Acq On : 28 Mar 2018 15:58
Operator : SJ/JU
Sample : J1950-07
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
C0AK4

Manual Integrations
APPROVED

Sohil
3/29/2018 5:17:48 PM

Quant Time: Mar 29 11:38:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 16:31:37 2018
Response via : Initial Calibration

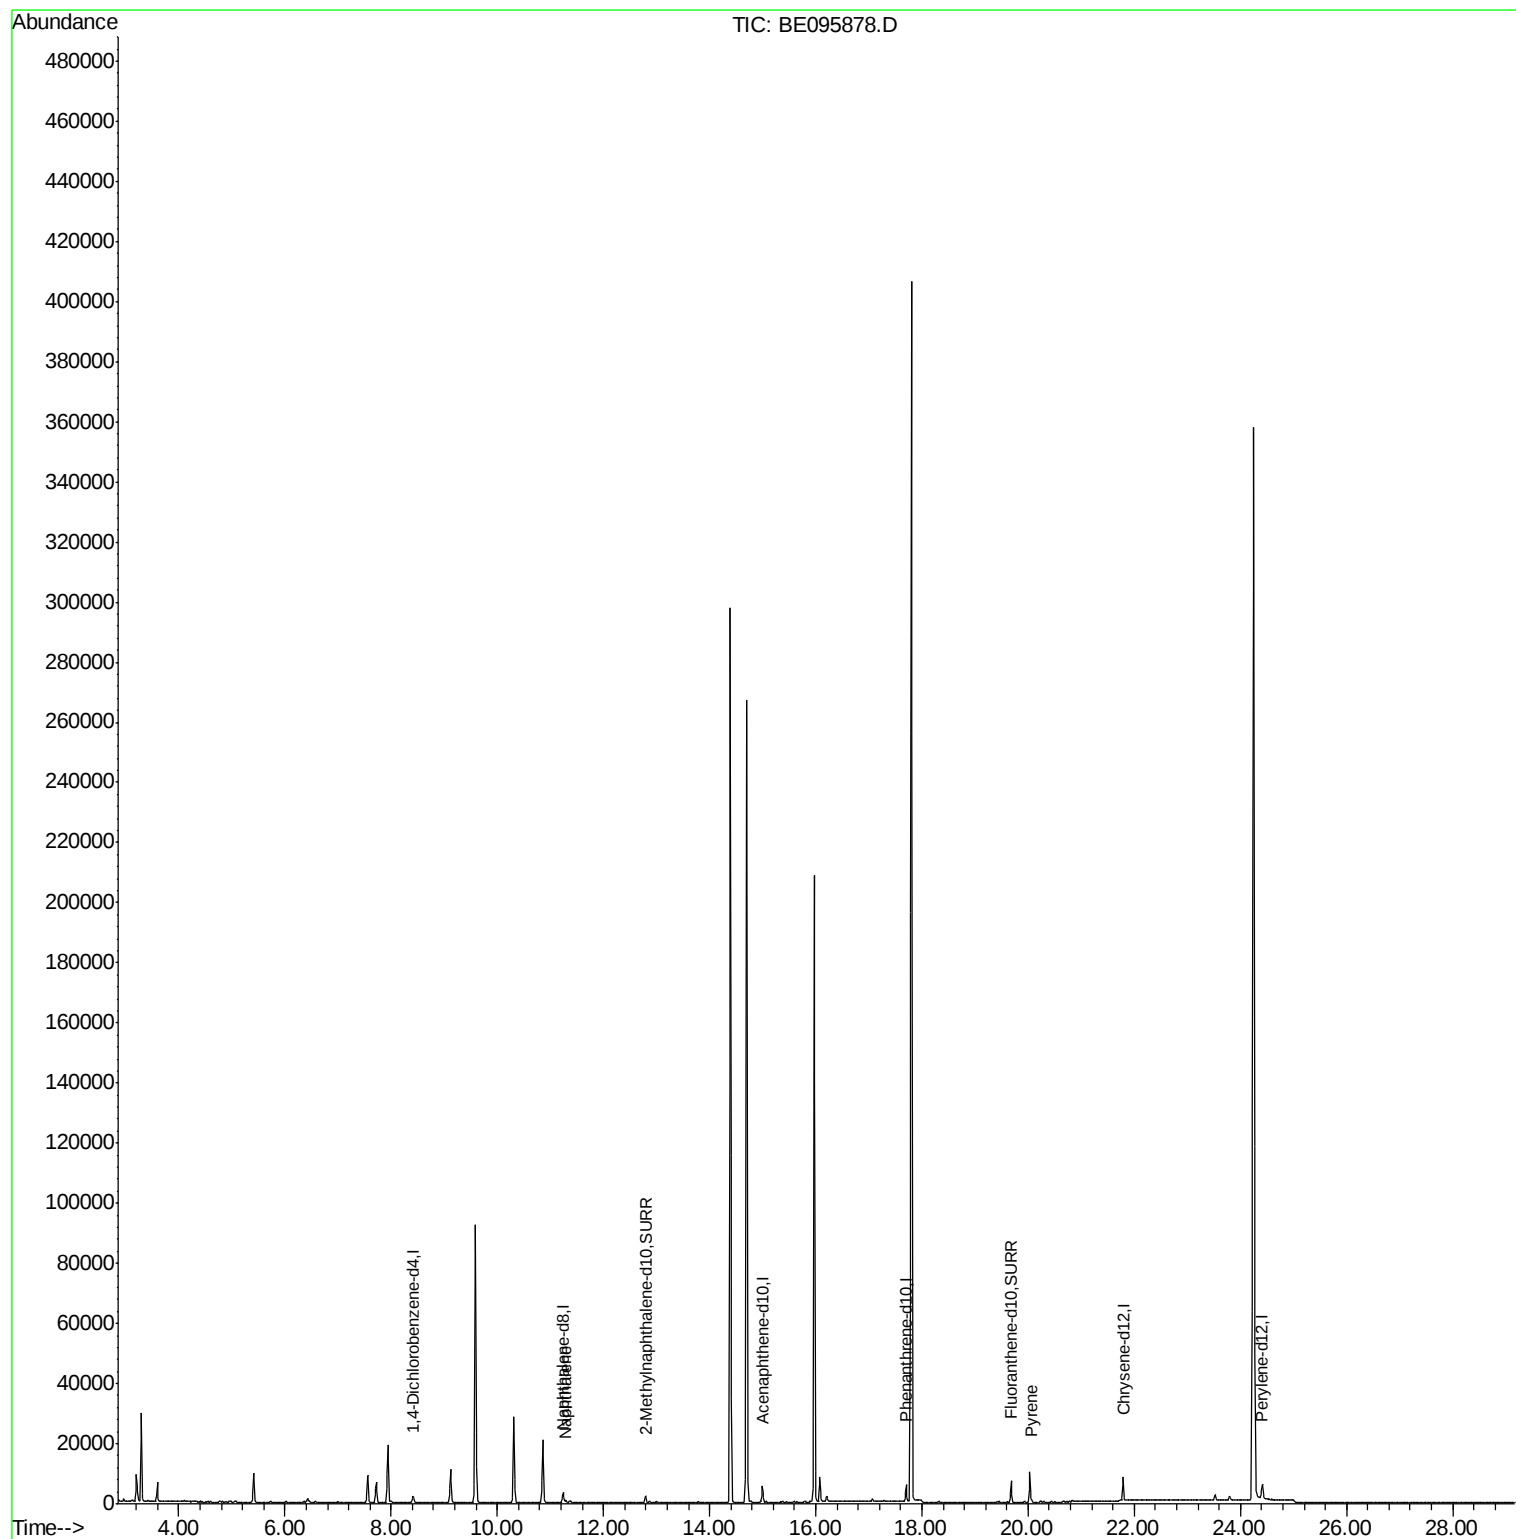

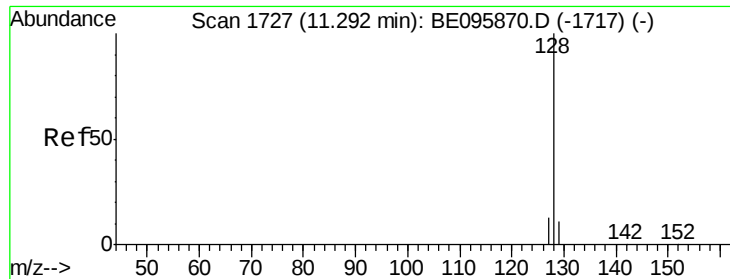

#3

Naphthalene

Concen: 0.062 ng/ul

RT: 11.29 min Scan# 1727

Delta R.T. -0.01 min

Lab File: BE095878.D

Acq: 28 Mar 2018 15:58

Instrument :

BNA_E


ClientSampleId :

C0AK4




Tot Ion:	128	Resp:	780
Ion Ratio	Lower	Upper	
128	100		
129	21.2	11.3	16.9#
127	22.3	4.0	6.0#

Manual Integrations
APPROVED

Sohil
3/29/2018 5:17:48 PM

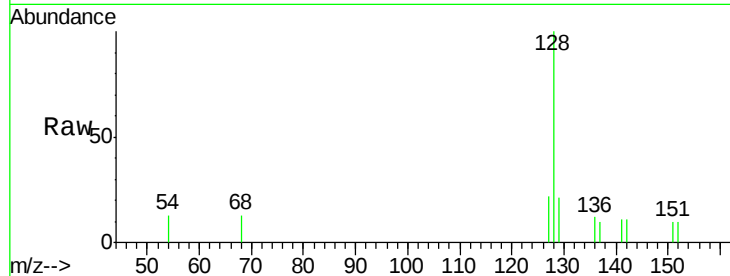

Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E

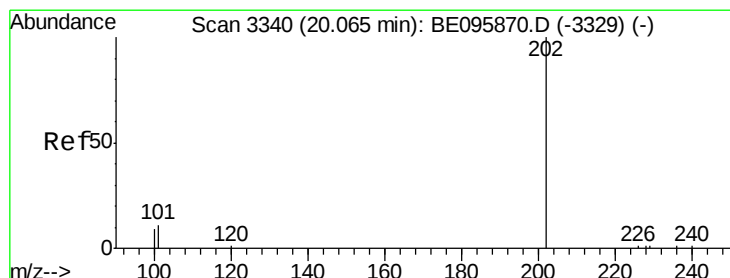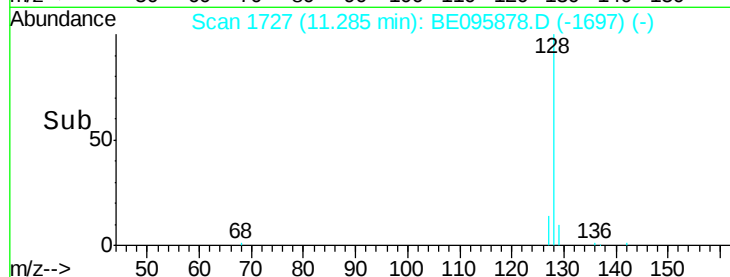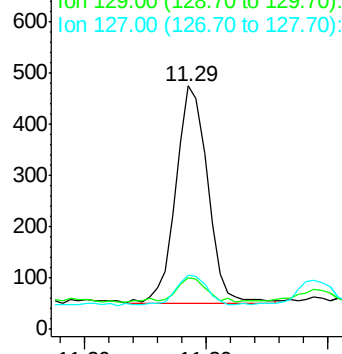

#17

Pyrene

Concen: 0.031 ng/ul m

RT: 20.07 min Scan# 3341

Delta R.T. 0.00 min

Lab File: BE095878.D

Acq: 28 Mar 2018 15:58

Tgt Ion:	202	Resp:	912
Ion Ratio	Lower	Upper	
202	100		
101	22.4	18.2	27.4
100	25.2	15.6	23.4#

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): E

