
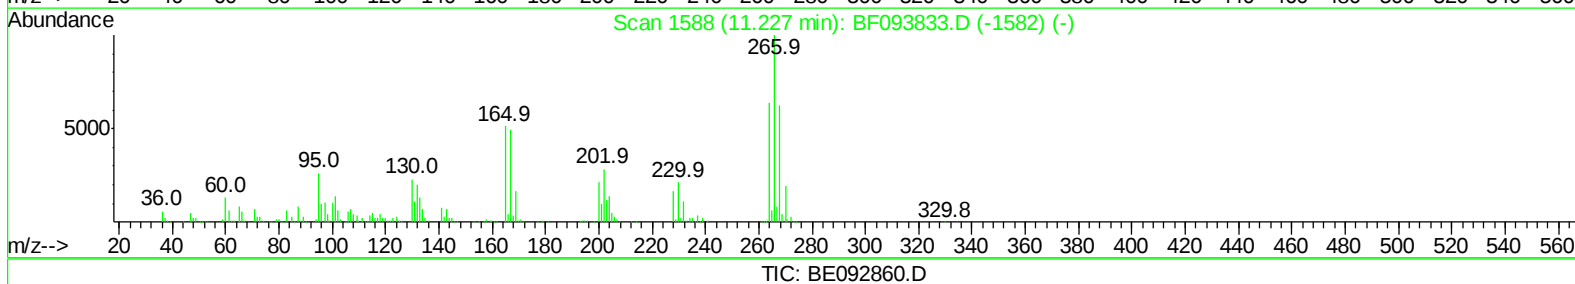
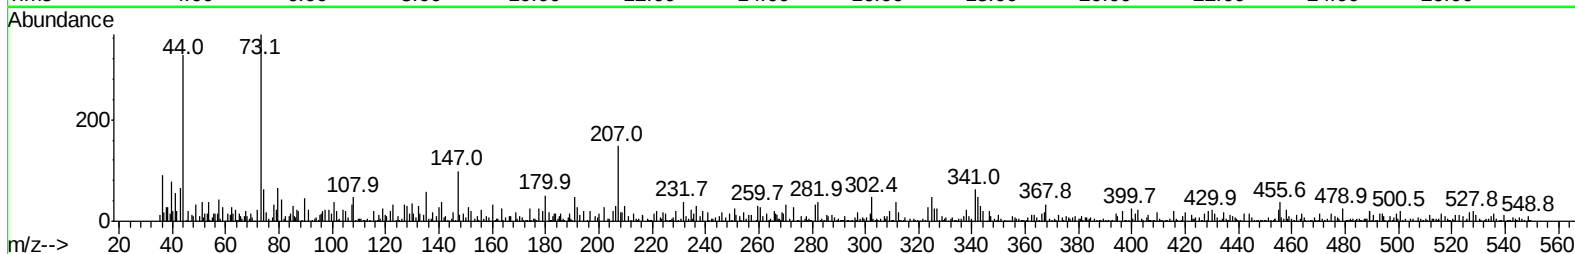


Data Path : Z:\HPCHEM1\BNA E\Data\BE032917\
Data File : BE092860.D
Acq On : 29 Mar 2017 8:58
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 07:25:29 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 27 16:10:49 2017
Response via : Initial Calibration

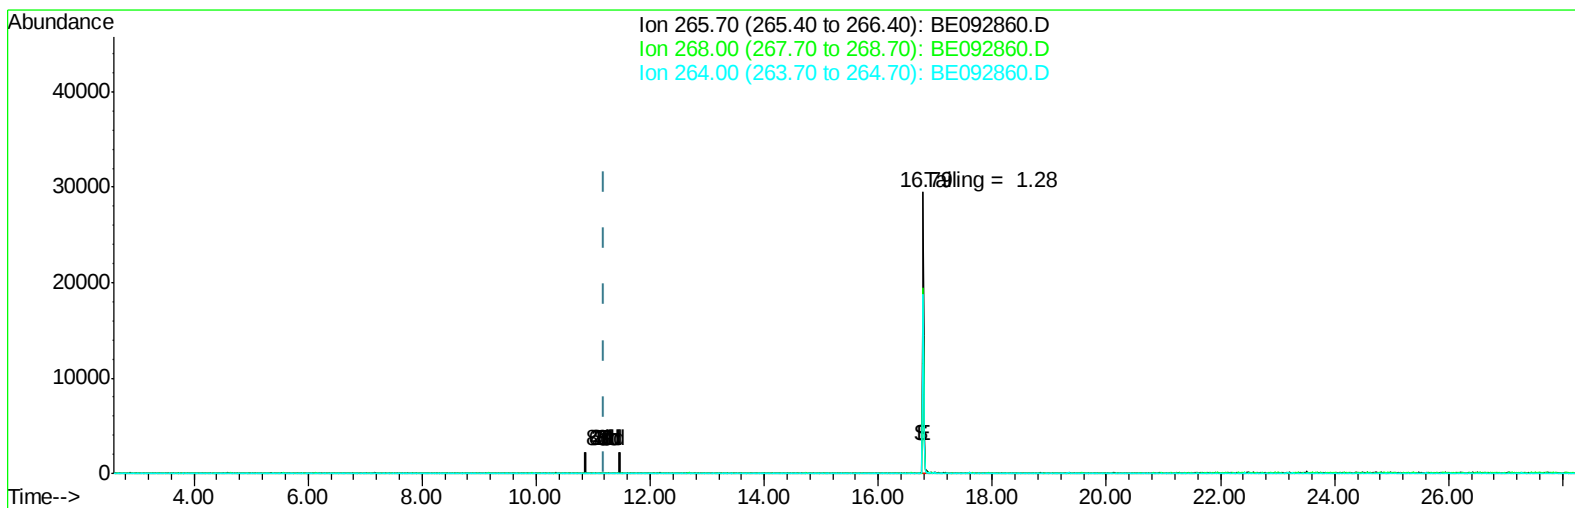

TIC: BE092860.D

(69) Pentachlorophenol (C)




11.209min (+0.011) 105.24ng

response 15

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	22.22#
264.00	64.60	27.78#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE032917\
Data File : BE092860.D
Acq On : 29 Mar 2017 8:58
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 07:25:29 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 27 16:10:49 2017
Response via : Initial Calibration

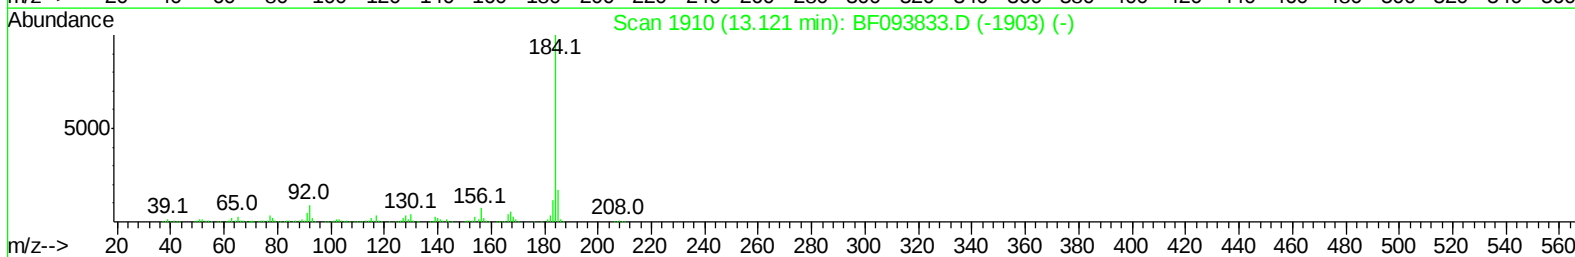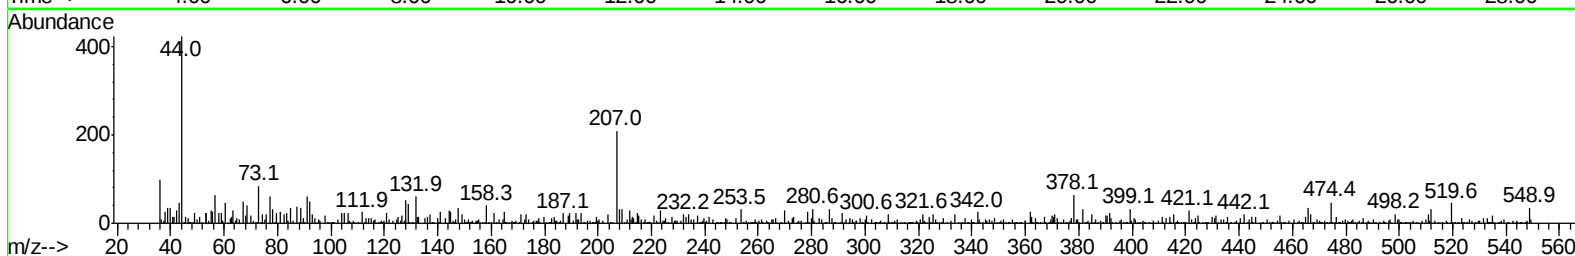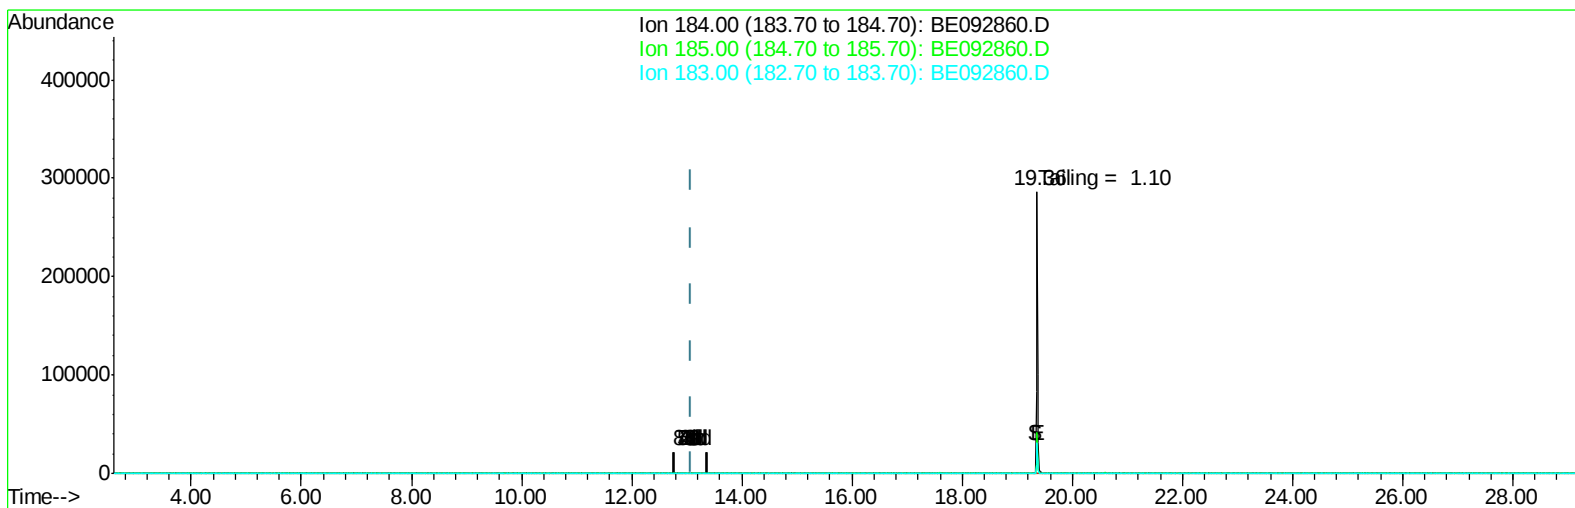

TIC: BE092860.D

(76) Benzidine

13.131min (+0.044) 9.63ng

response 8

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	58.33#
183.00	12.20	208.33#
0.00	0.00	0.00