


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032917\
 Data File : BE092860.D
 Acq On : 29 Mar 2017 8:58
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 29 17:47:56 2017

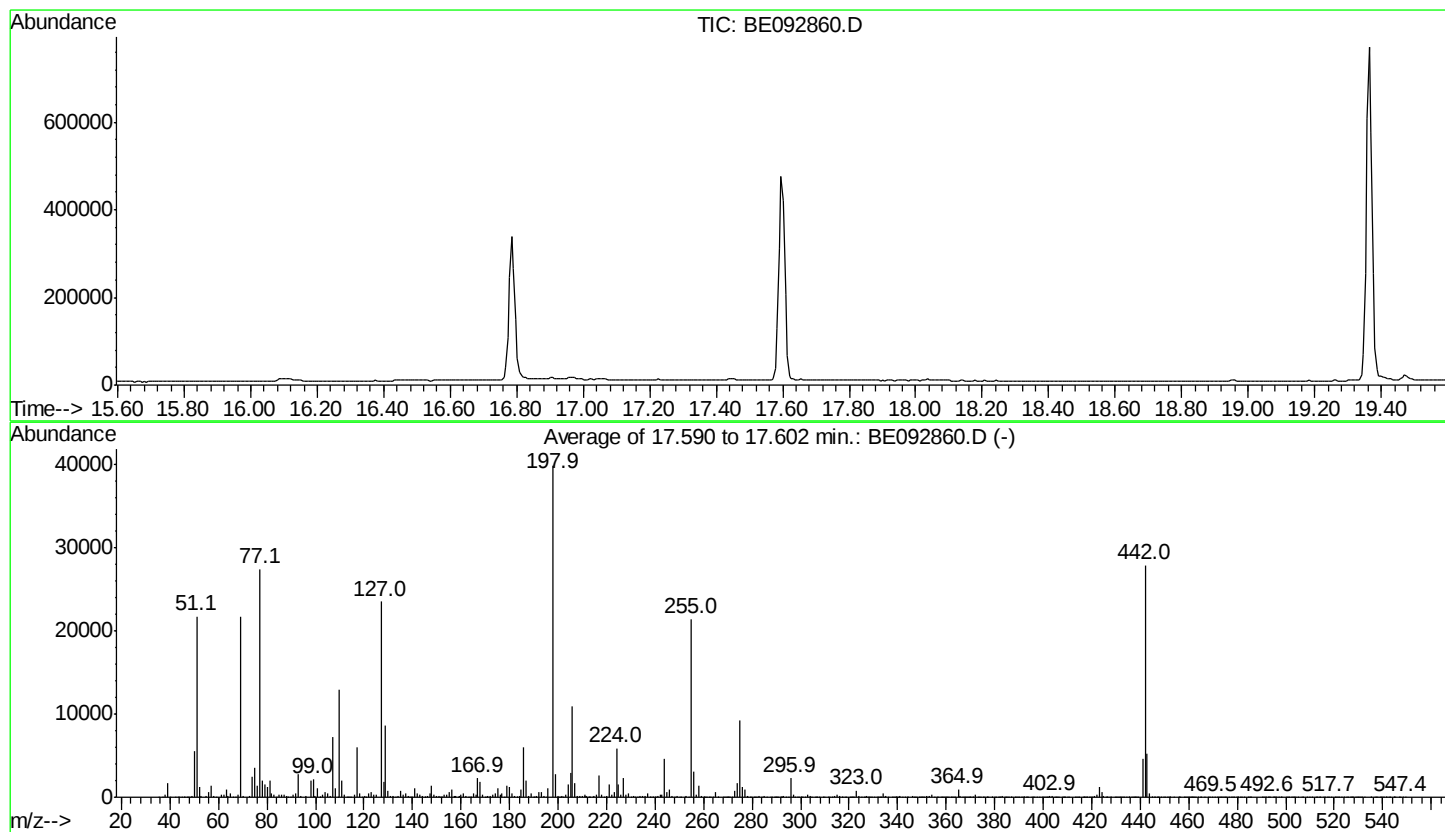

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.5	21690	PASS
68	69	0.00	2	1.1	241	PASS
69	198	0.00	100	54.5	21695	PASS
70	69	0.00	2	0.6	140	PASS
127	198	10	80	59.0	23456	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39789	PASS
199	198	5	9	6.8	2707	PASS
275	198	10	60	23.2	9220	PASS
365	198	1	100	2.5	1002	PASS
441	442	0.01	24	16.5	4598	PASS
442	198	50	100	69.9	27832	PASS
443	442	15	24	18.7	5198	PASS