


Data Path : Z:\HPCHEM1\BNA_E\Data\BE033016\
 Data File : BE091552.D
 Acq On : 30 Mar 2016 10:46
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE033016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 30 18:45:59 2016

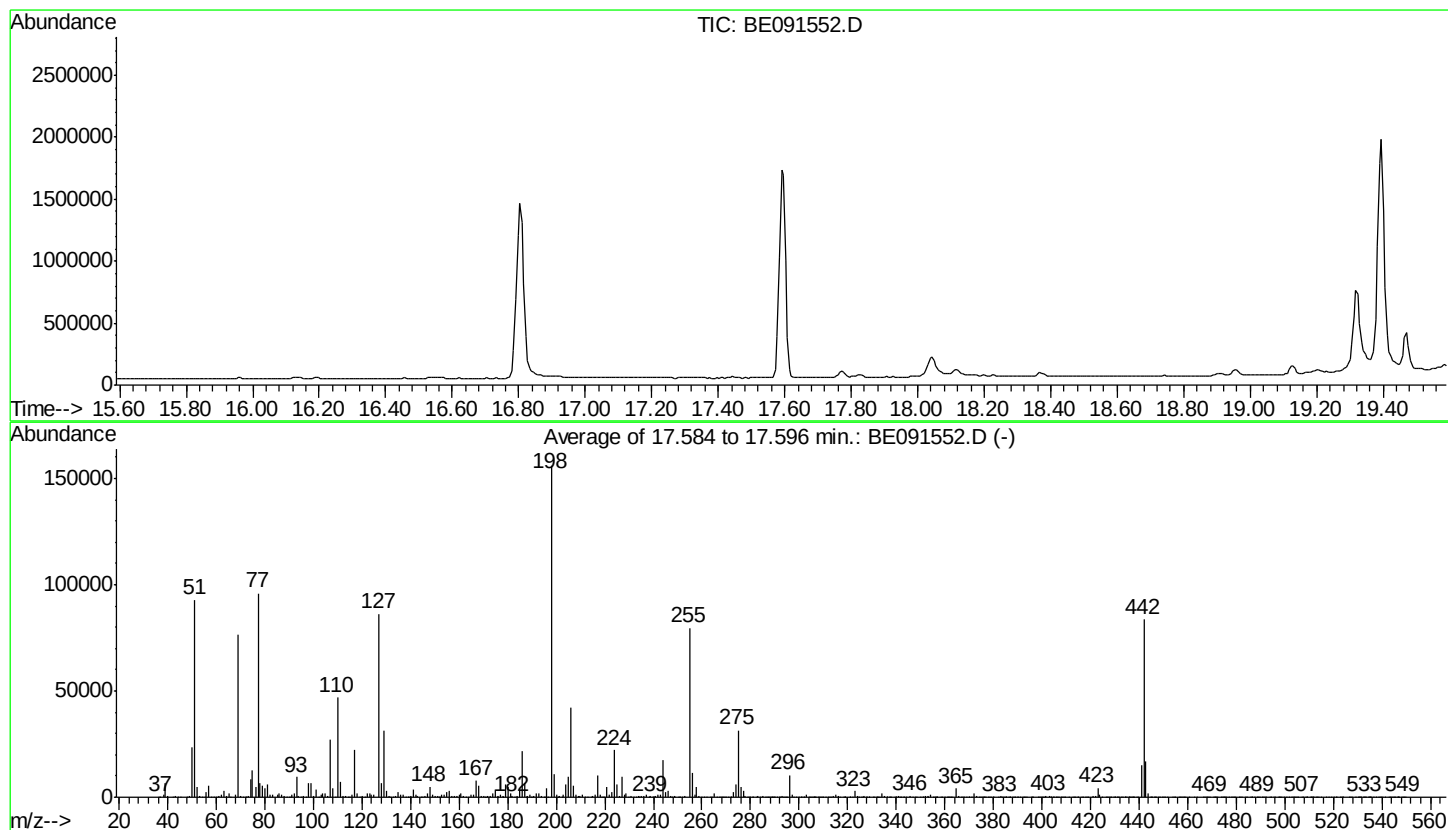

AutoFind: Scans 2552, 2553, 2554; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.5	92780	PASS
68	69	0.00	2	1.8	1360	PASS
69	198	0.00	100	49.0	76429	PASS
70	69	0.00	2	0.4	333	PASS
127	198	10	80	55.4	86368	PASS
197	198	0.00	2	0.1	185	PASS
198	198	100	100	100.0	155973	PASS
199	198	5	9	6.8	10656	PASS
275	198	10	60	20.2	31461	PASS
365	198	1	100	2.6	4122	PASS
441	442	0.01	24	17.7	14792	PASS
442	198	50	100	53.6	83637	PASS
443	442	15	24	20.1	16798	PASS