
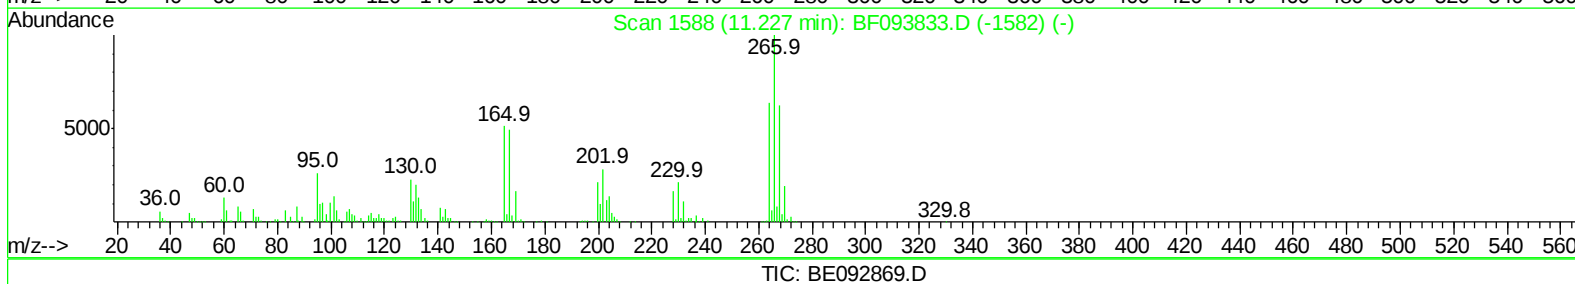
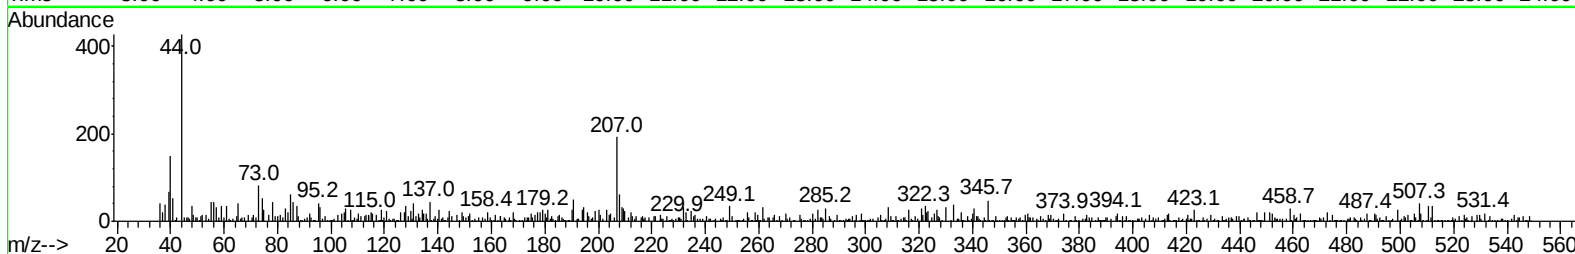


Data Path : Z:\HPCHEM1\BNA E\Data\BE033017\
Data File : BE092869.D
Acq On : 30 Mar 2017 9:14
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 06:44:10 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 27 16:10:49 2017
Response via : Initial Calibration

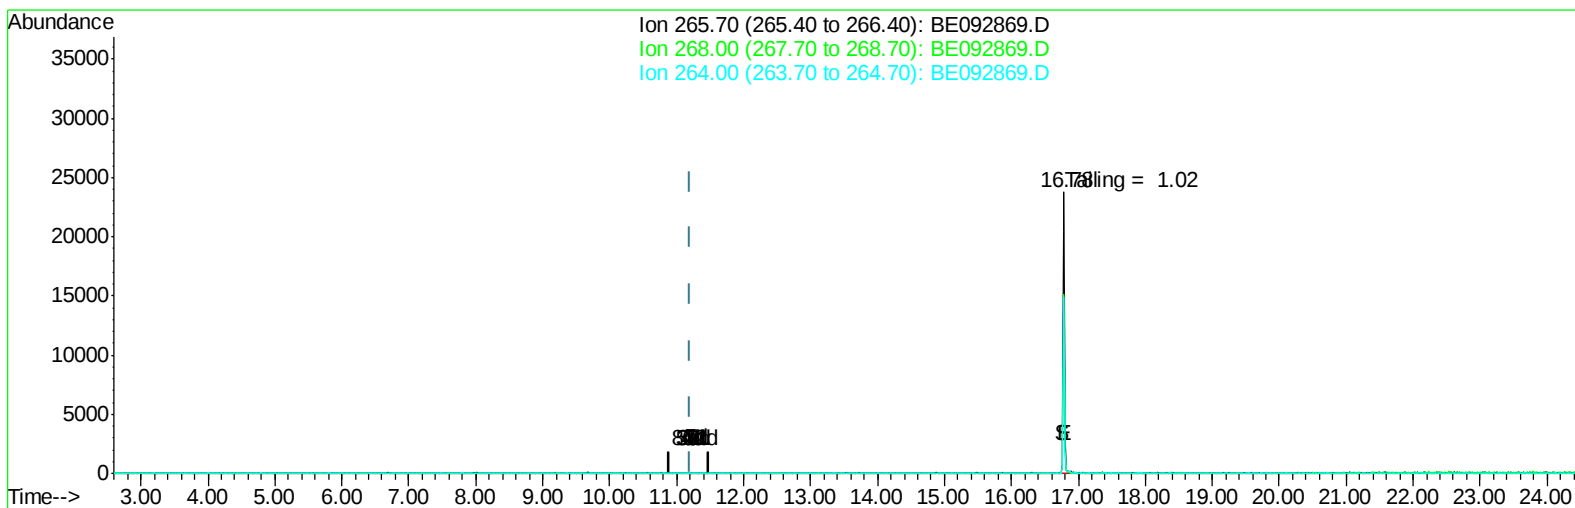

TIC: BE092869.D

(69) Pentachlorophenol (C)




11.426min (+0.228) 371.16ng

response 23

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	75.00
264.00	64.60	56.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE033017\
Data File : BE092869.D
Acq On : 30 Mar 2017 9:14
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 06:44:10 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 27 16:10:49 2017
Response via : Initial Calibration

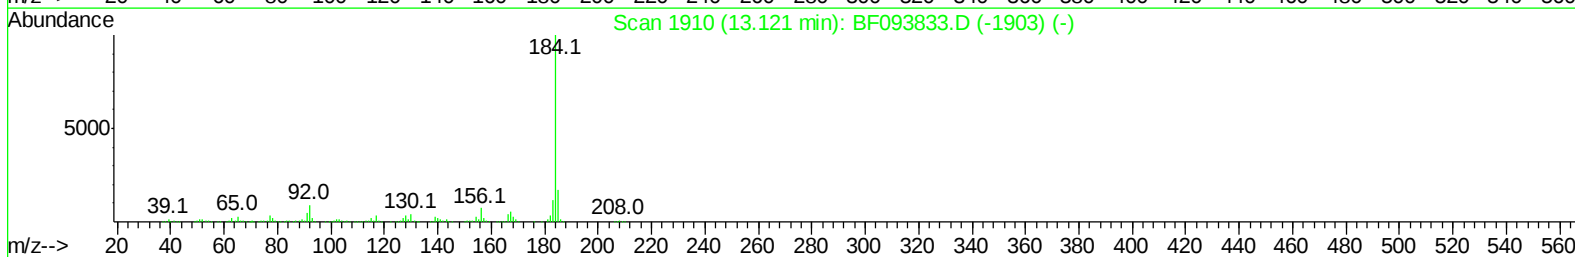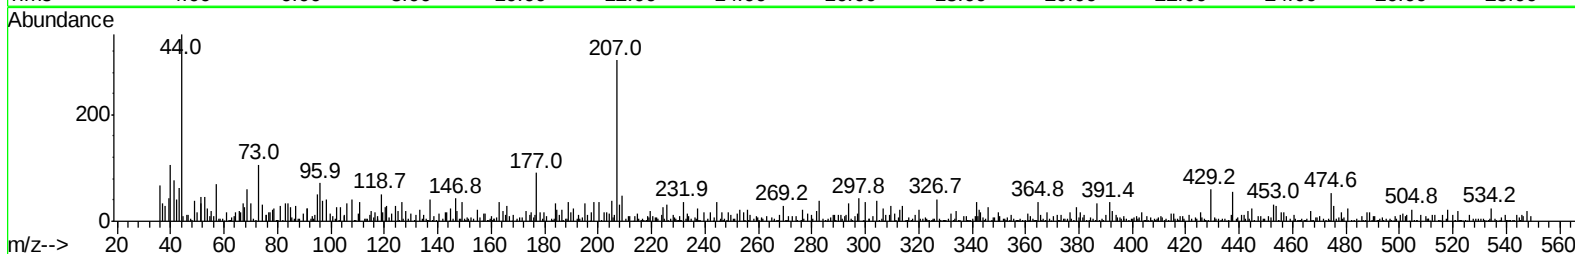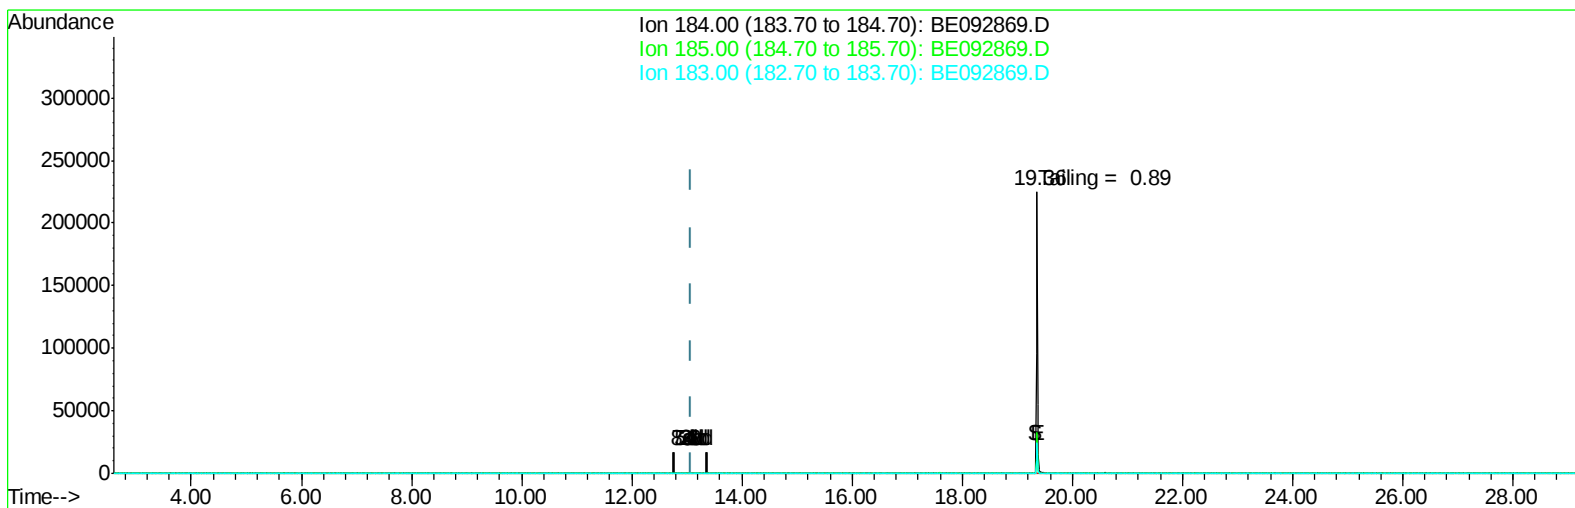

TIC: BE092869.D

(76) Benzidine

13.142min (+0.055) 39.42ng

response 39

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	19.64
183.00	12.20	14.29
0.00	0.00	0.00