


Data Path : Z:\HPCHEM1\BNA E\DATA\BE033017\  
 Data File : BE092869.D  
 Acq On : 30 Mar 2017 9:14  
 Operator : SJ/MA  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE032817.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Mar 29 17:47:56 2017

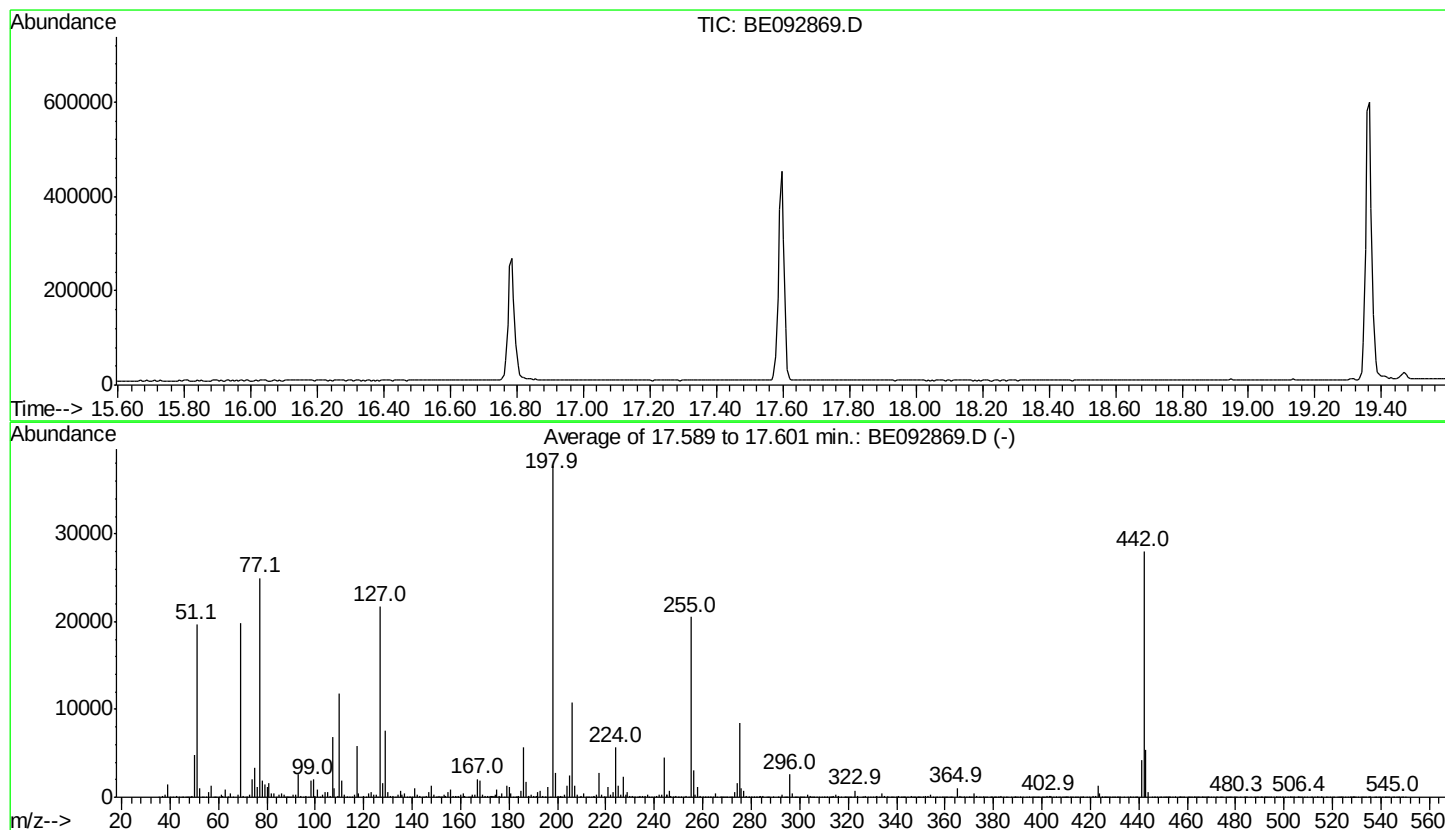

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2546

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 52.0      | 19638   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.5       | 297     | PASS             |
| 69          | 198          | 0.00         | 100          | 52.3      | 19770   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 126     | PASS             |
| 127         | 198          | 10           | 80           | 57.5      | 21702   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.1       | 33      | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 37773   | PASS             |
| 199         | 198          | 5            | 9            | 7.2       | 2719    | PASS             |
| 275         | 198          | 10           | 60           | 22.4      | 8463    | PASS             |
| 365         | 198          | 1            | 100          | 2.7       | 1022    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.2      | 4258    | PASS             |
| 442         | 198          | 50           | 100          | 74.0      | 27964   | PASS             |
| 443         | 442          | 15           | 24           | 19.4      | 5419    | PASS             |