


Data Path : Z:\HPCHEM1\BNA_E\Data\BE033116\
Data File : BE091563.D
Acq On : 30 Mar 2016 20:43
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE033016.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 30 18:45:59 2016

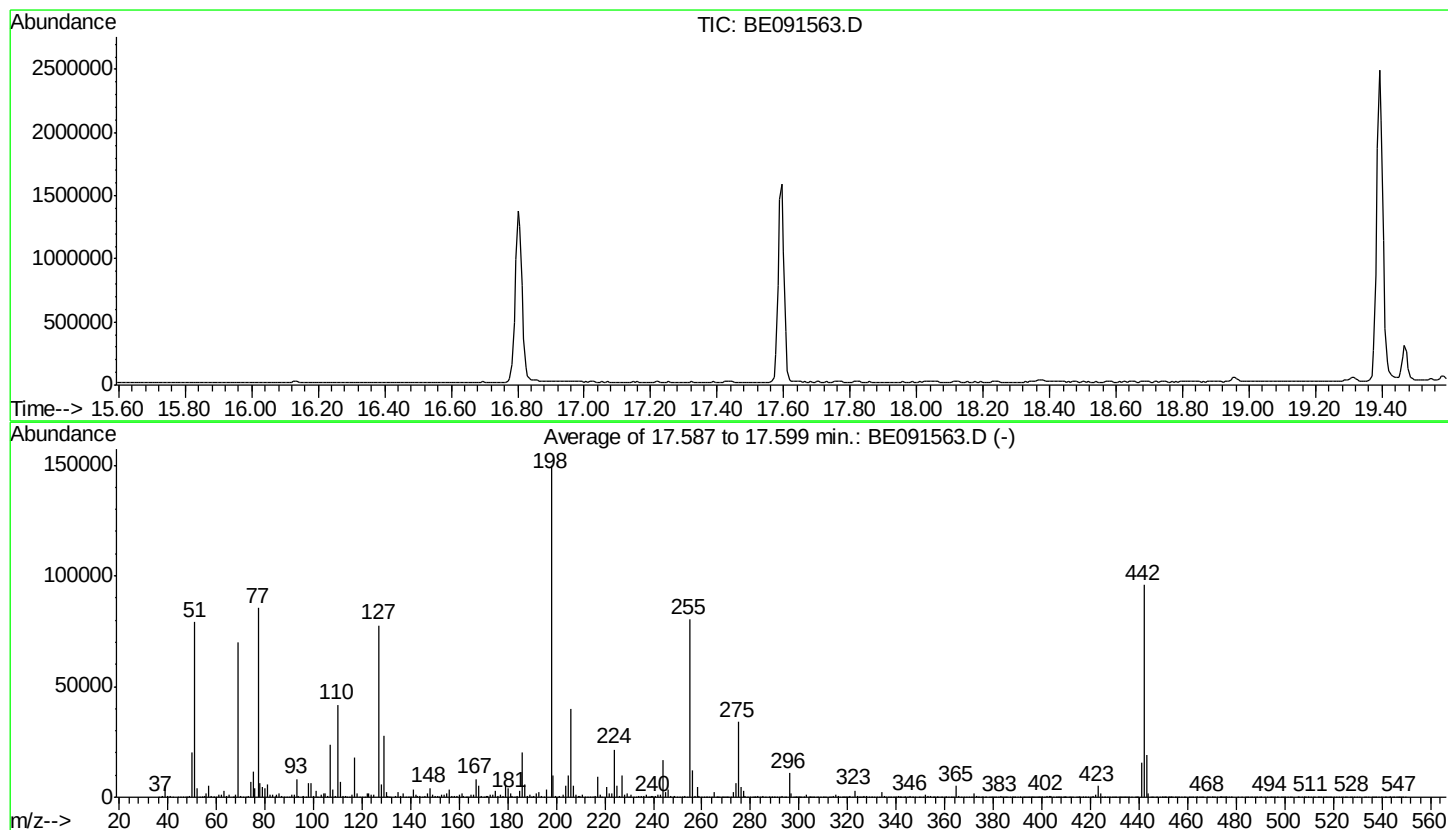

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.7	78977	PASS
68	69	0.00	2	1.7	1175	PASS
69	198	0.00	100	46.7	69939	PASS
70	69	0.00	2	0.6	386	PASS
127	198	10	80	51.8	77496	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	149728	PASS
199	198	5	9	6.4	9609	PASS
275	198	10	60	22.7	33968	PASS
365	198	1	100	3.3	4940	PASS
441	442	0.01	24	16.5	15782	PASS
442	198	50	100	64.0	95886	PASS
443	442	15	24	20.0	19187	PASS