
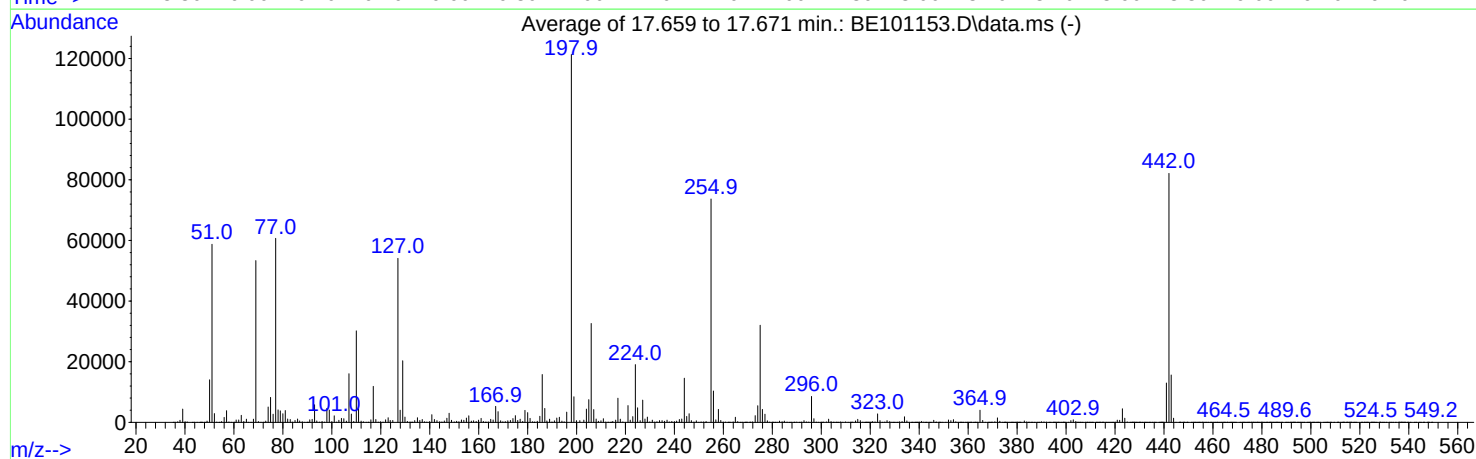


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE033121\
 Data File : BE101153.D
 Acq On : 31 Mar 2021 9:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE032421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 31 11:11:33 2021

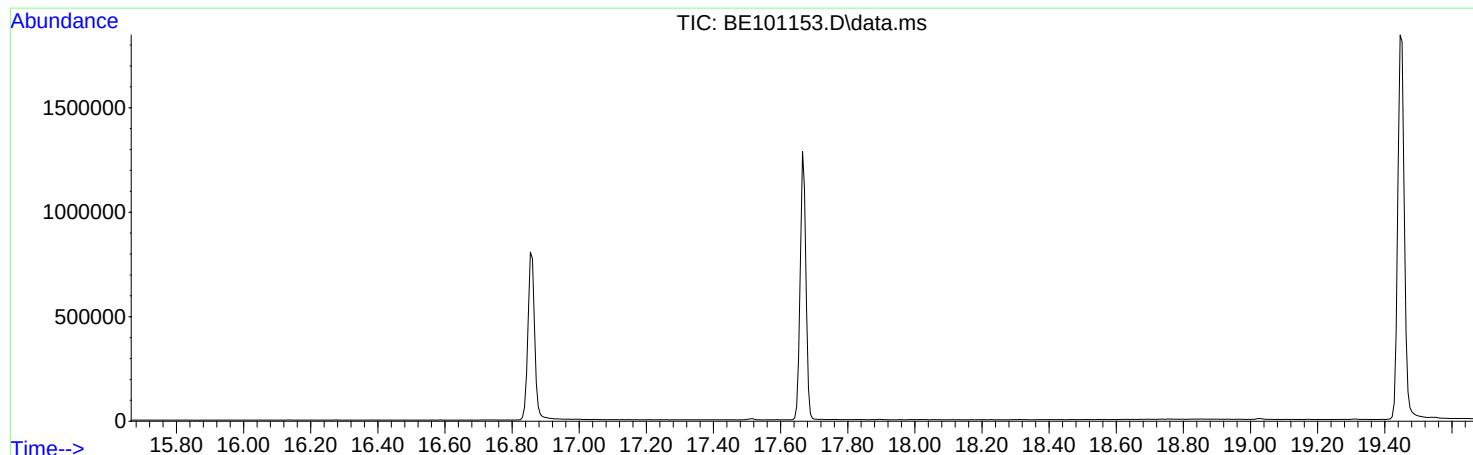




AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	58712	PASS
68	69	0.00	2	2.0	1042	PASS
69	198	0.00	100	44.0	53359	PASS
70	69	0.00	2	0.5	245	PASS
127	198	10	80	44.6	54101	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	121323	PASS
199	198	5	9	7.0	8465	PASS
275	198	10	60	26.4	32014	PASS
365	198	1	100	3.3	3991	PASS
441	198	0.01	100	10.7	12980	PASS
442	442	50	100	100.0	82120	PASS
443	442	15	24	19.1	15649	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE033121\
Data File : BE101153.D
Acq On : 31 Mar 2021 9:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Mar 31 10:54:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 10:54:22 2021
Response via : Initial Calibration

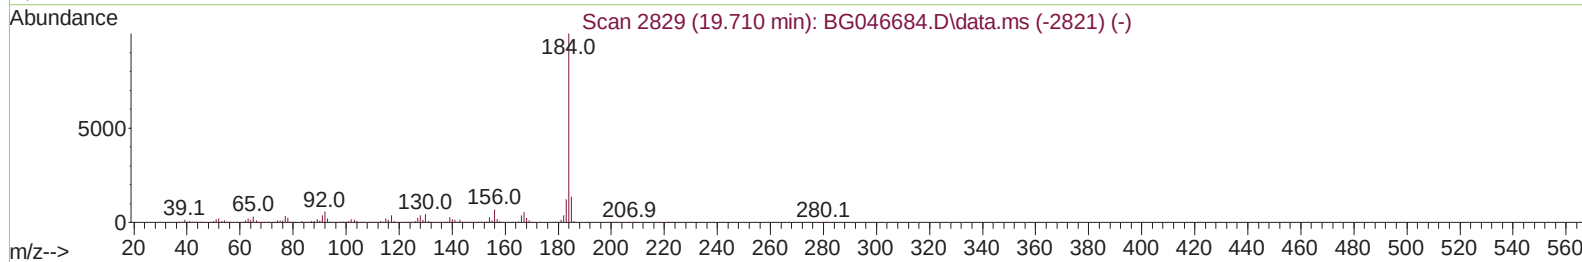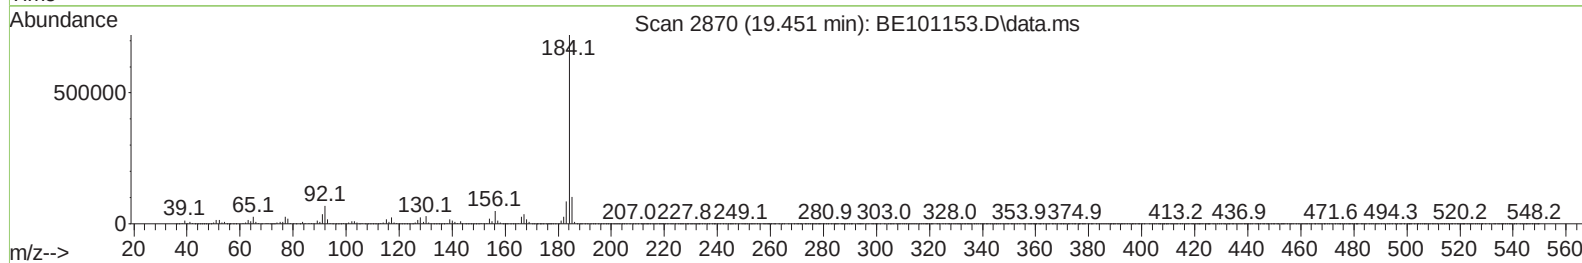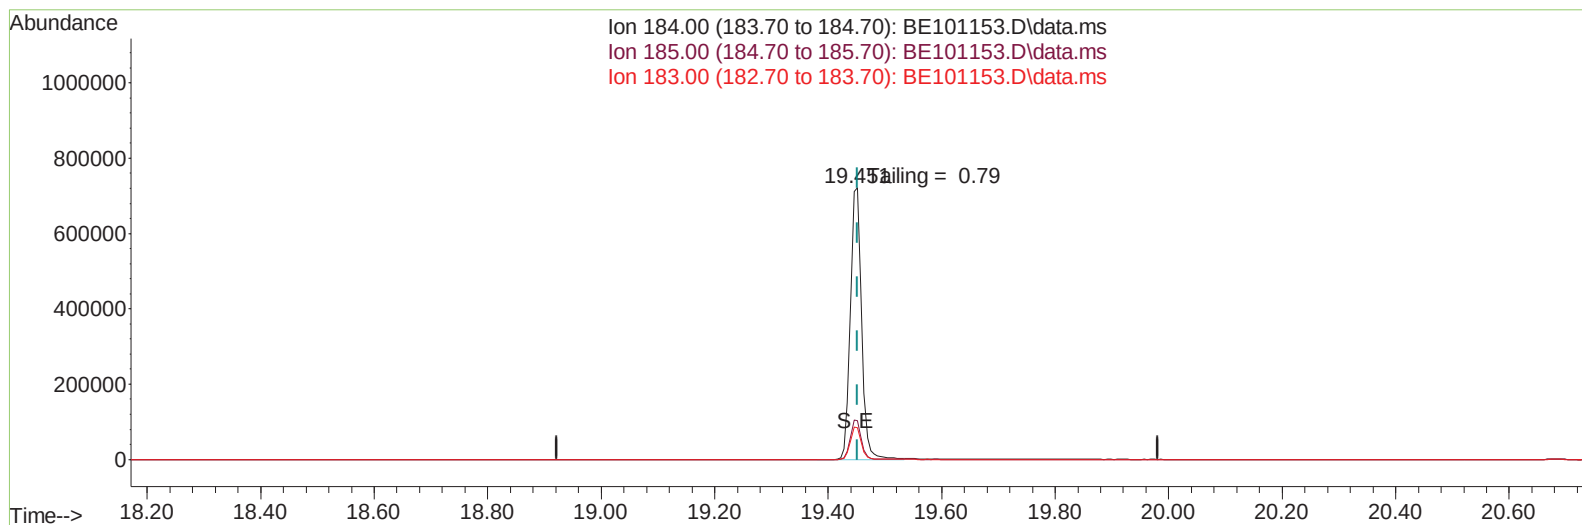

TIC: BE101153.D\data.ms

(77) Benzidine

19.451min (0.000) 5970.13 ng

response 1012726

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.22
183.00	13.20	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/31/2021	BNA_E	<u>BE101153.D</u>
Compound Name	Response	Retention Time
DDT	355376	20.685
DDD	603	20.245
DDE	637	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1240	356616	0.35