


Data Path : Z:\HPCHEM1\BNA_E\Data\BE040116\
 Data File : BE091577.D
 Acq On : 31 Mar 2016 9:39
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE033016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 30 18:45:59 2016

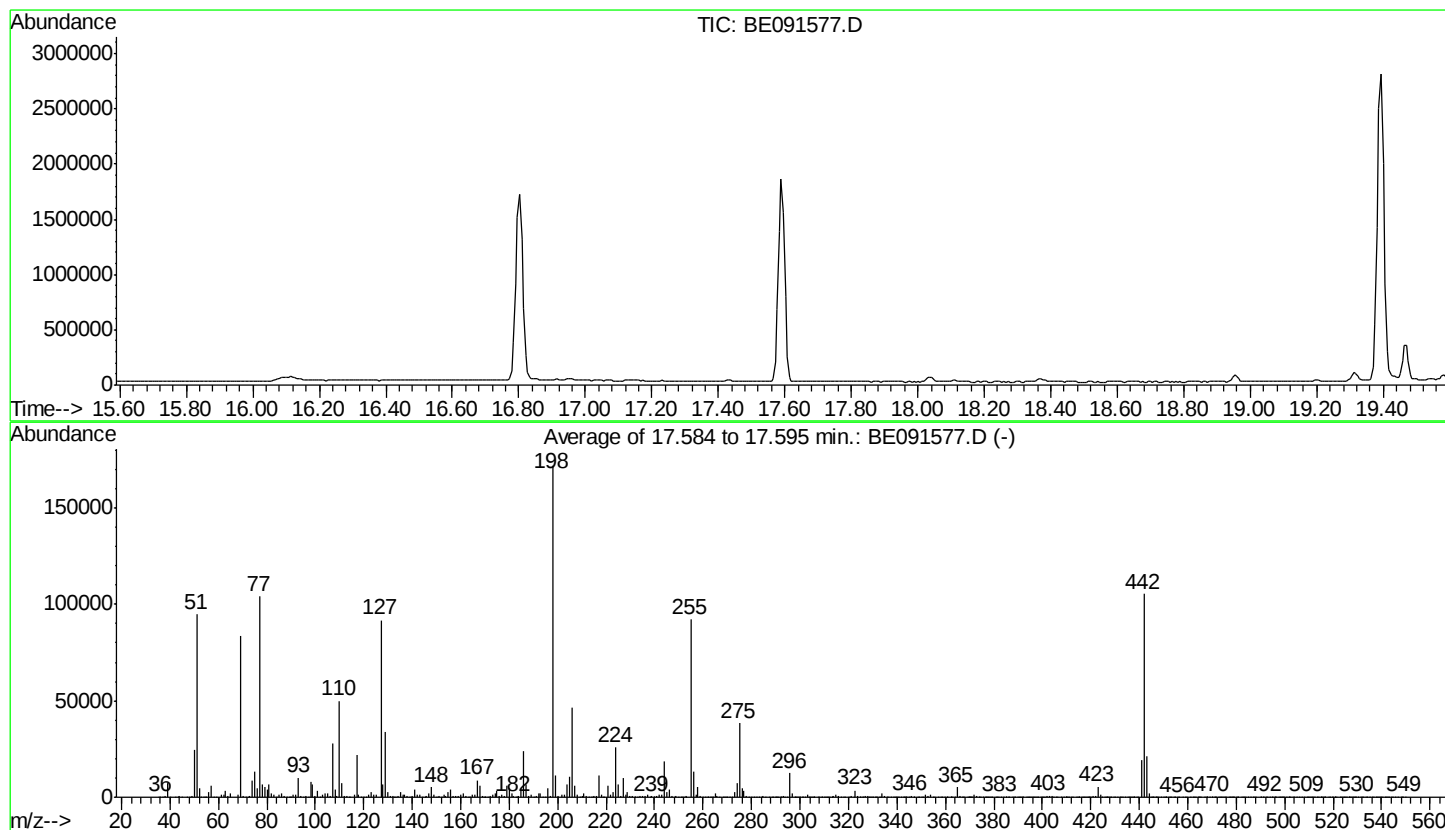

AutoFind: Scans 2552, 2553, 2554; Background Corrected with Scan 2543

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.2	94878	PASS
68	69	0.00	2	1.5	1240	PASS
69	198	0.00	100	48.5	83379	PASS
70	69	0.00	2	0.5	450	PASS
127	198	10	80	53.4	91842	PASS
197	198	0.00	2	0.2	379	PASS
198	198	100	100	100.0	171877	PASS
199	198	5	9	6.7	11487	PASS
275	198	10	60	22.4	38420	PASS
365	198	1	100	3.0	5144	PASS
441	442	0.01	24	18.1	19080	PASS
442	198	50	100	61.3	105365	PASS
443	442	15	24	20.2	21273	PASS