



Abundance

Ion 265.70 (265.40 to 266.40): BE101171.D\data.ms  
Ion 268.00 (267.70 to 268.70): BE101171.D\data.ms  
Ion 264.00 (263.70 to 264.70): BE101171.D\data.ms

16.853  
16.853  
Tailing = 1.23

S E

me--> 15.60 15.80 16.00 16.20 16.40 16.60 16.80 17.00 17.20 17.40 17.60 17.80 18.00

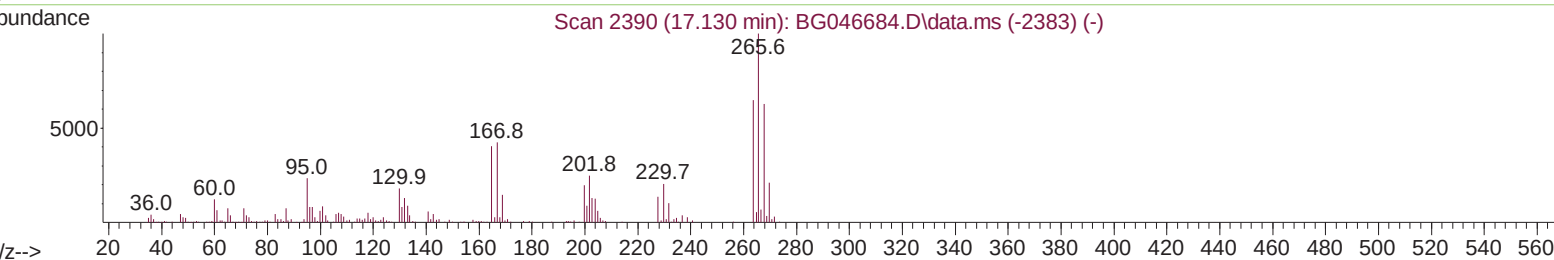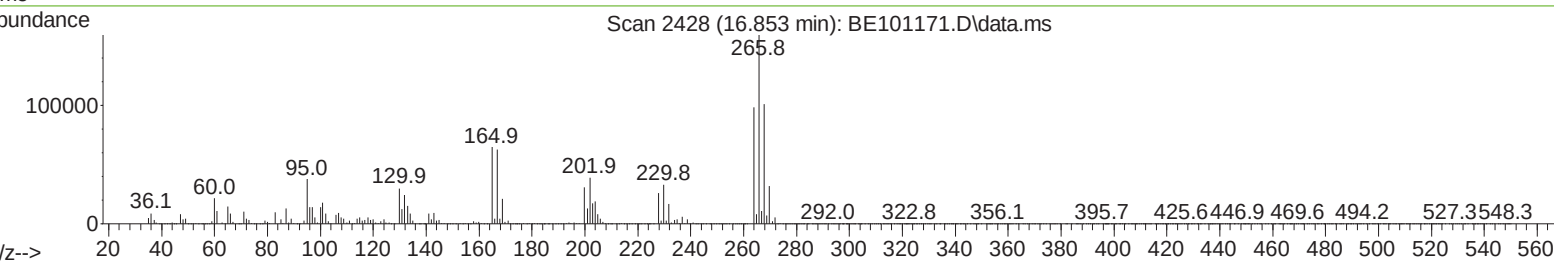




TIC: BE101171.D\data.ms

**response**      **216482**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.51  |
| 264.00 | 61.60  | 61.80  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE040121\  
Data File : BE101171.D  
Acq On : 1 Apr 2021 11:10  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 12:16:46 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 31 10:54:22 2021  
Response via : Initial Calibration

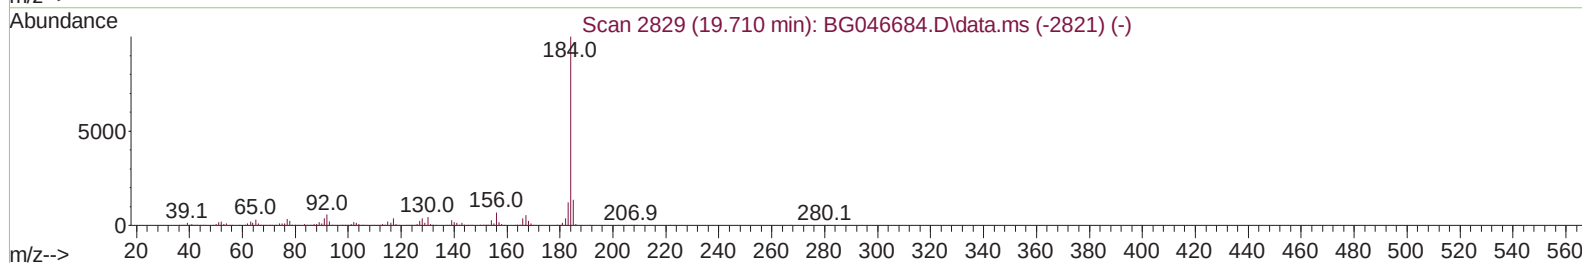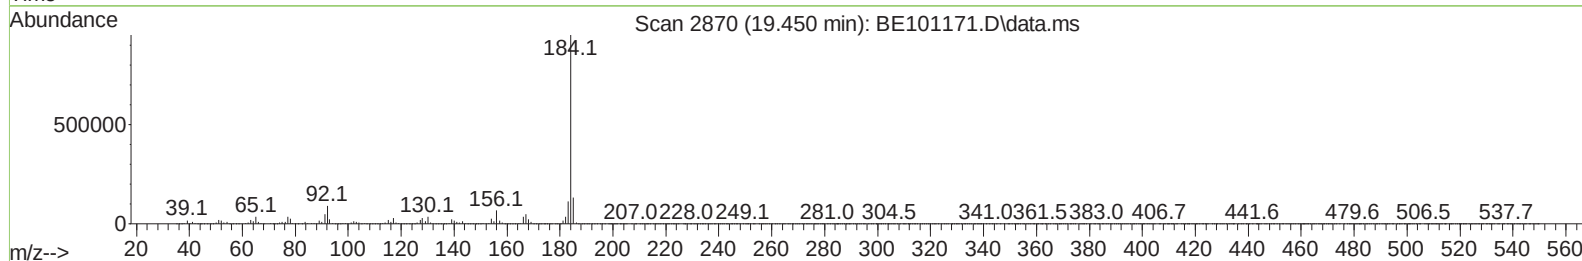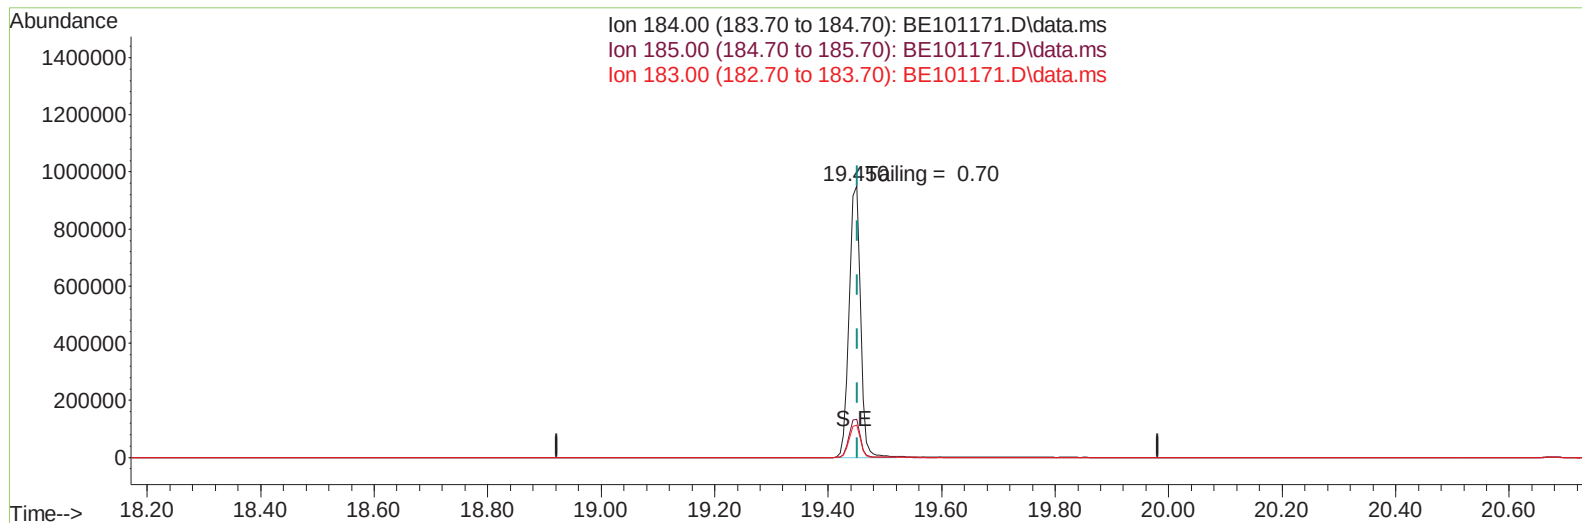

TIC: BE101171.D\data.ms

**(77) Benzidine****19.450min (-0.001) 4952.59 ng****response 1331089**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.00  |
| 183.00 | 13.20  | 11.82  |
| 0.00   | 0.00   | 0.00   |