


Data Path : Z:\HPCHEM1\BNA E\Data\BE040216\
 Data File : BE091591.D
 Acq On : 1 Apr 2016 15:20
 Operator : UM/SJ
 Sample : DFTPP
 Misc : LOO WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE033016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 30 18:45:59 2016

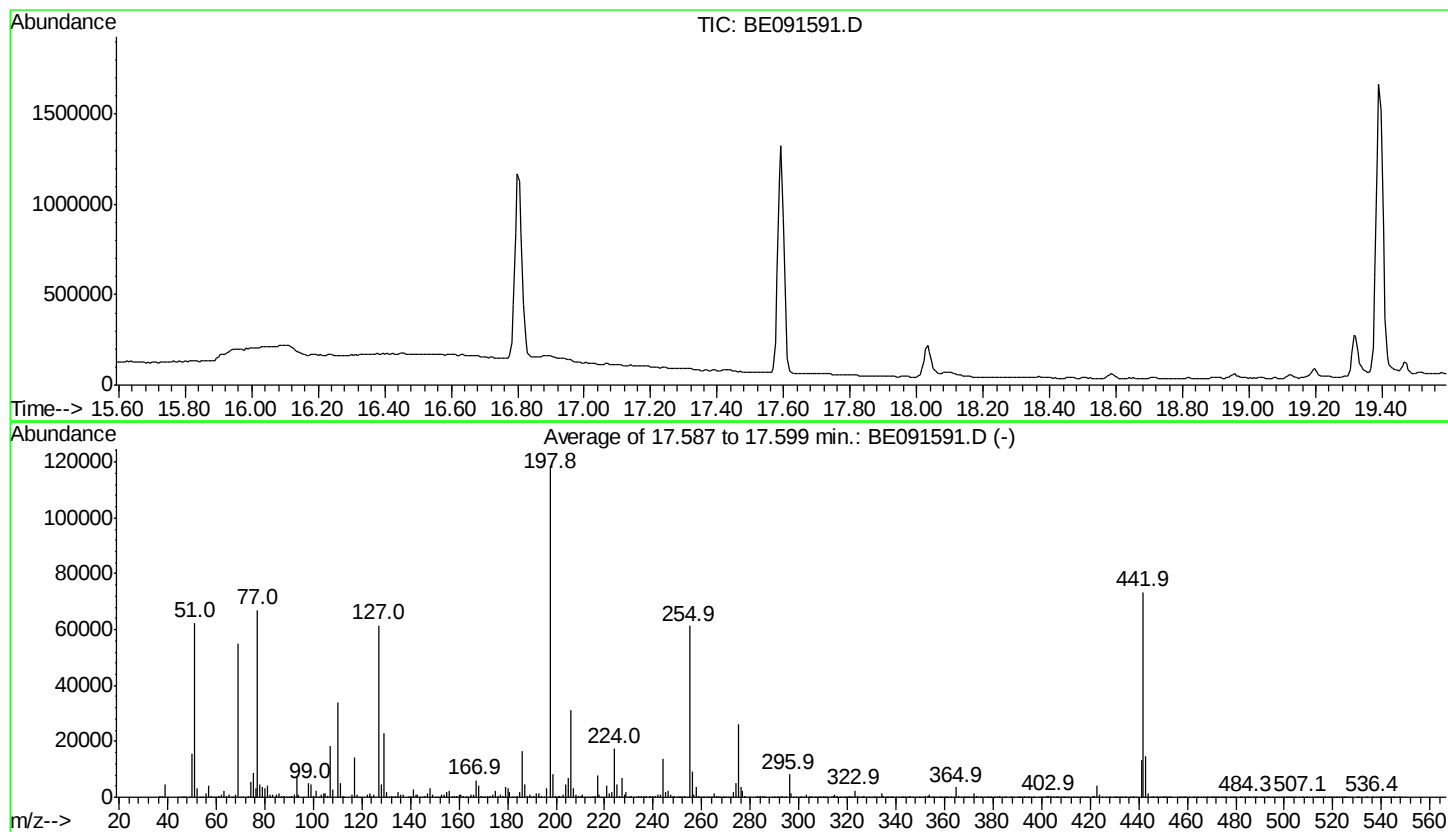

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2545

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.6	62431	PASS
68	69	0.00	2	1.6	870	PASS
69	198	0.00	100	46.5	55201	PASS
70	69	0.00	2	0.4	233	PASS
127	198	10	80	51.8	61464	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	118692	PASS
199	198	5	9	7.1	8449	PASS
275	198	10	60	22.1	26178	PASS
365	198	1	100	2.9	3454	PASS
441	442	0.01	24	18.1	13288	PASS
442	198	50	100	61.8	73360	PASS
443	442	15	24	19.8	14506	PASS