

Data Path : Z:\HPCHEM1\BNA E\DATA\BE040218\
 Data File : BE095928.D
 Acq On : 2 Apr 2018 15:33
 Operator : SJ/JU
 Sample : J2116-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Apr 03 03:50:40 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE032318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 23 12:41:11 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.42	152	1179	0.40	ng	0.00
7) Naphthalene-d8	11.26	136	4787	0.40	ng	0.00
13) Acenaphthene-d10	14.99	164	2776	0.40	ng	-0.01
19) Phenanthrene-d10	17.70	188	6455	0.40	ng	-0.01
27) Chrysene-d12	21.79	240	6918	0.40	ng	-0.01
34) Perylene-d12	24.42	264	6805	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.91	112	616	0.16	ng	0.00
5) Phenol-d6	7.56	99	518	0.10	ng	0.00
8) Nitrobenzene-d5	9.59	82	2282	0.40	ng	0.00
11) 2-Methylnaphthalene-d10	12.79	152	3210	0.40	ng	0.00
14) 2,4,6-Tribromophenol	16.46	330	642	0.40	ng	-0.01
15) 2-Fluorobiphenyl	13.63	172	5442	0.47	ng	-0.01
25) Fluoranthene-d10	19.68	212	36530	0.38	ng	0.00
29) Terphenyl-d14	20.24	244	7426	0.51	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.63	88	889	0.461	ng	93
22) Pentachlorophenol	17.36	266	46	0.162	ng	92
23) Phenanthrene	17.74	178	498	0.026	ng	# 82
32) Bis(2-ethylhexyl)phthalate	21.64	149	7411	0.101	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE040218\
Data File : BE095928.D
Acq On : 2 Apr 2018 15:33
Operator : SJ/JU
Sample : J2116-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Apr 03 03:50:40 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE032318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 23 12:41:11 2018
Response via : Initial Calibration

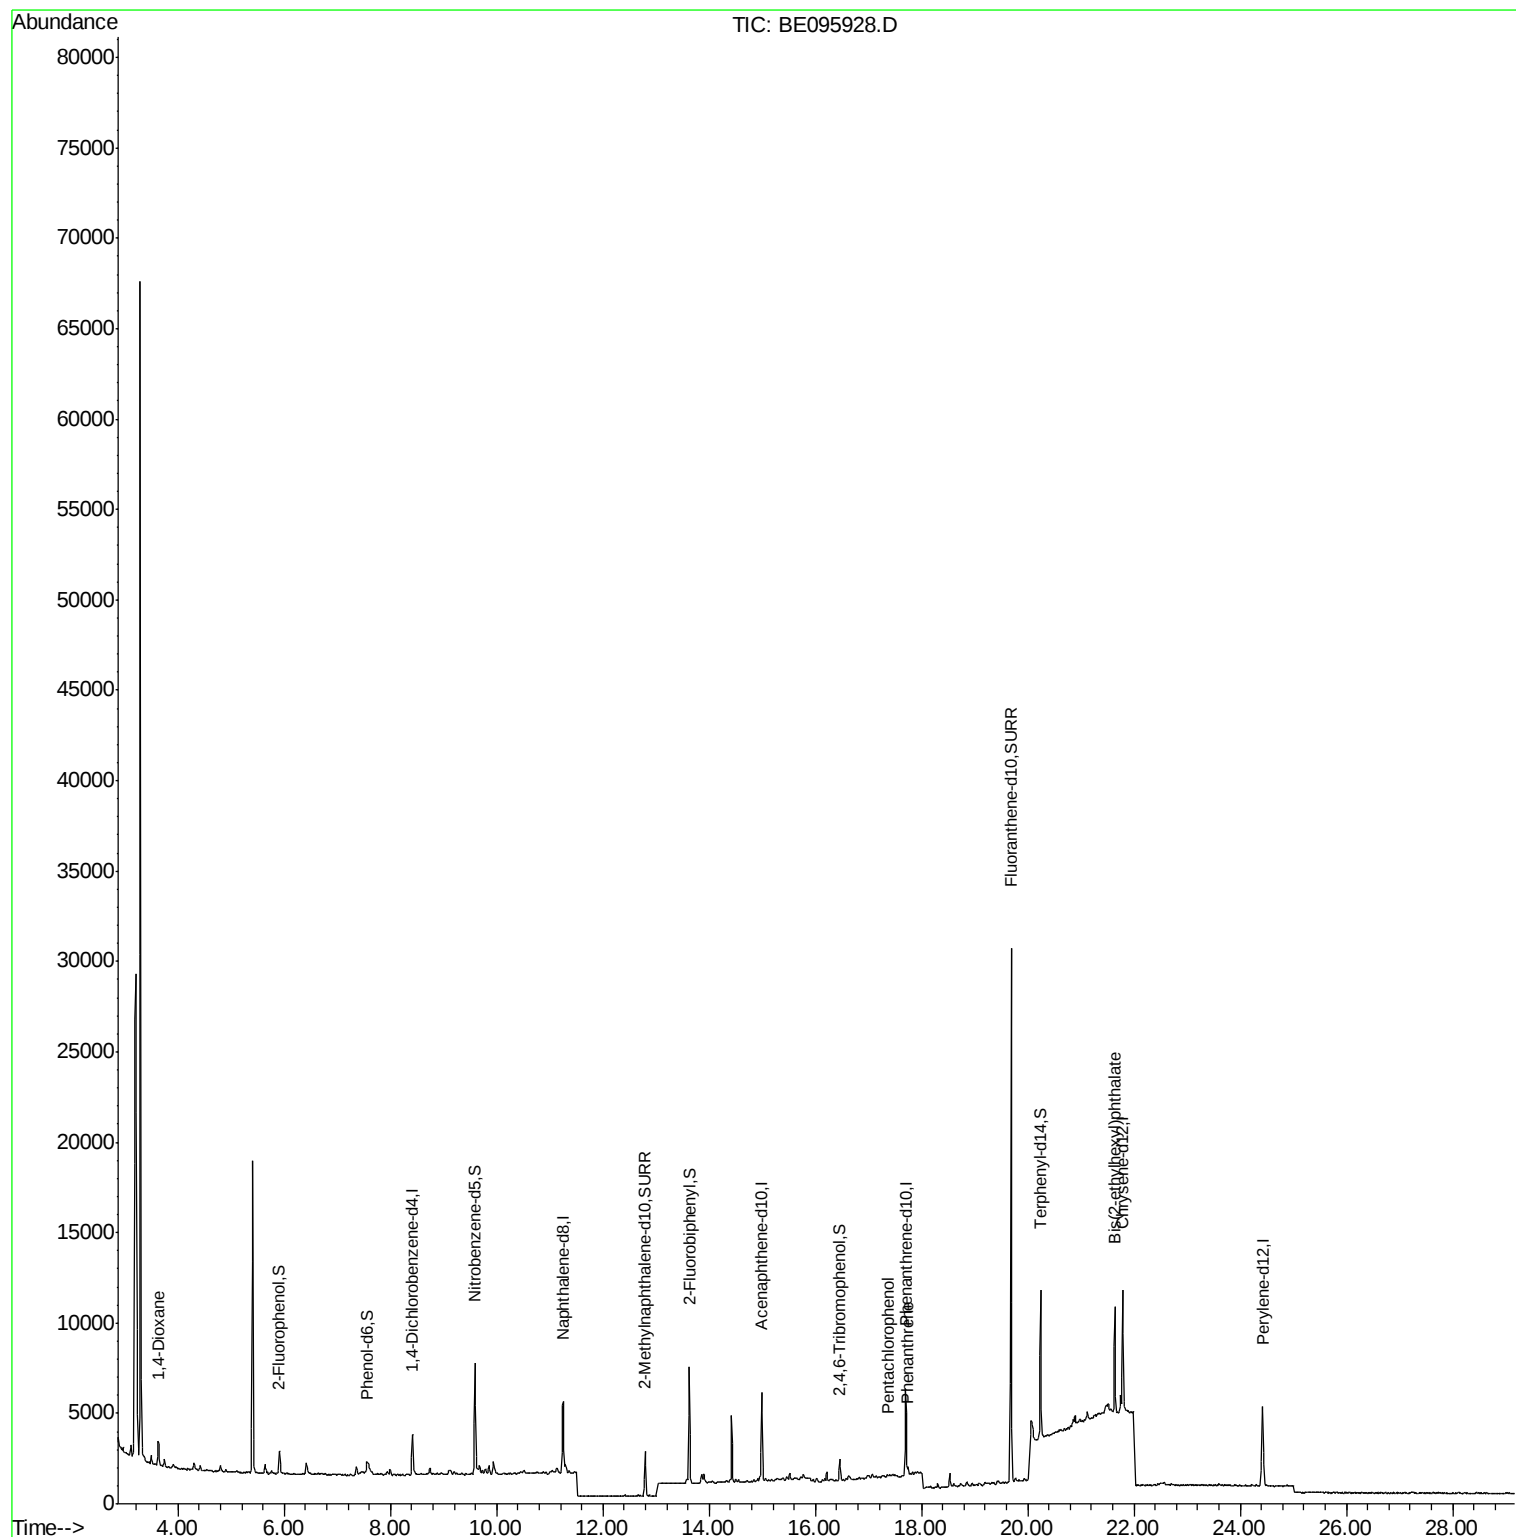

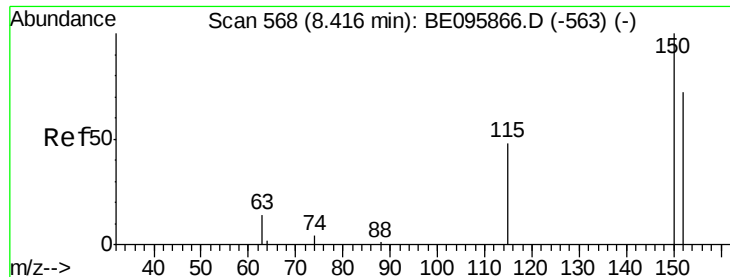


#1


1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.42 min Scan# 568
Delta R.T. -0.01 min
Lab File: BE095928.D
Acq: 2 Apr 2018 15:33

Instrument :
BNA_E
ClientSampled :



Tot Ion:152 Resp: 1179
Ion Ratio Lower Upper
152 100
150 146.6 117.2 175.8
115 67.3 57.0 85.6

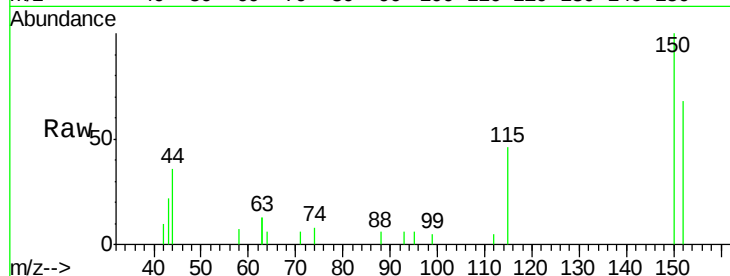

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

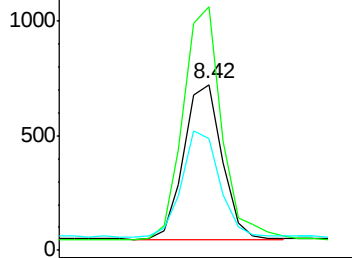


Time-->

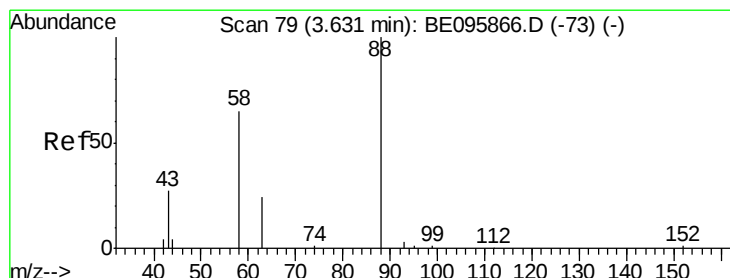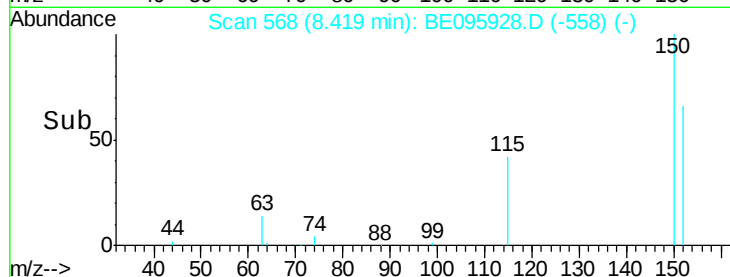


#2

1,4-Dioxane
Concen: 0.461 ng
RT: 3.63 min Scan# 79
Delta R.T. 0.00 min
Lab File: BE095928.D
Acq: 2 Apr 2018 15:33


Tgt Ion: 88 Resp: 889
Ion Ratio Lower Upper
88 100
58 81.4 63.2 94.8
43 60.4 41.2 61.8

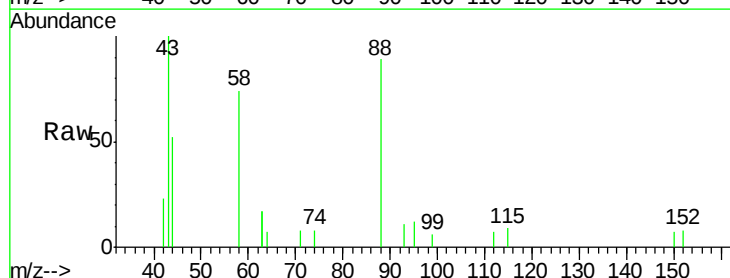


Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

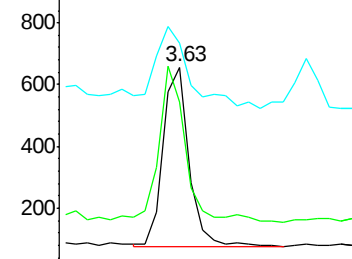

Time-->

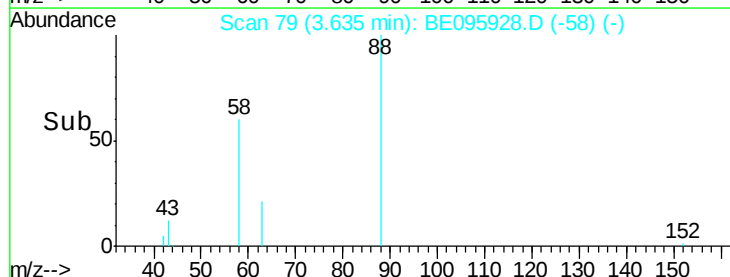

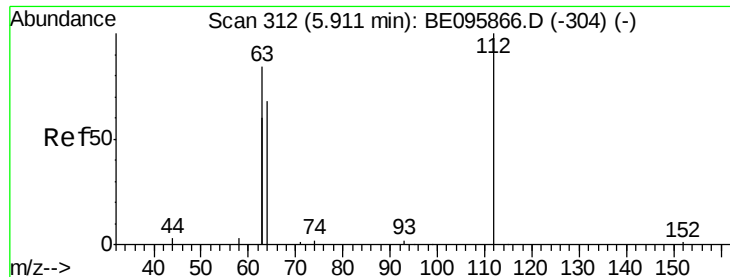

#4

2-Fluorophenol

Concen: 0.158 ng

RT: 5.91 min Scan# 312

Delta R.T. -0.01 min

Lab File: BE095928.D

Acq: 2 Apr 2018 15:33

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 112 Resp: 616

Ion Ratio Lower Upper

112 100

64 79.7 60.1 90.1




63 173.4 116.8 175.2

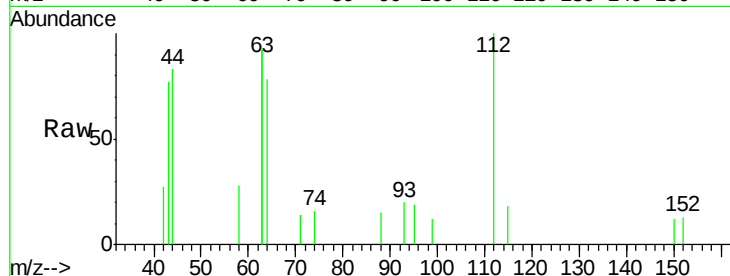

Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

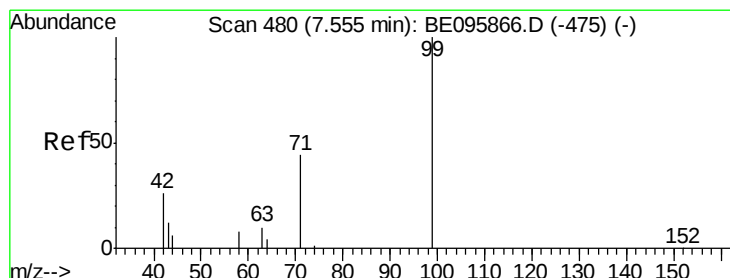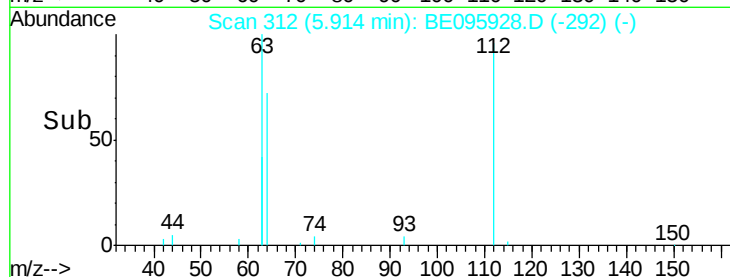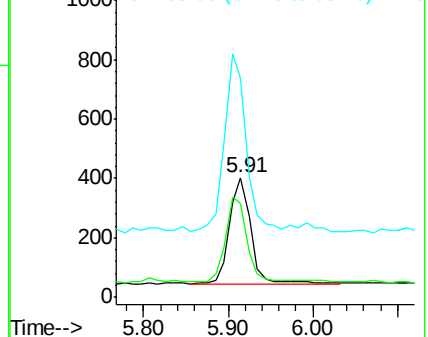

#5

Phenol-d6

Concen: 0.097 ng

RT: 7.56 min Scan# 480

Delta R.T. -0.01 min

Lab File: BE095928.D

Acq: 2 Apr 2018 15:33


Tgt Ion: 99 Resp: 518

Ion Ratio Lower Upper

99 100

42 29.2 20.2 30.2



71 51.4 28.4 42.6#

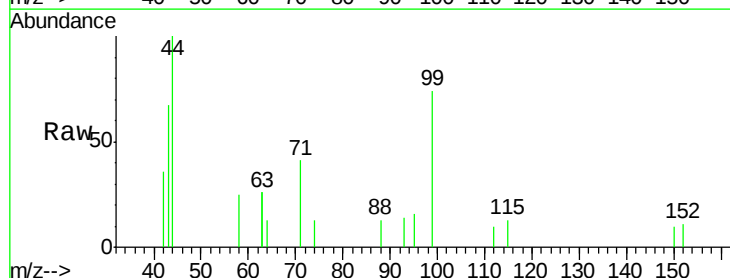


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

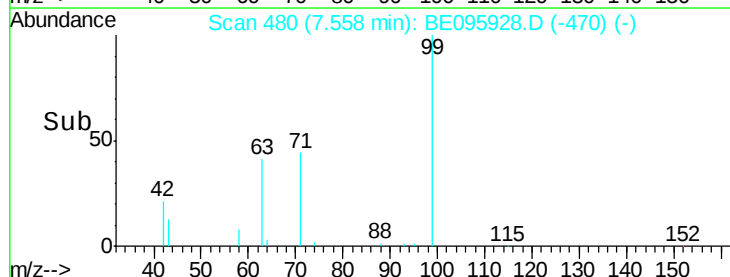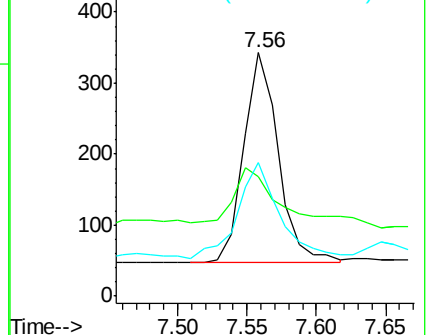

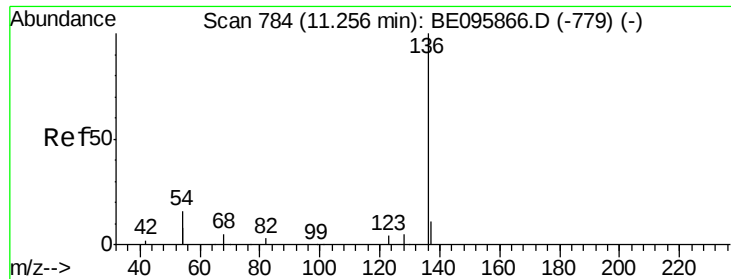

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 11.26 min Scan# 784

Delta R.T. -0.00 min

Lab File: BE095928.D

Acq: 2 Apr 2018 15:33

Instrument :

BNA_E

ClientSampleId :

Tot Ion:136 Resp: 4787


Ion Ratio Lower Upper

136 100

137 12.5 9.5 14.3

54 32.5 29.1 43.7

68 7.3 6.2 9.2



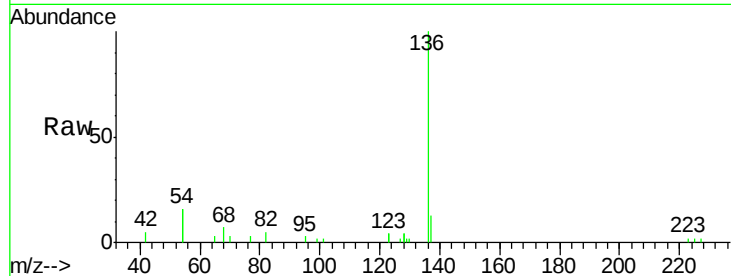


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

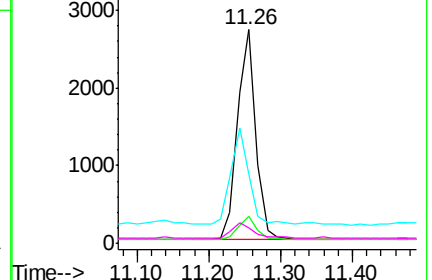

#8

Nitrobenzene-d5

Concen: 0.404 ng

RT: 9.59 min Scan# 656

Delta R.T. -0.00 min

Lab File: BE095928.D

Acq: 2 Apr 2018 15:33


Tgt Ion: 82 Resp: 2282

Ion Ratio Lower Upper

82 100

128 123.5 150.0 225.0#



54 240.7 154.2 231.4#




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

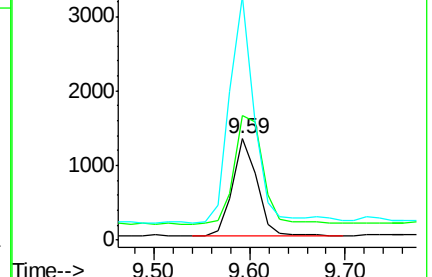


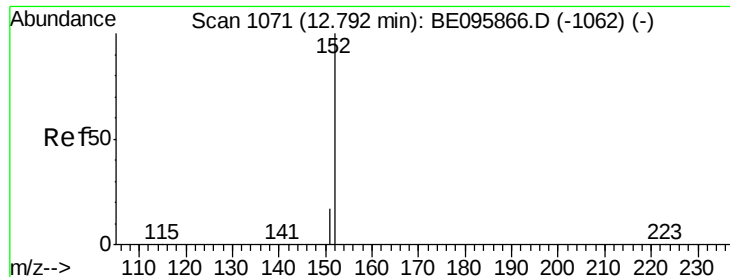




#11
2-Methylnaphthalene-d10
Concen: 0.402 ng
RT: 12.79 min Scan# 1071
Delta R.T. -0.01 min
Lab File: BE095928.D
Acq: 2 Apr 2018 15:33

Instrument :
BNA_E
ClientSampled :

Tot Ion:152 Resp: 3210
Ion Ratio Lower Upper
152 100
151 20.4 15.4 23.0

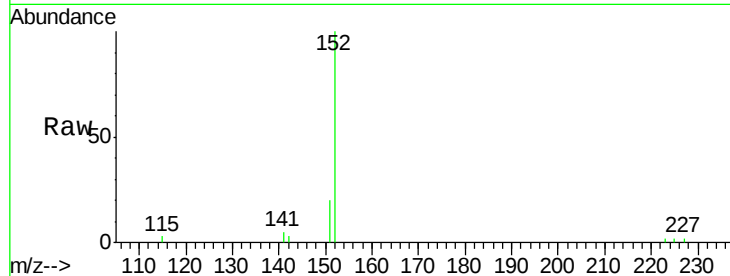


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E

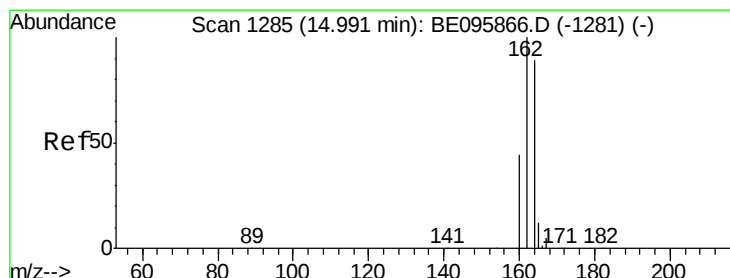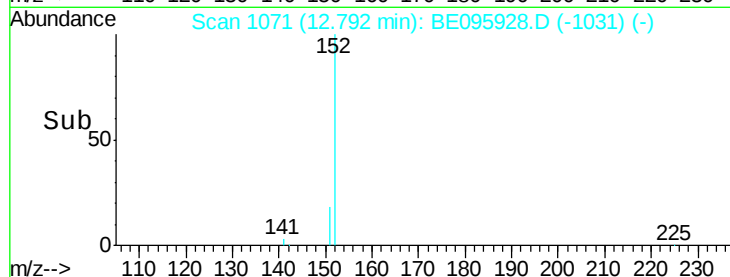
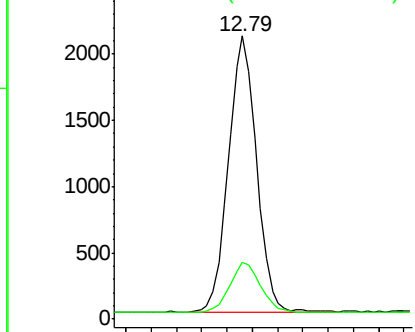



#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.99 min Scan# 1285
Delta R.T. -0.01 min
Lab File: BE095928.D
Acq: 2 Apr 2018 15:33

Tgt Ion:164 Resp: 2776
Ion Ratio Lower Upper
164 100
162 111.9 83.1 124.7
160 50.2 37.1 55.7

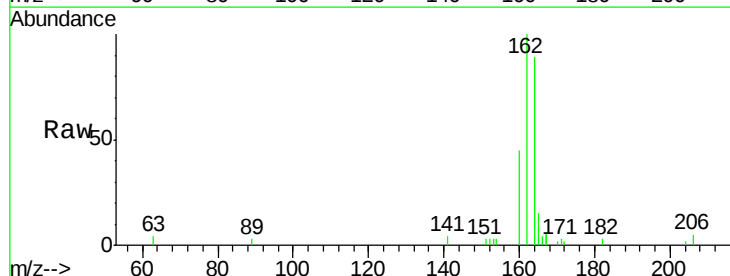

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

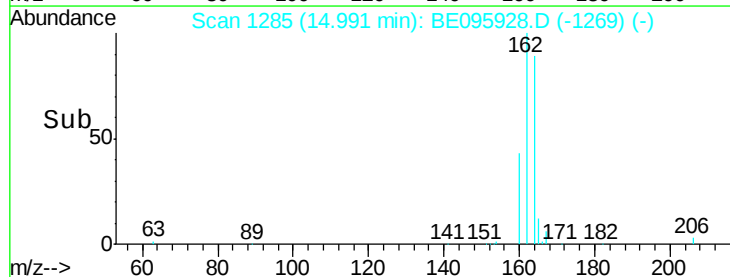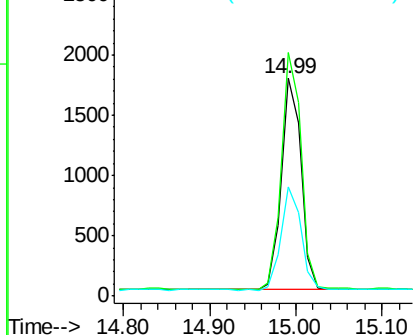







#14
 2,4,6-Tribromophenol
 Concen: 0.401 ng
 RT: 16.46 min Scan# 1408
 Delta R.T. -0.01 min
 Lab File: BE095928.D
 Acq: 2 Apr 2018 15:33

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:330 Resp: 642
 Ion Ratio Lower Upper
 330 100
 332 95.5 152.7 229.1#
 141 52.0 33.7 50.5#

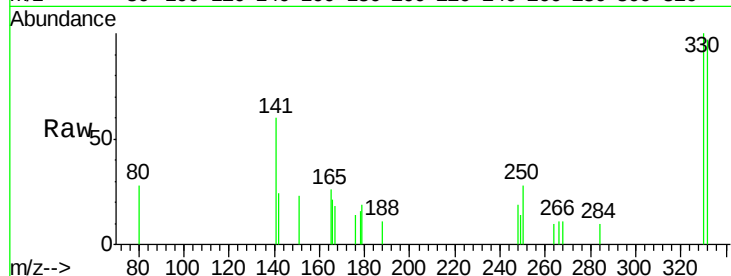


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


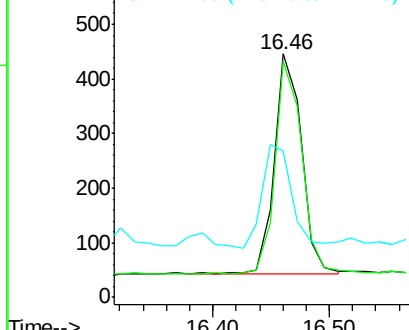



#15
 2-Fluorobiphenyl
 Concen: 0.465 ng
 RT: 13.63 min Scan# 1167
 Delta R.T. -0.01 min
 Lab File: BE095928.D
 Acq: 2 Apr 2018 15:33

Tgt Ion:172 Resp: 5442
 Ion Ratio Lower Upper
 172 100
 171 35.1 29.9 44.9
 170 22.9 21.8 32.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

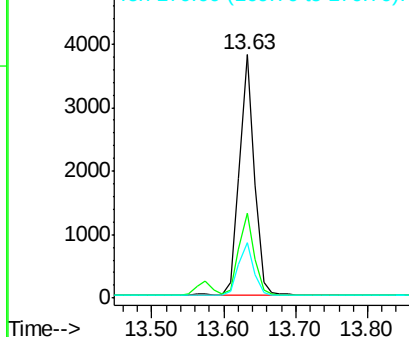



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.70 min Scan# 1514

Delta R.T. -0.01 min

Lab File: BE095928.D

Acq: 2 Apr 2018 15:33

Instrument :

BNA_E

ClientSampleId :


Tot Ion:188 Resp: 6455

Ion Ratio Lower Upper

188 100

94 0.0 3.9 5.9#




80 15.8 3.6 5.4#

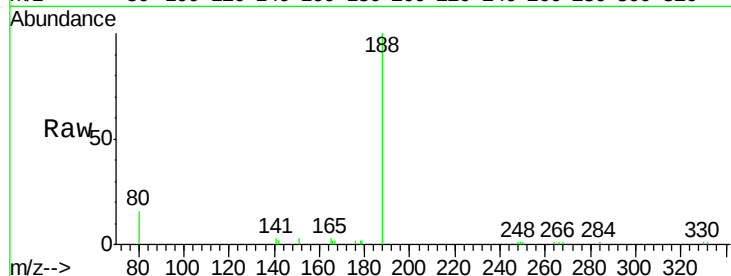

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

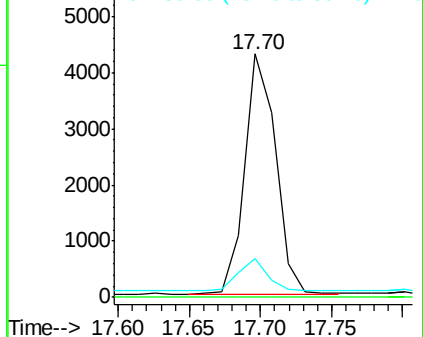

#22

Pentachlorophenol

Concen: 0.162 ng

RT: 17.36 min Scan# 1485

Delta R.T. -0.01 min

Lab File: BE095928.D

Acq: 2 Apr 2018 15:33


Tgt Ion:266 Resp: 46

Ion Ratio Lower Upper

266 100

264 82.9 72.5 108.7



268 84.3 73.8 110.6




Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

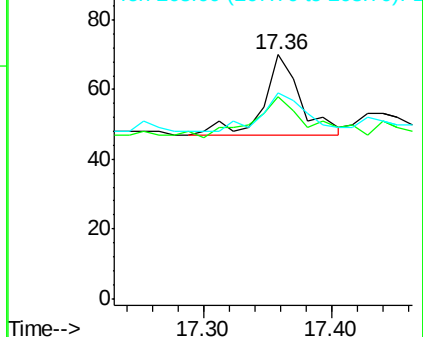

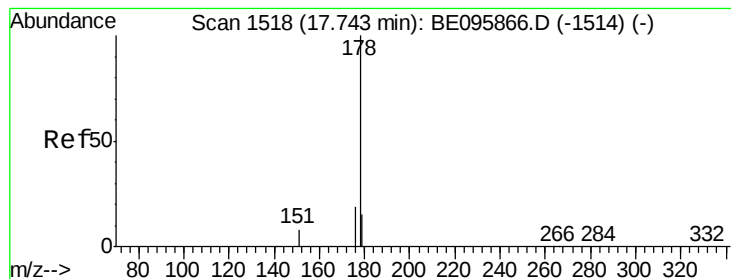

#23

Phenanthrene

Concen: 0.026 ng

RT: 17.74 min Scan# 1518

Delta R.T. -0.00 min

Lab File: BE095928.D

Acq: 2 Apr 2018 15:33

Instrument :

BNA_E

ClientSampleId :


Tot Ion:178 Resp: 498

Ion Ratio Lower Upper

178 100

176 23.1 15.1 22.7#




179 26.7 11.8 17.6#



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

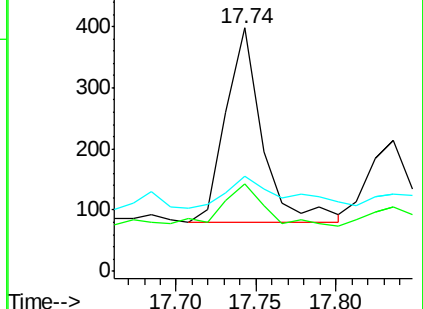

#25

Fluoranthene-d10

Concen: 0.381 ng

RT: 19.68 min Scan# 1828

Delta R.T. -0.01 min

Lab File: BE095928.D

Acq: 2 Apr 2018 15:33


Tgt Ion:212 Resp: 36530

Ion Ratio Lower Upper

212 100

106 3.1 2.8 4.2



104 1.8 1.6 2.4




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

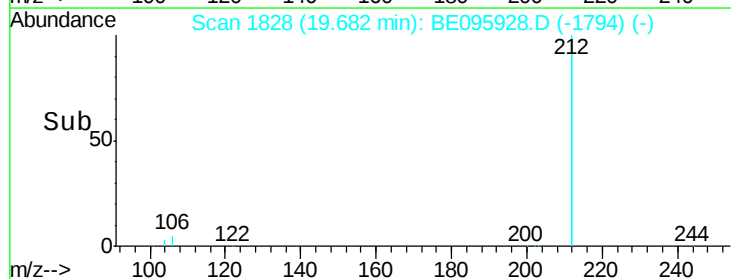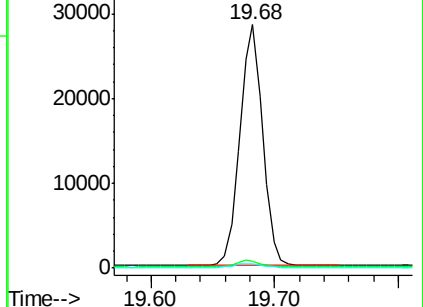



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.79 min Scan# 2028

Delta R.T. -0.01 min

Lab File: BE095928.D

Acq: 2 Apr 2018 15:33

Instrument :

BNA_E

ClientSampleId :


Tot Ion:240 Resp: 6918

Ion Ratio Lower Upper

240 100

120 13.8 5.5 8.3#




236 28.5 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

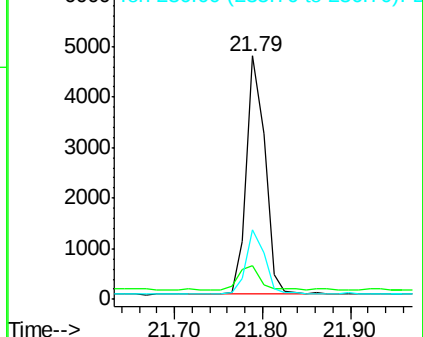

#29

Terphenyl-d14

Concen: 0.505 ng

RT: 20.24 min Scan# 1900

Delta R.T. -0.00 min

Lab File: BE095928.D

Acq: 2 Apr 2018 15:33


Tgt Ion:244 Resp: 7426

Ion Ratio Lower Upper

244 100

212 8.7 25.4 38.0#



122 7.7 8.1 12.1#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

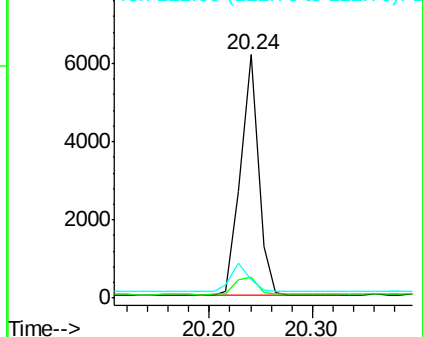



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.101 ng

RT: 21.64 min Scan# 2016

Delta R.T. -0.00 min

Lab File: BE095928.D

Acq: 2 Apr 2018 15:33

Instrument :

BNA_E

ClientSampleId :


Tot Ion:149 Resp: 7411

Ion Ratio Lower Upper

149 100

167 6.2 5.4 8.0




279 0.8 0.7 1.1



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

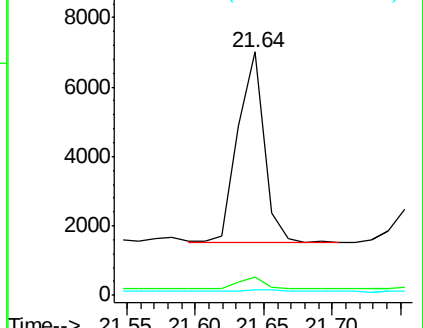

#34

Perylene-d12

Concen: 0.400 ng

RT: 24.42 min Scan# 2717

Delta R.T. -0.01 min

Lab File: BE095928.D

Acq: 2 Apr 2018 15:33


Tgt Ion:264 Resp: 6805

Ion Ratio Lower Upper

264 100

260 26.2 20.5 30.7

265 29.6 22.8 34.2



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

