
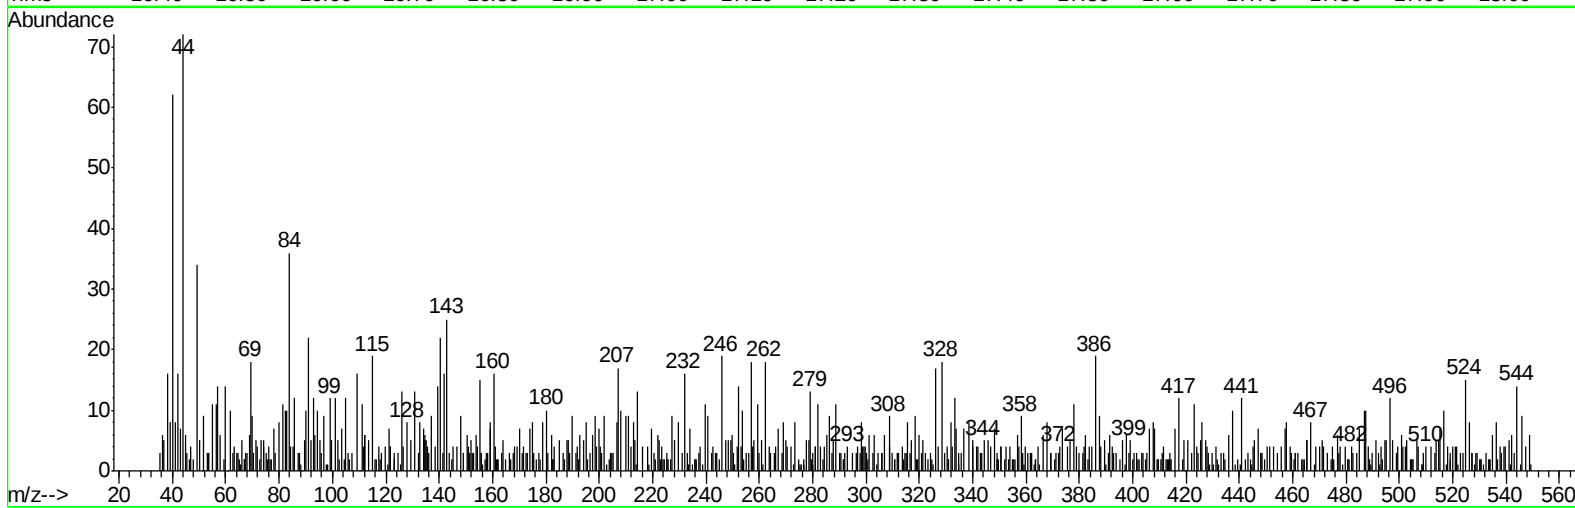


Data Path : Z:\HPCHEM1\BNA E\DATA\BE040218\
Data File : BE095918.D
Acq On : 2 Apr 2018 9:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 05:11:50 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 02 13:40:00 2018
Response via : Initial Calibration

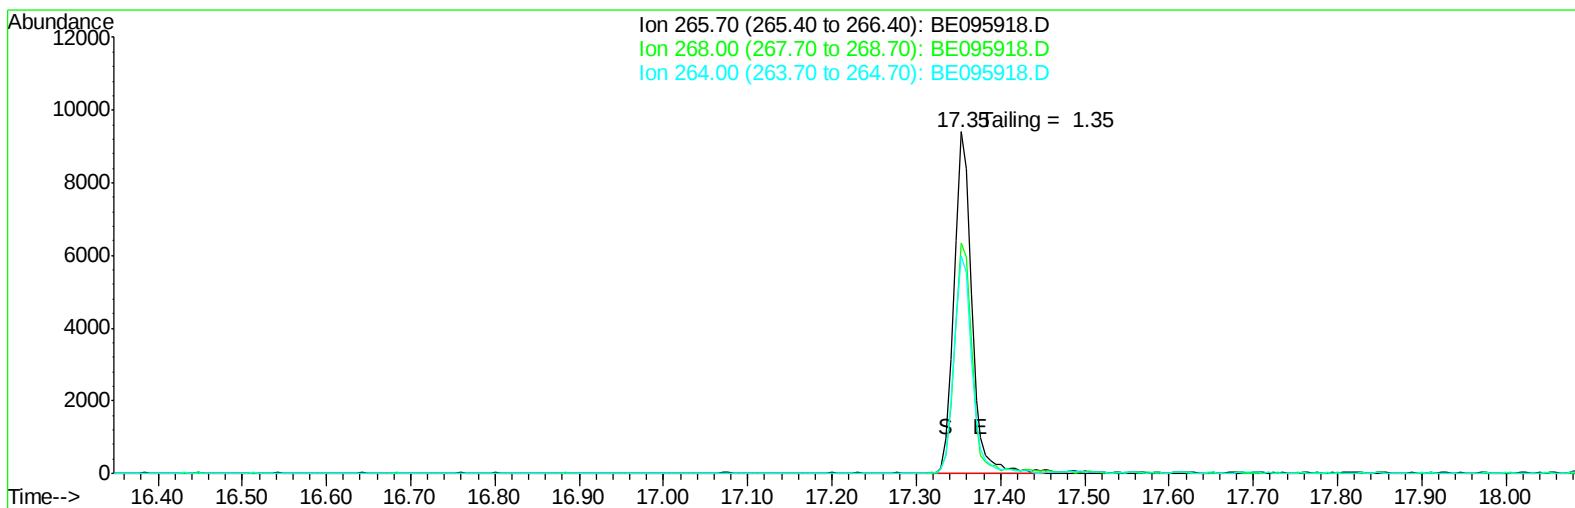

(69) Pentachlorophenol (C)



11.372min (+0.074) 28.58ng

response 6

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	42.86#
264.00	61.90	42.86#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE040218\
Data File : BE095918.D
Acq On : 2 Apr 2018 9:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 05:11:50 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 02 13:40:00 2018
Response via : Initial Calibration

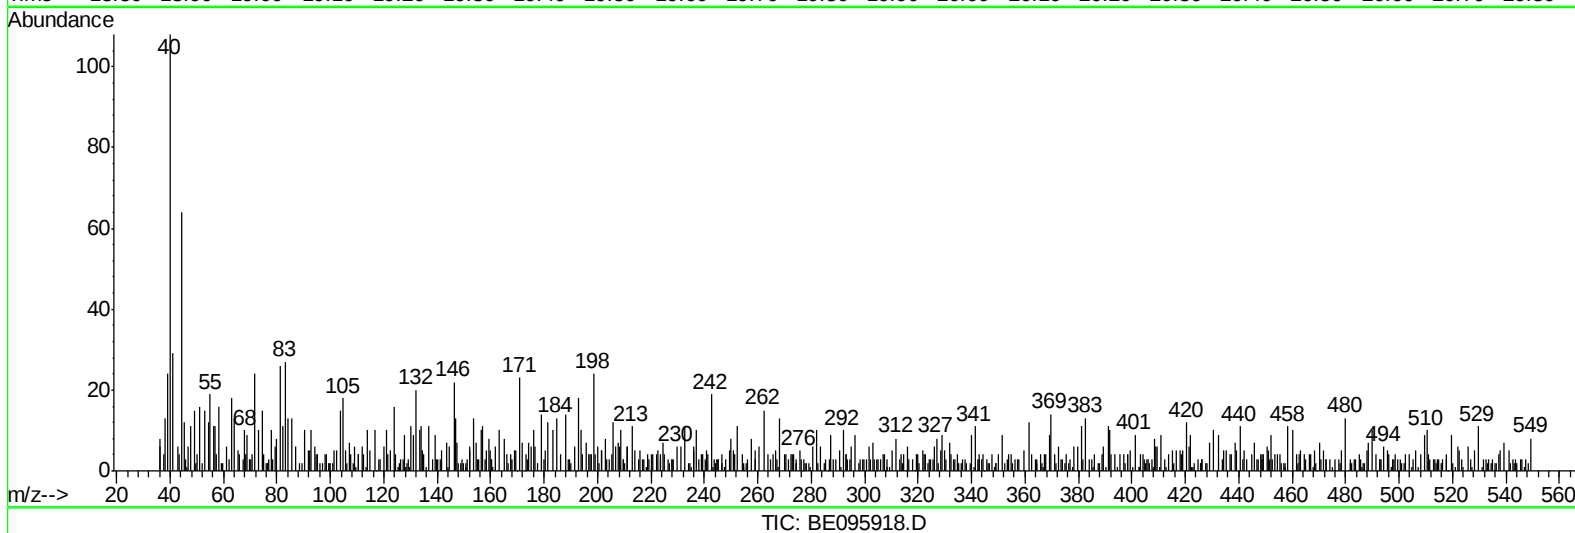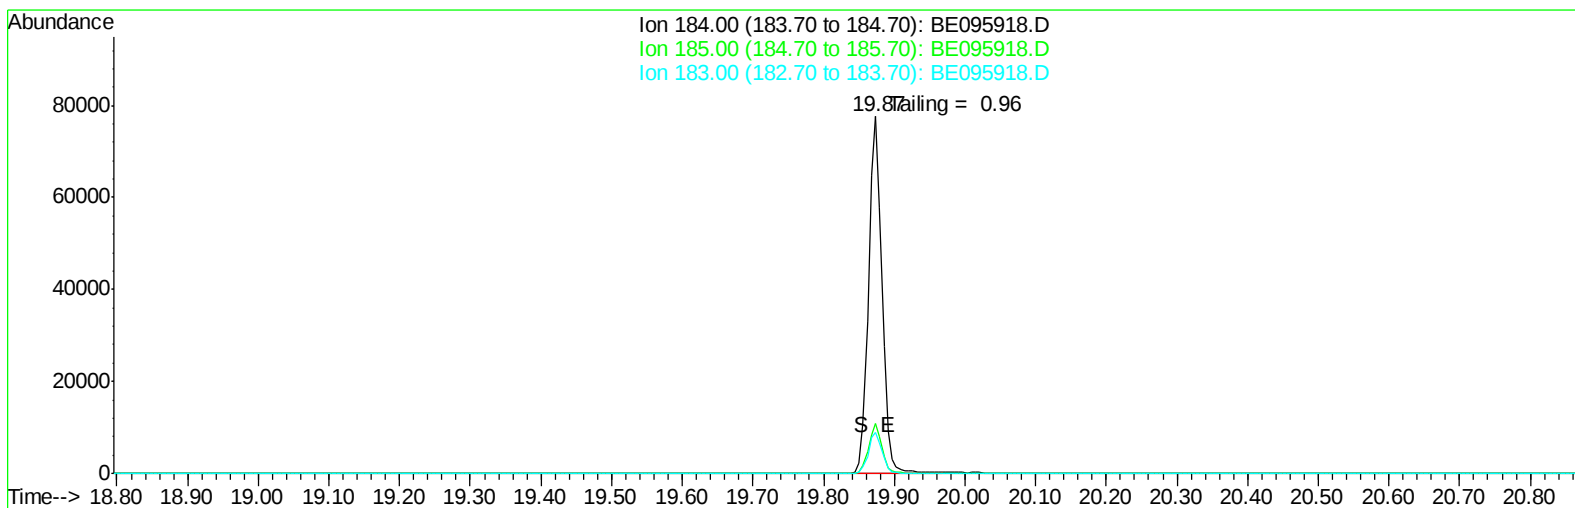

(76) Benzidine

12.917min (+0.078) 38.01ng

response 13

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	0.00#
183.00	11.60	76.92#
0.00	0.00	0.00