


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA E\Data\BE040218\
 Data File : BE095918.D
 Acq On : 2 Apr 2018 9:36
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 23 12:41:11 2018

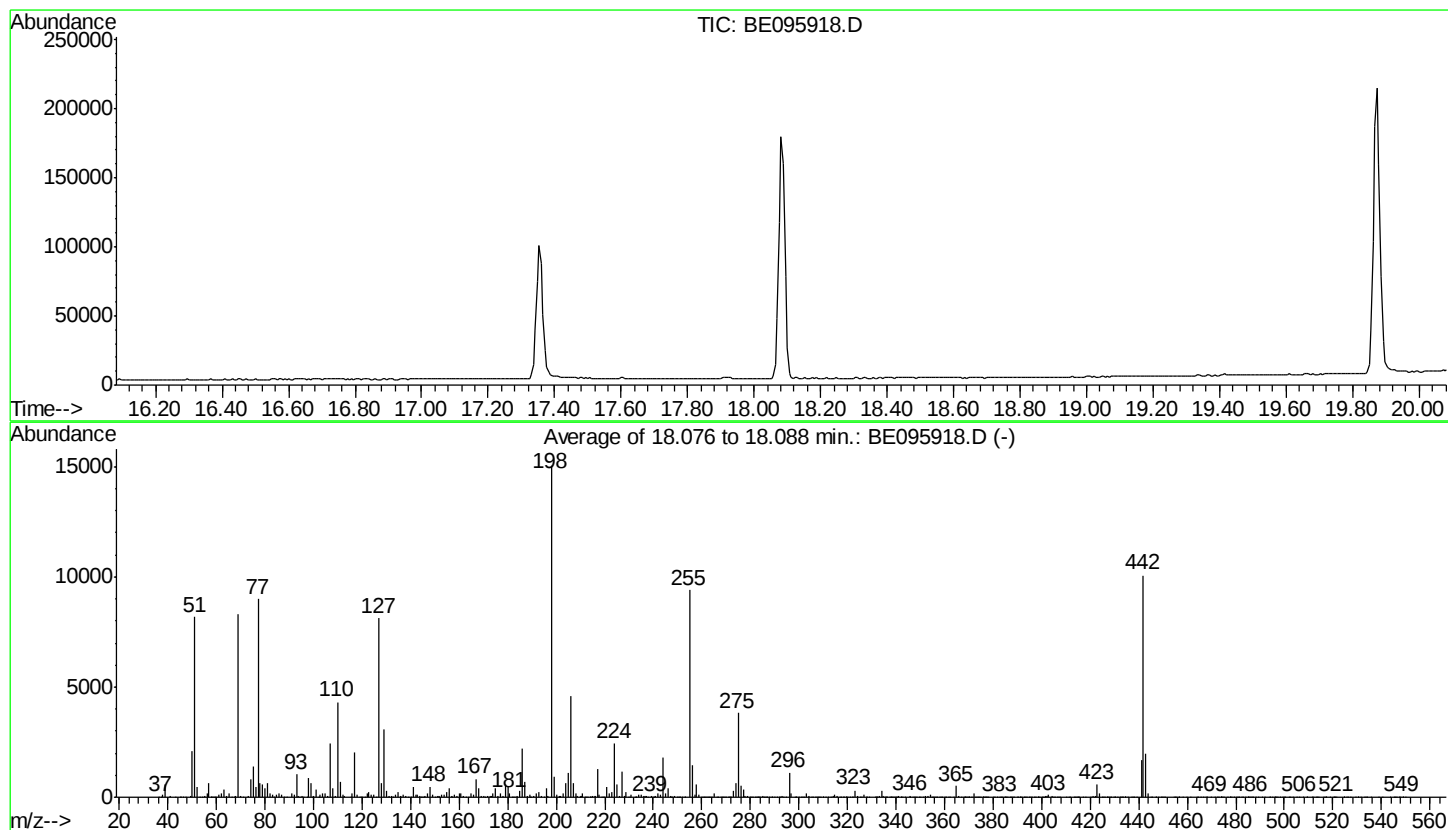

AutoFind: Scans 2636, 2637, 2638; Background Corrected with Scan 2630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.3	8168	PASS
68	69	0.00	2	0.4	31	PASS
69	198	0.00	100	55.2	8307	PASS
70	69	0.00	2	0.5	40	PASS
127	198	10	80	53.9	8107	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	15045	PASS
199	198	5	9	6.2	940	PASS
275	198	10	60	25.4	3818	PASS
365	198	1	100	3.4	514	PASS
441	443	0.01	100	84.2	1668	PASS
442	198	50	100	67.0	10073	PASS
443	442	15	24	19.7	1980	PASS