
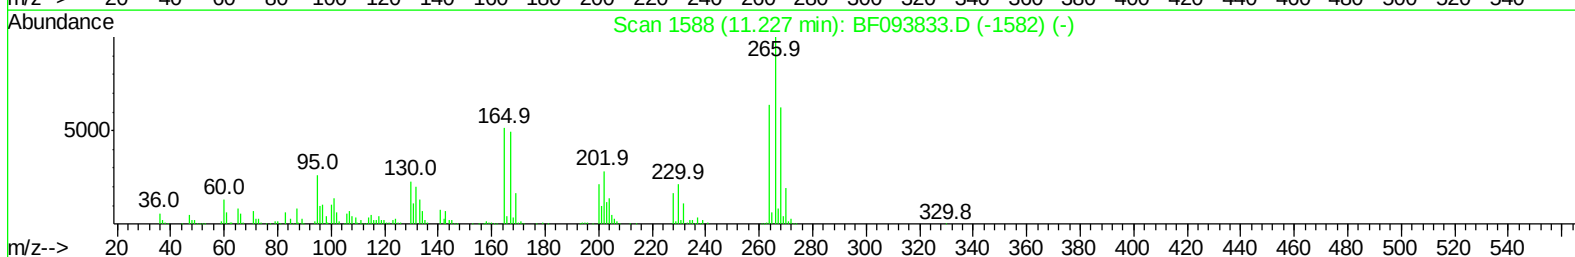
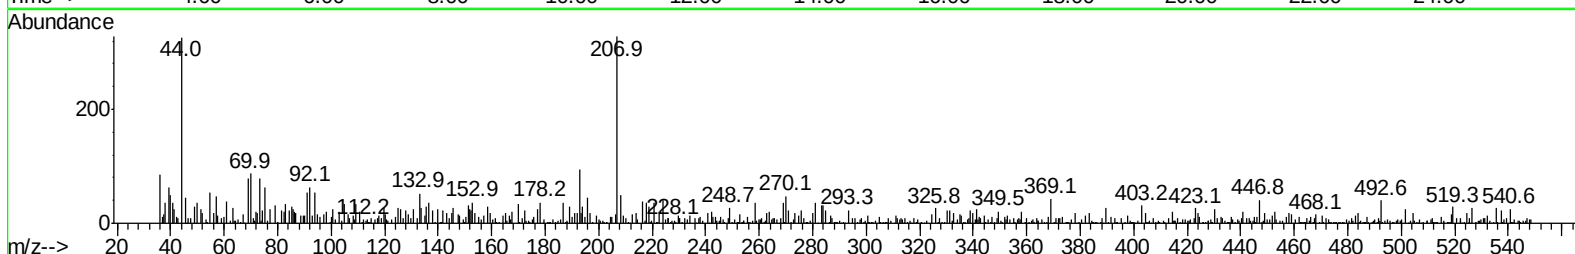


Data Path : Z:\HPCHEM1\BNA E\Data\BE040417\  
Data File : BE092877.D  
Acq On : 4 Apr 2017 10:18  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 14:00:41 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 31 14:38:29 2017  
Response via : Initial Calibration

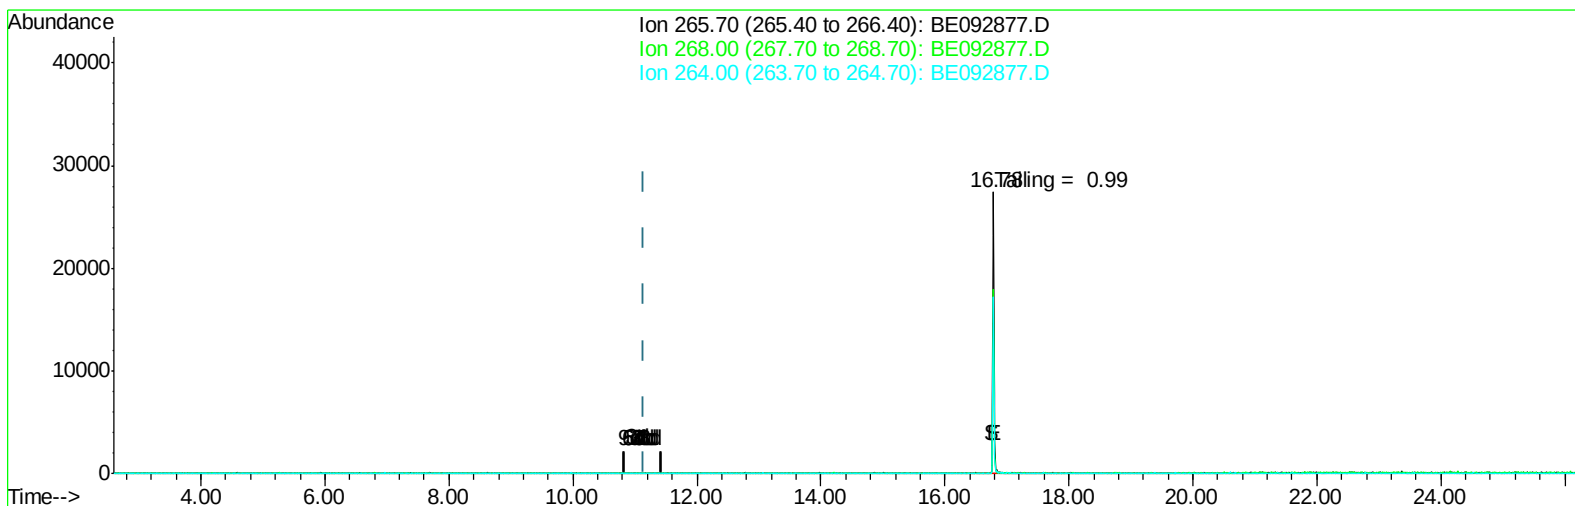




TIC: BE092877.D

(69) Pentachlorophenol (C)  
11.072min (-0.073) 119.11ng  
response 31

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 265.70 | 100   | 100     |
| 268.00 | 63.90 | 45.00#  |
| 264.00 | 64.60 | 105.00# |
| 0.00   | 0.00  | 0.00    |

Data Path : Z:\HPCHEM1\BNA E\Data\BE040417\  
Data File : BE092877.D  
Acq On : 4 Apr 2017 10:18  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 14:00:41 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 31 14:38:29 2017  
Response via : Initial Calibration

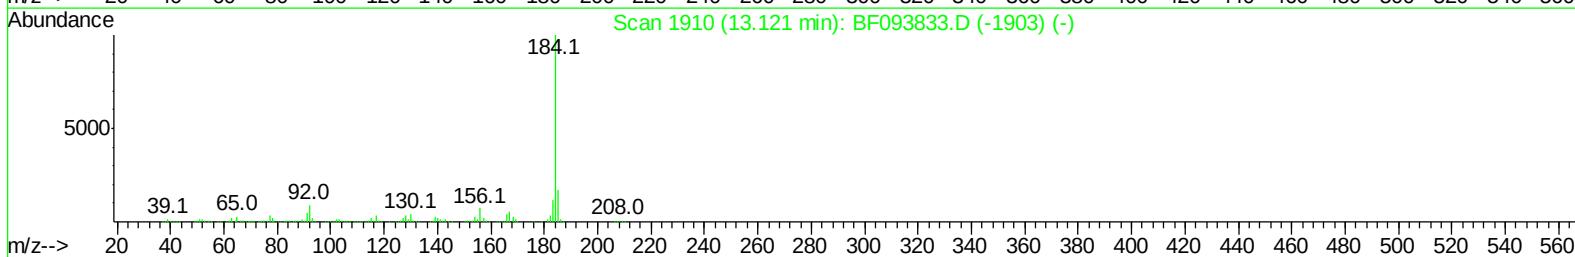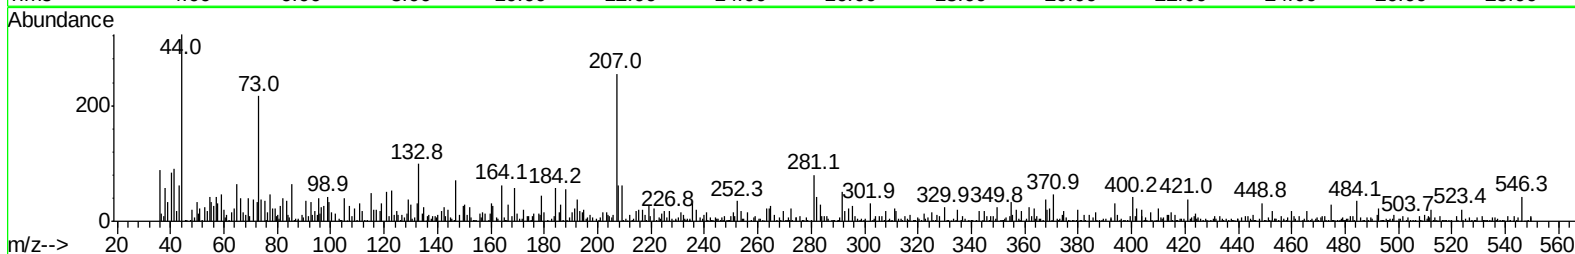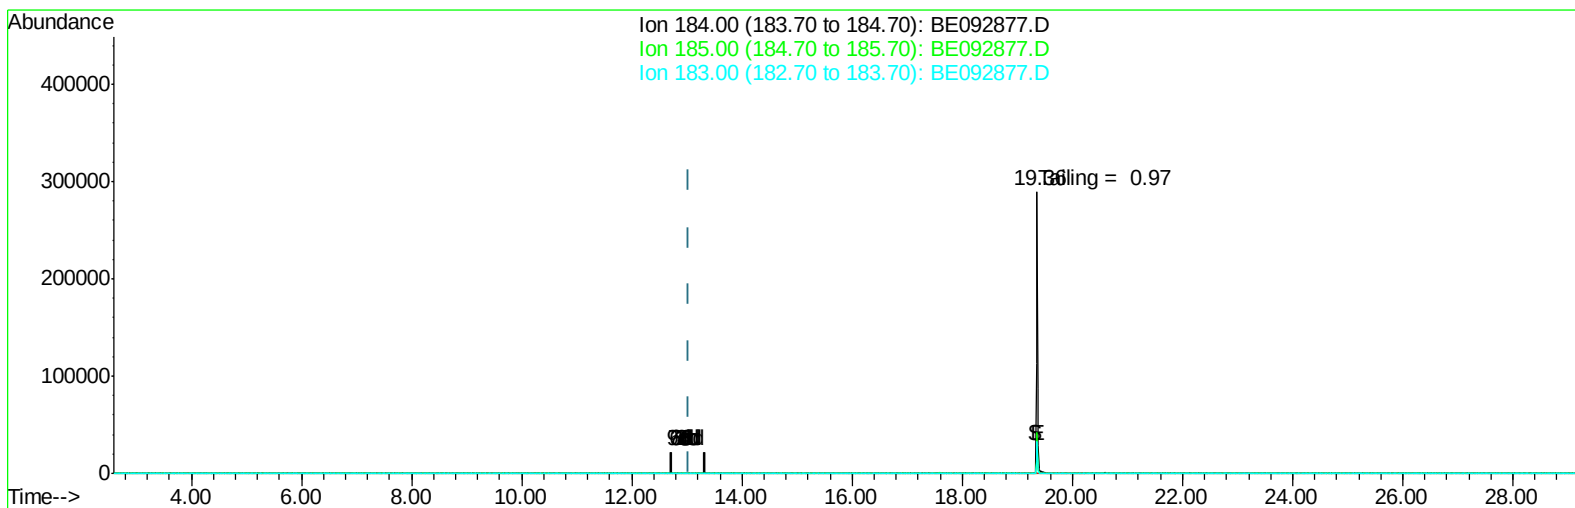

TIC: BE092877.D

(76) Benzidine

13.005min (-0.028) 81.63ng

response 42

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 19.40 | 24.24# |
| 183.00 | 12.20 | 13.64  |
| 0.00   | 0.00  | 0.00   |