


Data Path : Z:\HPCHEM1\BNA E\DATA\BE040417\
 Data File : BE092877.D
 Acq On : 4 Apr 2017 10:18
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE040417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 04 16:35:54 2017

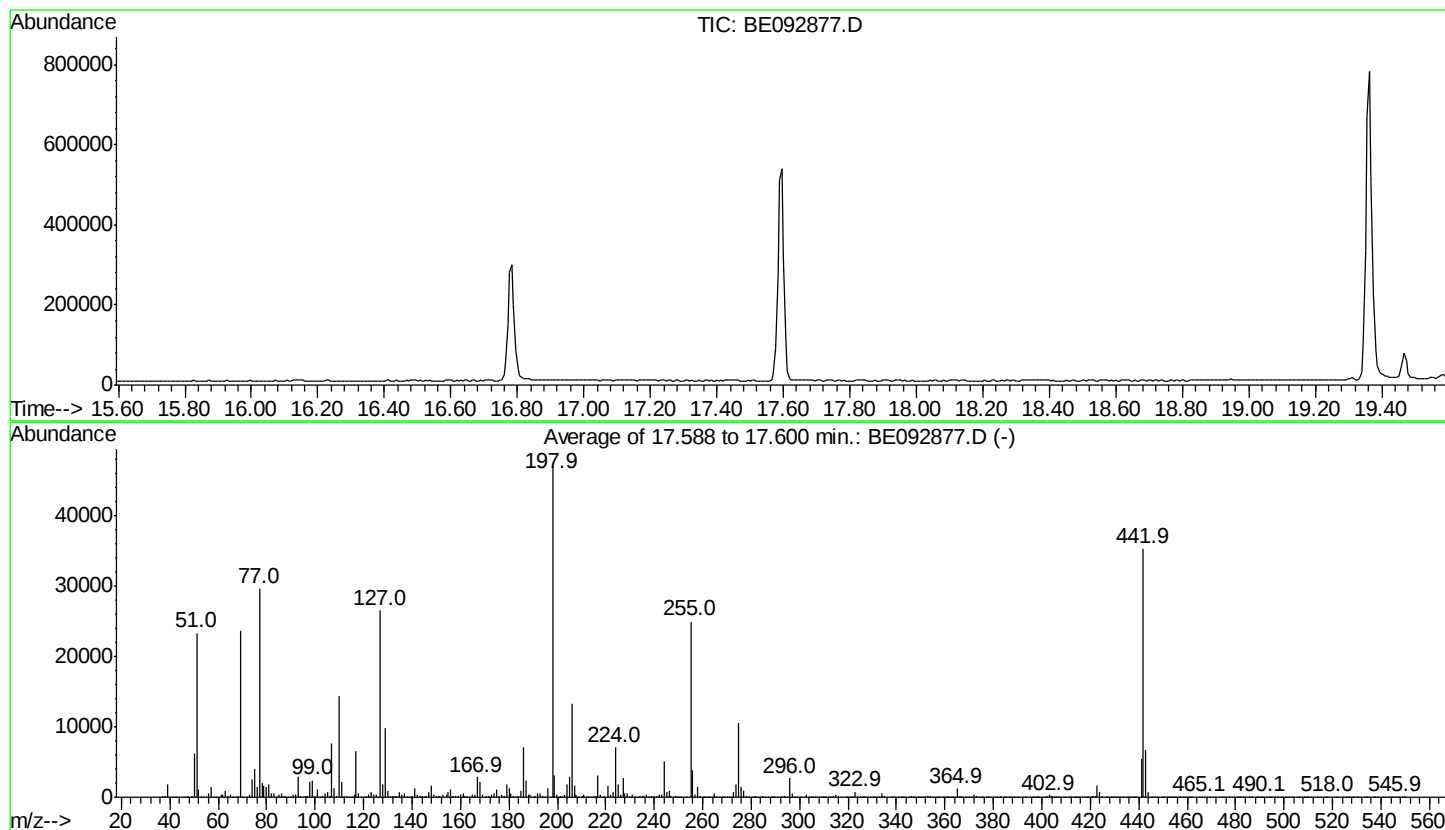

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2545

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.4	23270	PASS
68	69	0.00	2	0.5	124	PASS
69	198	0.00	100	50.3	23705	PASS
70	69	0.00	2	0.3	66	PASS
127	198	10	80	56.3	26516	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47090	PASS
199	198	5	9	6.4	3026	PASS
275	198	10	60	22.4	10549	PASS
365	198	1	100	2.6	1202	PASS
441	442	0.01	24	15.3	5421	PASS
442	198	50	100	75.0	35319	PASS
443	442	15	24	18.8	6652	PASS