
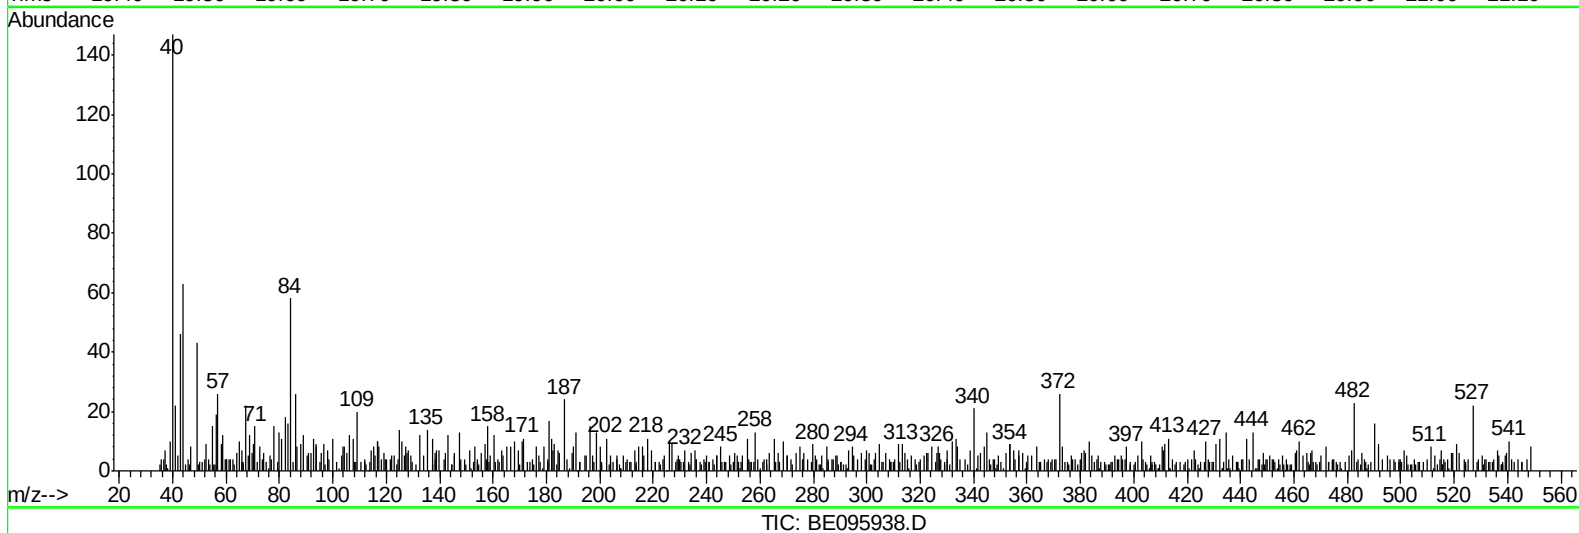


Data Path : Z:\HPCHEM1\BNA E\DATA\BE040418\
Data File : BE095938.D
Acq On : 4 Apr 2018 9:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 04:03:31 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 04 18:06:58 2018
Response via : Initial Calibration

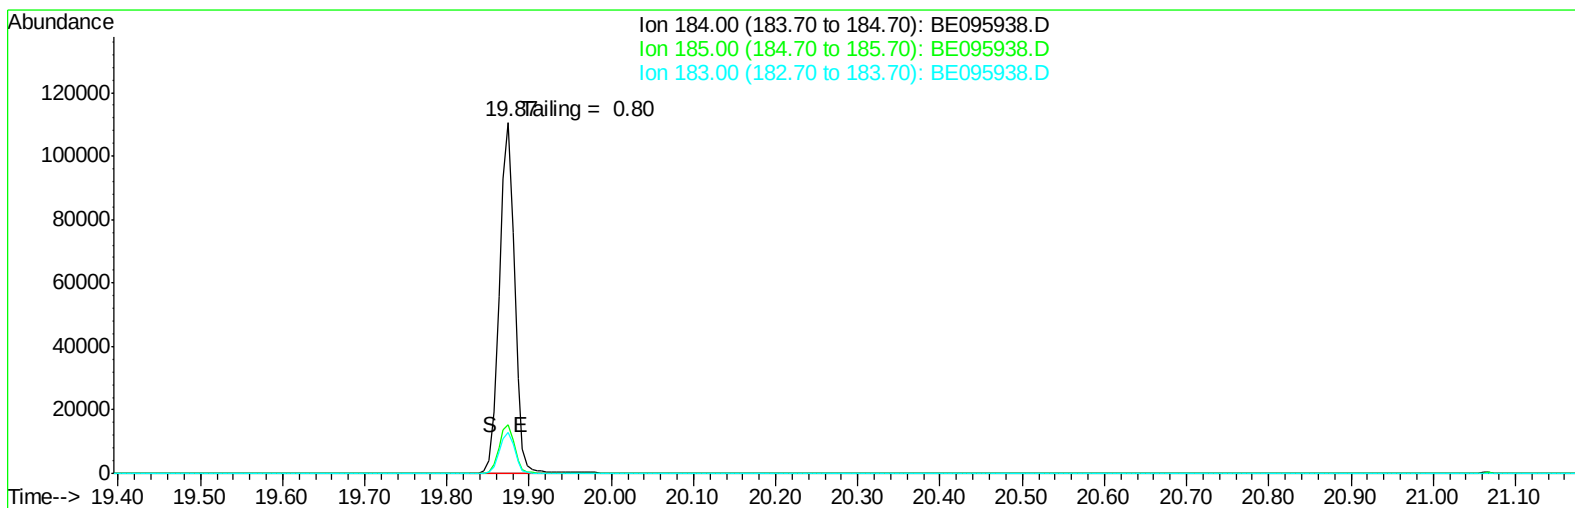

(76) Benzidine



12.953min (+0.114) 21.93ng

response 5

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	66.67#
183.00	11.60	100.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE040418\
Data File : BE095938.D
Acq On : 4 Apr 2018 9:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 04:03:31 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 04 18:06:58 2018
Response via : Initial Calibration

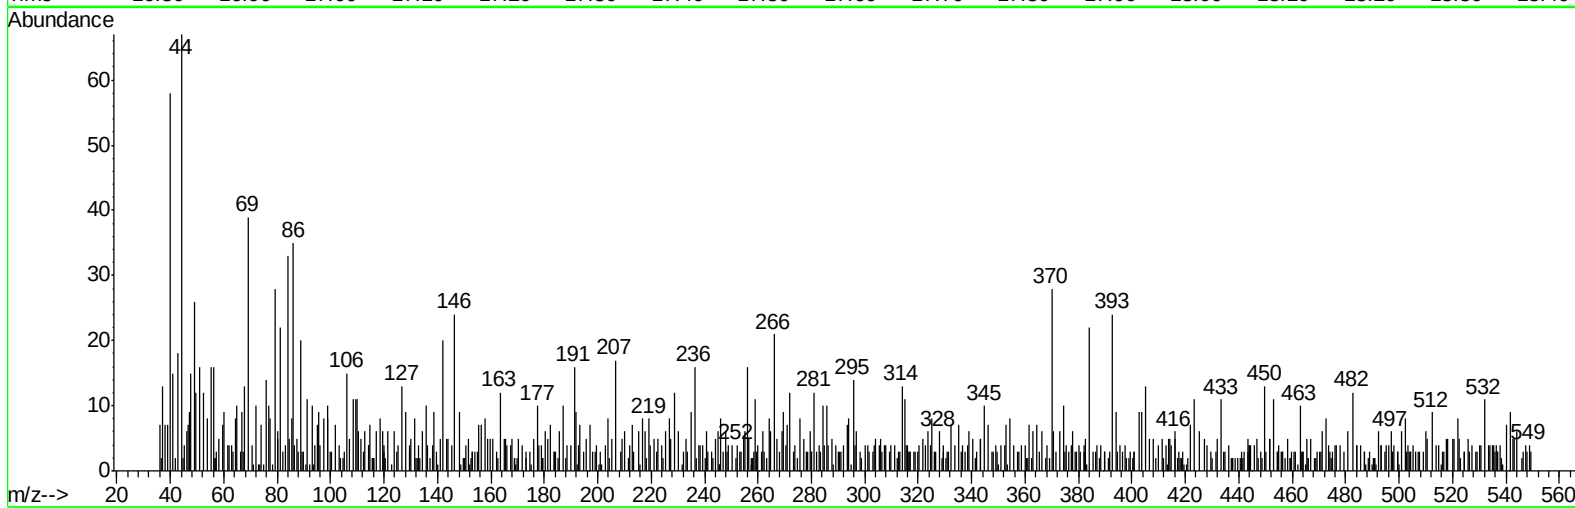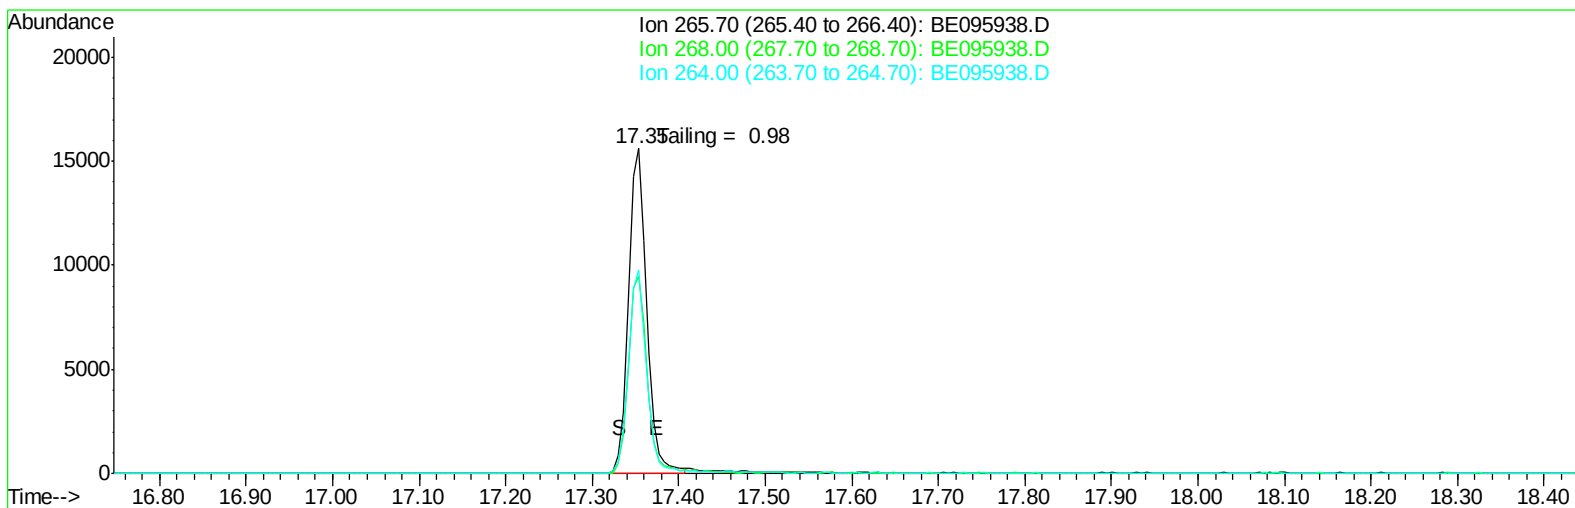

TIC: BE095938.D

(69) Pentachlorophenol (C)

11.390min (+0.098) 255.06ng

response 19

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	14.29#
264.00	61.90	66.67
0.00	0.00	0.00