


Data Path : Z:\HPCHEM1\BNA E\Data\BE040418\
 Data File : BE095938.D
 Acq On : 4 Apr 2018 9:29
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 23 12:41:11 2018

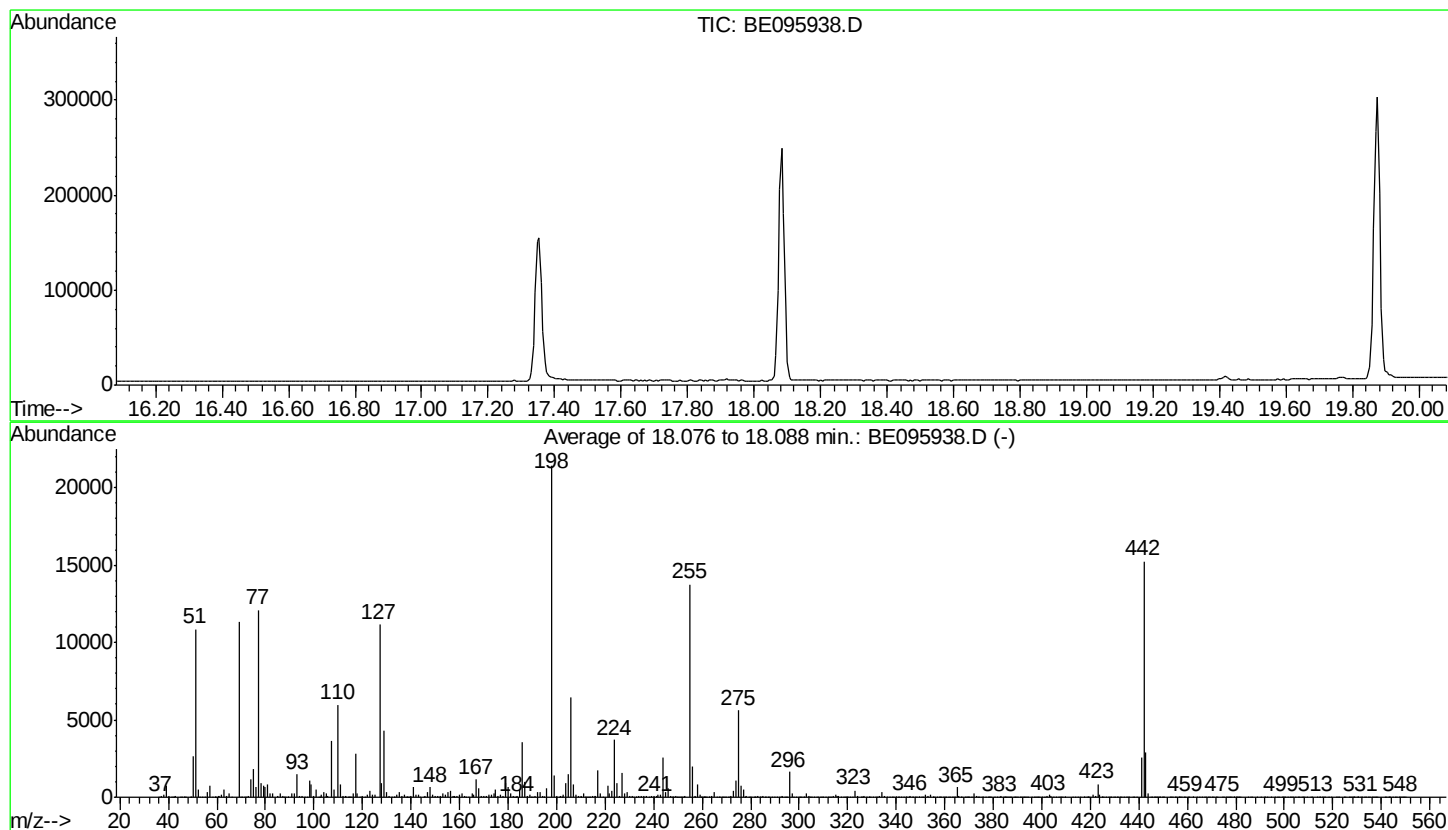

AutoFind: Scans 2636, 2637, 2638; Background Corrected with Scan 2626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.6	10853	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	53.1	11371	PASS
70	69	0.00	2	0.3	36	PASS
127	198	10	80	52.1	11157	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21429	PASS
199	198	5	9	6.6	1421	PASS
275	198	10	60	26.1	5593	PASS
365	198	1	100	3.0	637	PASS
441	443	0.01	100	87.3	2550	PASS
442	198	50	100	71.1	15235	PASS
443	442	15	24	19.2	2921	PASS