


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE040419\
 Data File : BE099292.D
 Acq On : 4 Apr 2019 15:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE040219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 02 17:16:42 2019

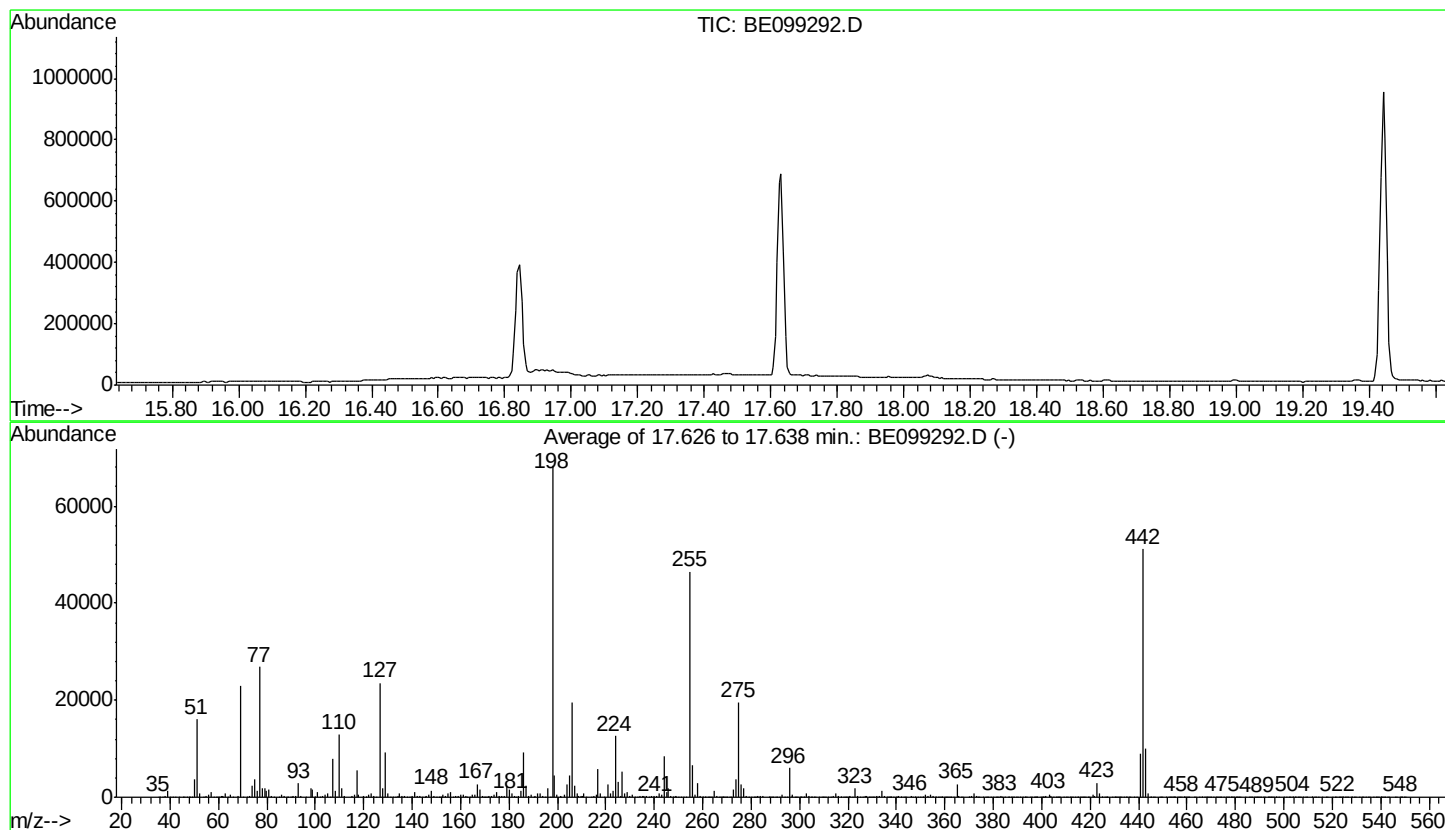

AutoFind: Scans 2559, 2560, 2561; Background Corrected with Scan 2549

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.5	16029	PASS
68	69	0.00	2	1.5	347	PASS
69	198	0.00	100	33.6	22959	PASS
70	69	0.00	2	0.5	120	PASS
127	198	10	80	34.4	23525	PASS
197	198	0.00	2	0.2	120	PASS
198	198	100	100	100.0	68352	PASS
199	198	5	9	6.6	4535	PASS
275	198	10	60	28.4	19433	PASS
365	198	1	100	4.0	2744	PASS
441	198	0.01	100	13.0	8875	PASS
442	198	50	100	74.9	51184	PASS
443	442	15	24	19.5	10002	PASS