
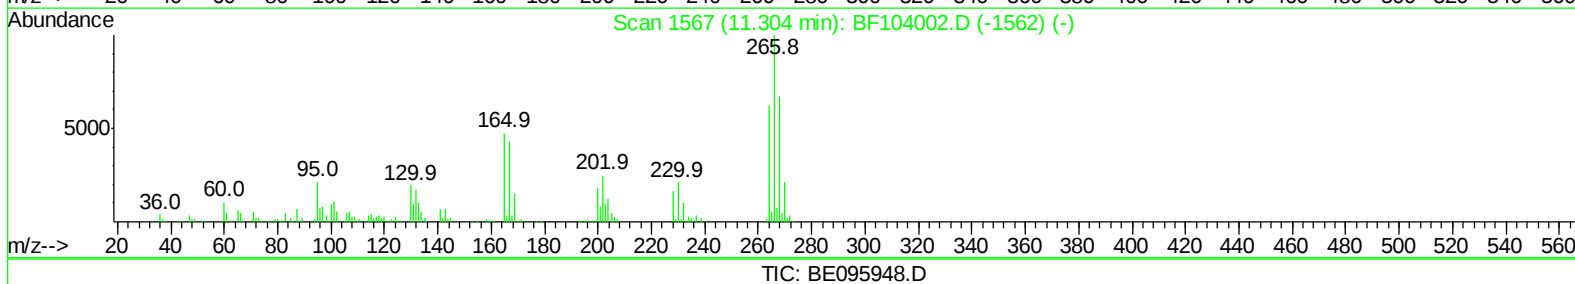
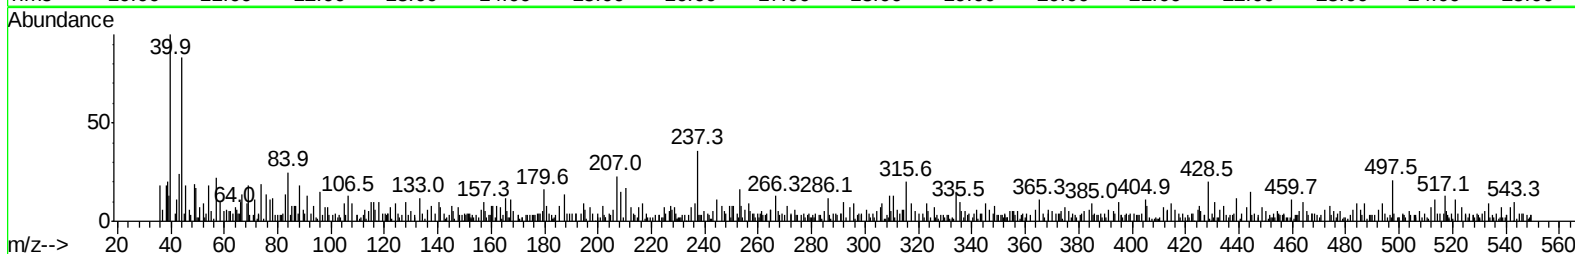


Data Path : Z:\HPCHEM1\BNA E\Data\BE040518\
Data File : BE095948.D
Acq On : 5 Apr 2018 8:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 06:50:06 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 04 18:06:58 2018
Response via : Initial Calibration

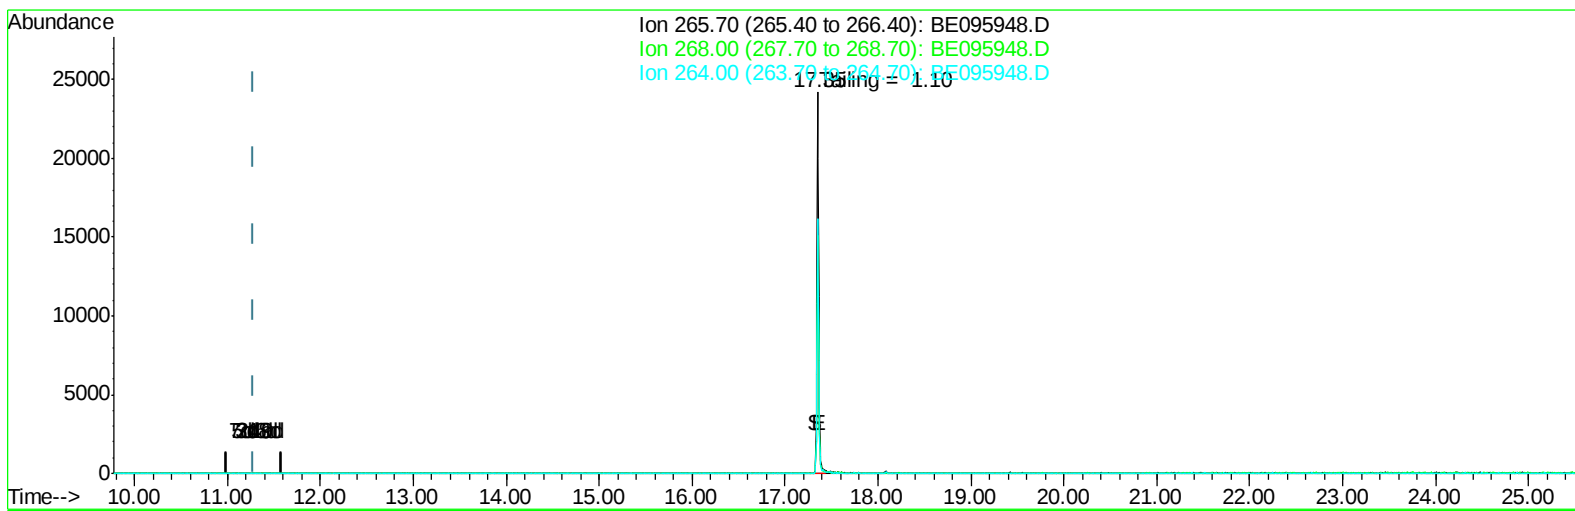

(69) Pentachlorophenol (C)




11.295min (+0.003) 175.35ng

response 19

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	23.08#
264.00	61.90	92.31#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE040518\
Data File : BE095948.D
Acq On : 5 Apr 2018 8:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 06:50:06 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 04 18:06:58 2018
Response via : Initial Calibration

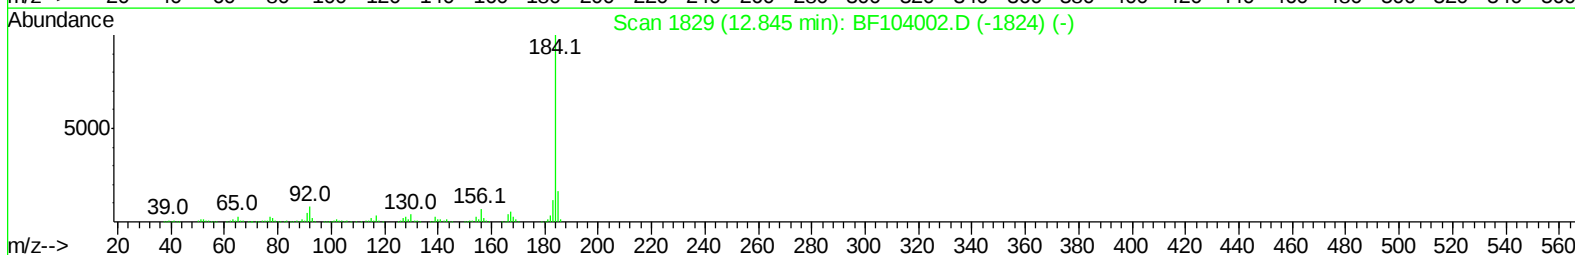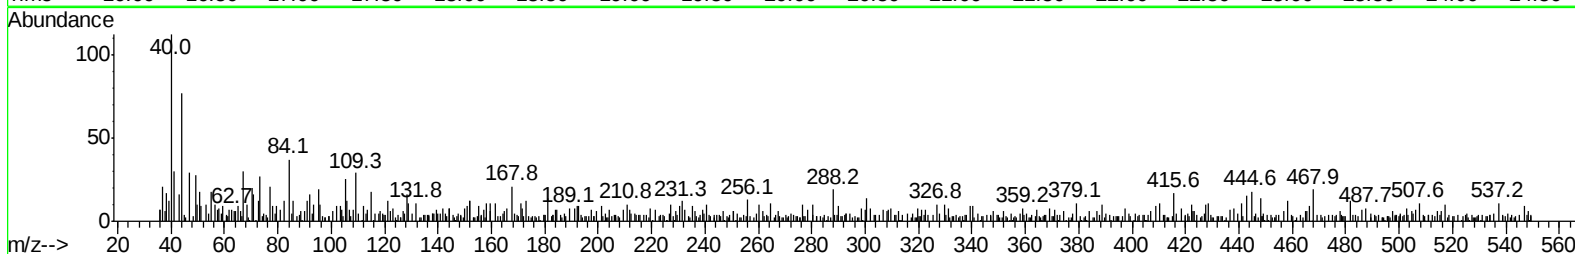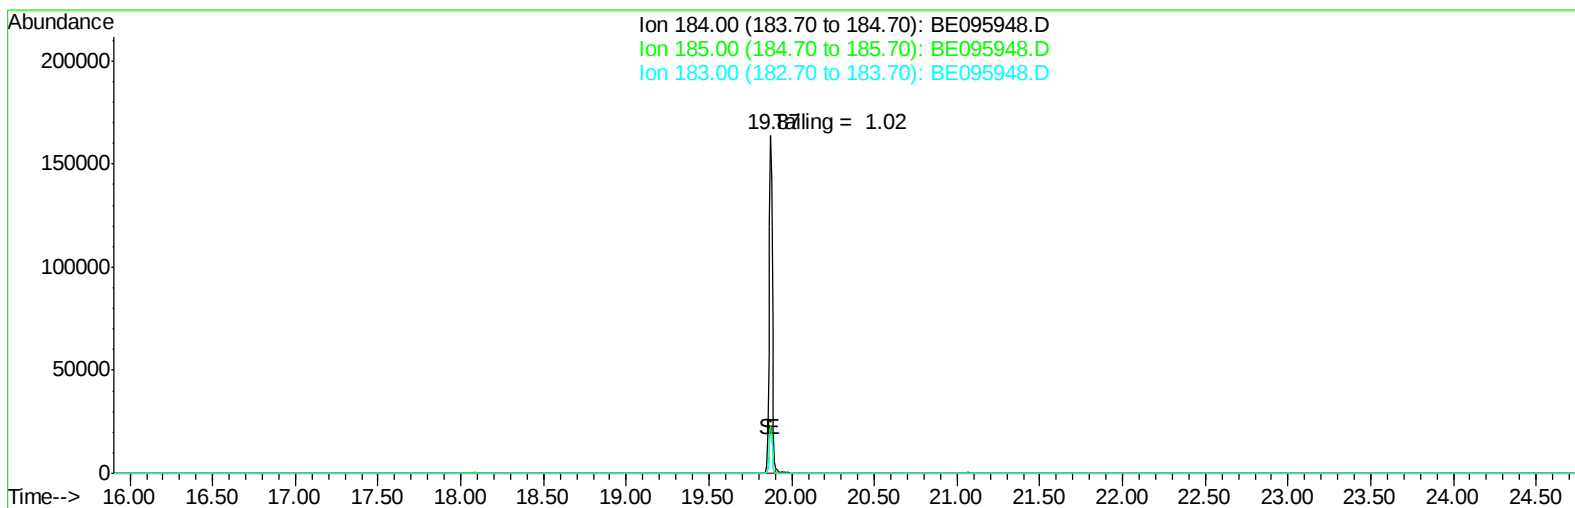

TIC: BE095948.D

(76) Benzidine

12.858min (+0.019) 119.31ng

response 17

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	28.57#
183.00	11.60	57.14#
0.00	0.00	0.00