


Data Path : Z:\HPCHEM1\BNA E\Data\BE040518\
 Data File : BE095948.D
 Acq On : 5 Apr 2018 8:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 23 12:41:11 2018

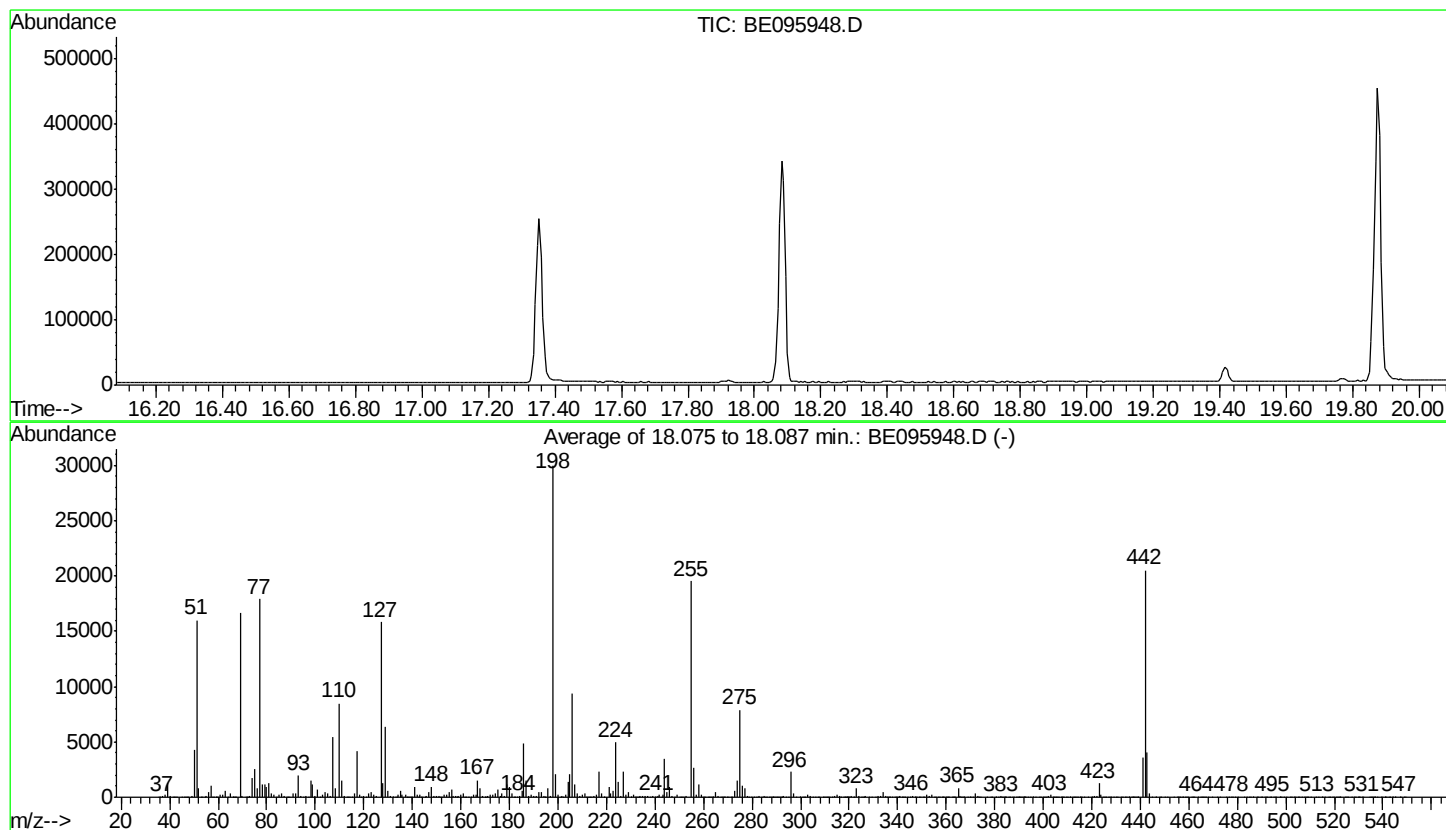

AutoFind: Scans 2636, 2637, 2638; Background Corrected with Scan 2629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.3	15975	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	55.7	16716	PASS
70	69	0.00	2	0.5	86	PASS
127	198	10	80	52.8	15819	PASS
197	198	0.00	2	0.2	65	PASS
198	198	100	100	100.0	29984	PASS
199	198	5	9	6.9	2060	PASS
275	198	10	60	26.5	7931	PASS
365	198	1	100	2.8	849	PASS
441	443	0.01	100	87.4	3549	PASS
442	198	50	100	68.4	20519	PASS
443	442	15	24	19.8	4062	PASS