

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040621\
 Data File : BE101213.D
 Acq On : 6 Apr 2021 13:00
 Operator : CG/JU
 Sample : SSTDICC0.4
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.4

Quant Time: Apr 06 13:45:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE040621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 06 13:45:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.838	152	3939	0.40	ng	0.00
7) Naphthalene-d8	10.615	136	17054	0.40	ng	0.00
13) Acenaphthene-d10	14.443	164	11193	0.40	ng	0.00
19) Phenanthrene-d10	17.211	188	27794	0.40	ng	0.00
29) Chrysene-d12	21.354	240	26065	0.40	ng	0.00
36) Perylene-d12	23.838	264	22638	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.420	112	3682	0.34	ng	0.00
5) Phenol-d6	6.986	99	5555	0.35	ng	0.00
8) Nitrobenzene-d5	8.978	82	4822	0.36	ng	0.00
11) 2-Methylnaphthalene-d10	12.196	152	15532	0.41	ng	0.00
14) 2,4,6-Tribromophenol	15.956	330	1087	0.31	ng	0.00
15) 2-Fluorobiphenyl	13.075	172	17067	0.42	ng	0.00
27) Fluoranthene-d10	19.220	212	158006	0.33	ng	0.00
31) Terphenyl-d14	19.818	244	24896	0.42	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.370	88	2501	0.36	ng	100
3) n-Nitrosodimethylamine	3.669	42	2463	0.35	ng	98
6) bis(2-Chloroethyl)ether	7.251	93	5408	0.42	ng	100
9) Naphthalene	10.667	128	75339	0.41	ng	100
10) Hexachlorobutadiene	10.965	225	3324	0.41	ng	100
12) 2-Methylnaphthalene	12.268	142	12851	0.40	ng	100
16) Acenaphthylene	14.170	152	16563	0.37	ng	100
17) Acenaphthene	14.515	154	12954	0.40	ng	100
18) Fluorene	15.502	166	16713	0.40	ng	100
20) 4,6-Dinitro-2-methylph...	15.578	198	1011	0.28	ng	100
21) 4-Bromophenyl-phenylether	16.409	248	5606	0.39	ng	100
22) Hexachlorobenzene	16.515	284	5951	0.41	ng	100
23) Atrazine	16.666	200	3409	0.30	ng	100
24) Pentachlorophenol	16.863	266	1467	0.25	ng	100
25) Phenanthrene	17.241	178	33199	0.40	ng	100
26) Anthracene	17.331	178	26104	0.37	ng	100
28) Fluoranthene	19.249	202	35153	0.34	ng	100
30) Pyrene	19.605	202	33443	0.44	ng	100
32) Benzo(a)anthracene	21.342	228	28035	0.36	ng	100
33) Chrysene	21.390	228	35303	0.41	ng	100
34) Bis(2-ethylhexyl)phtha...	21.281	149	20663	0.21	ng	100
35) Indeno(1,2,3-cd)pyrene	26.448	276	27979	0.37	ng	100
37) Benzo(b)fluoranthene	23.075	252	28973	0.42	ng	100
38) Benzo(k)fluoranthene	23.125	252	31553	0.40	ng	100
39) Benzo(a)pyrene	23.724	252	23705	0.39	ng	100
40) Dibenzo(a,h)anthracene	26.473	278	24168	0.40	ng	100
41) Benzo(g,h,i)perylene	27.247	276	27385	0.42	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040621\
Data File : BE101213.D
Acq On : 6 Apr 2021 13:00
Operator : CG/JU
Sample : SSTDICCC0.4
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4

Quant Time: Apr 06 13:45:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE040621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 06 13:45:08 2021
Response via : Initial Calibration




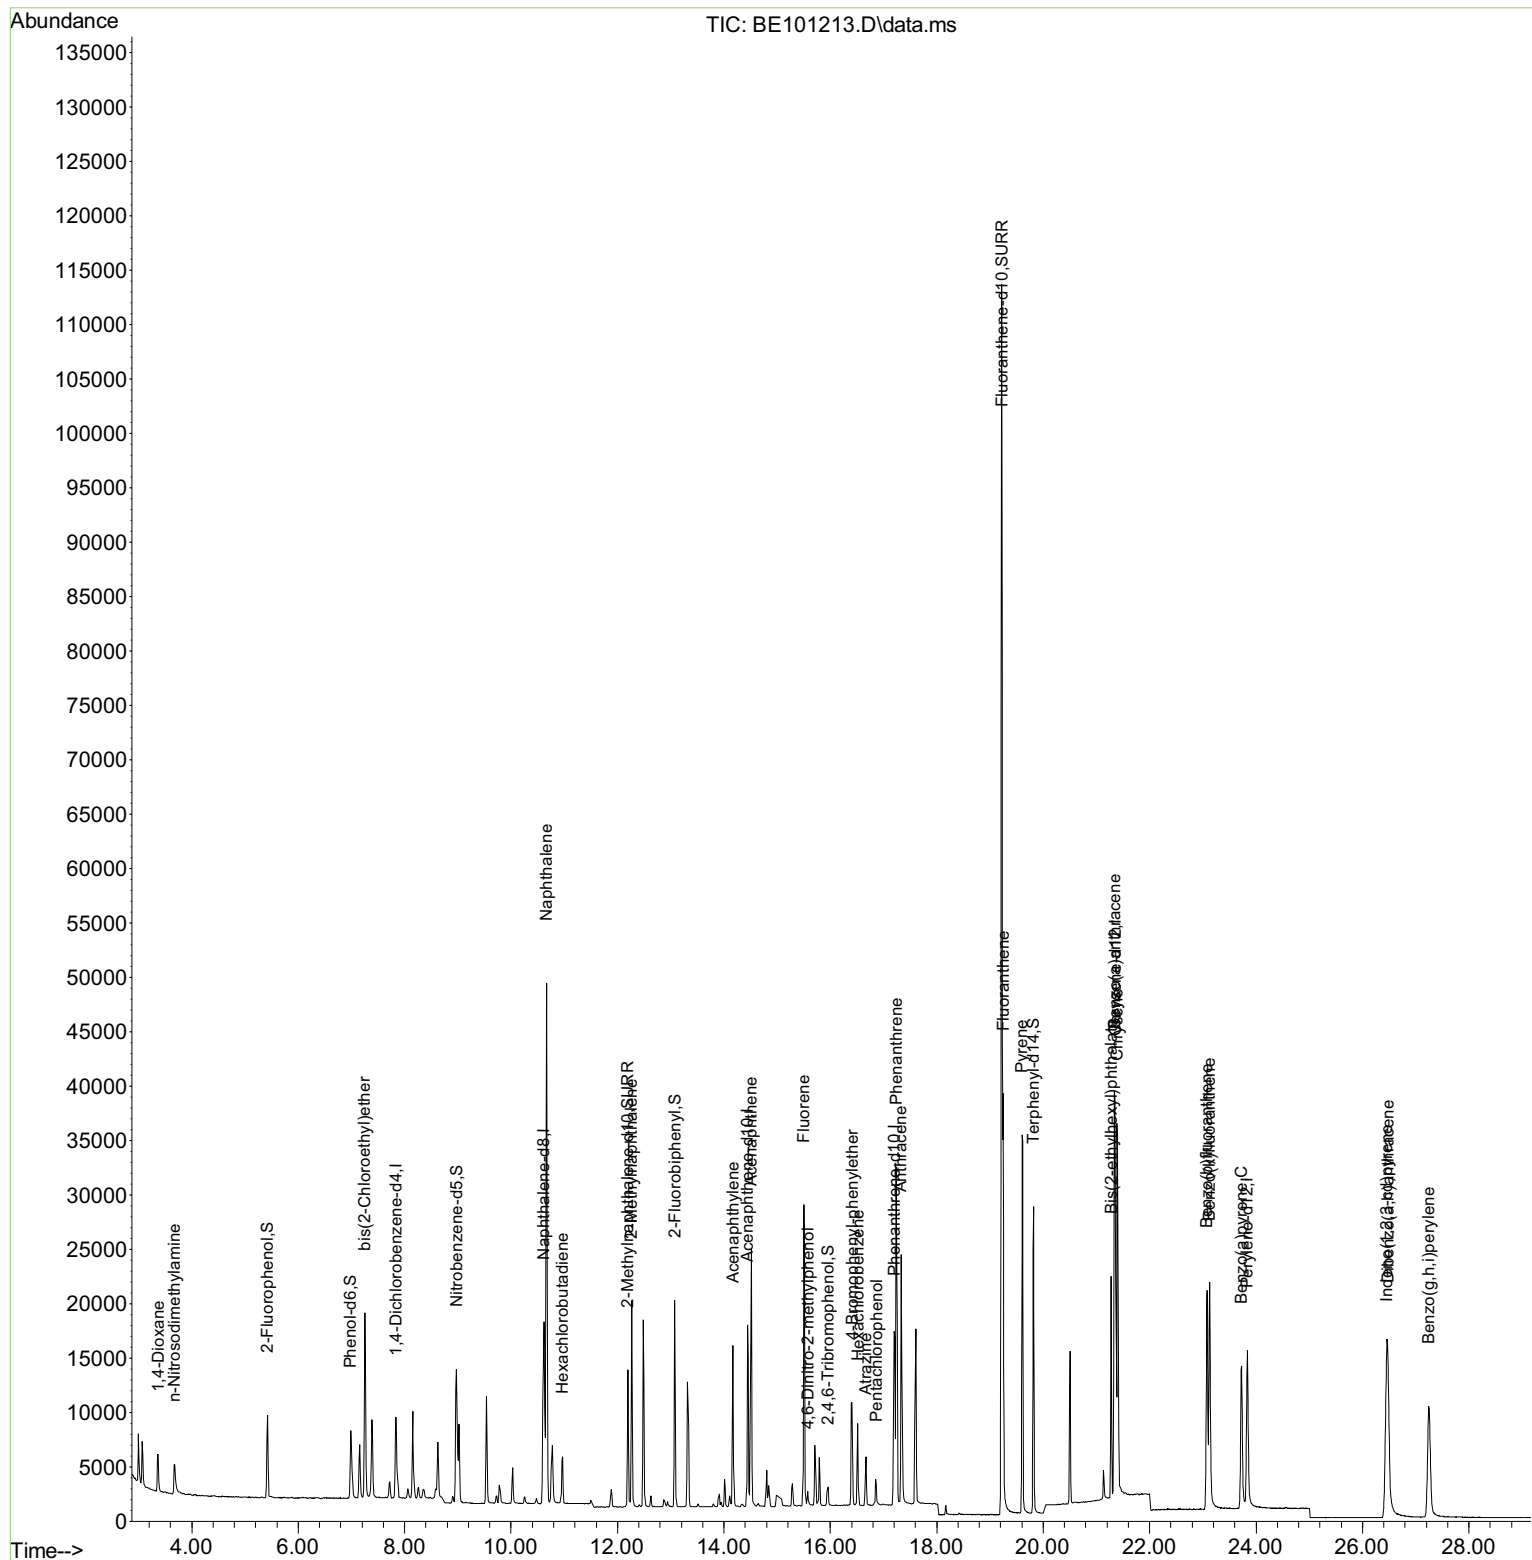


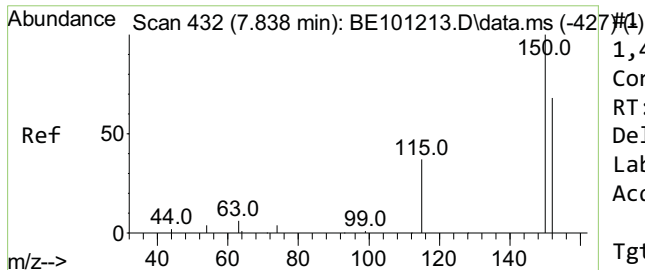

1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.838 min Scan# 432
 Delta R.T. 0.000 min
 Lab File: BE101213.D
 Acq: 6 Apr 2021 13:00




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.4


Tgt Ion:152 Resp: 3939
 Ion Ratio Lower Upper
 152 100
 150 146.1 116.9 175.3
 115 55.6 44.5 66.7

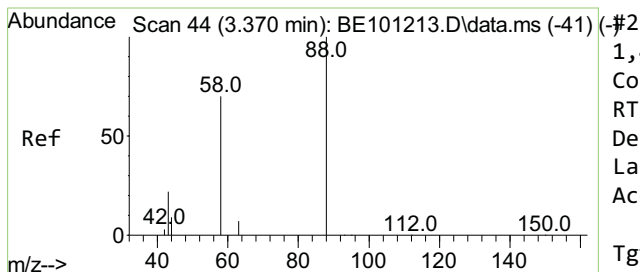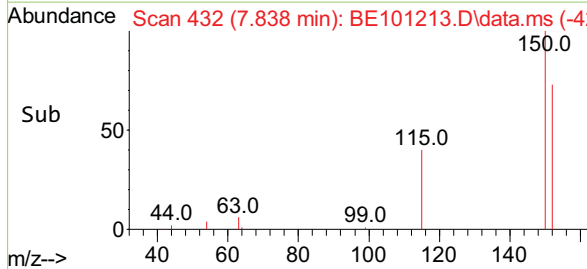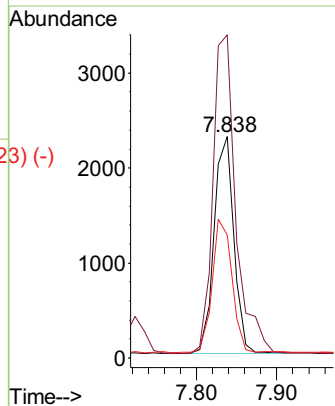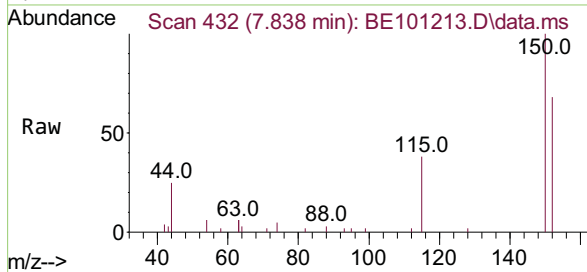

1,4-Dioxane
 Concen: 0.36 ng
 RT: 3.370 min Scan# 44
 Delta R.T. 0.000 min
 Lab File: BE101213.D
 Acq: 6 Apr 2021 13:00

Tgt Ion: 88 Resp: 2501
 Ion Ratio Lower Upper
 88 100
 58 92.0 73.6 110.4
 43 34.5 27.6 41.4


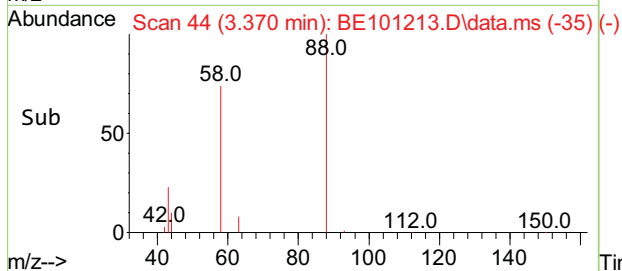
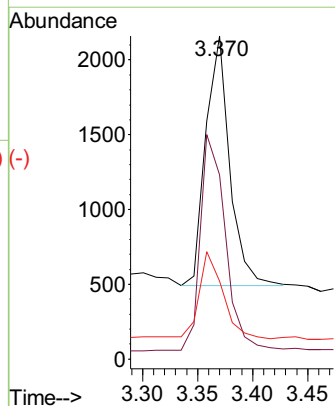
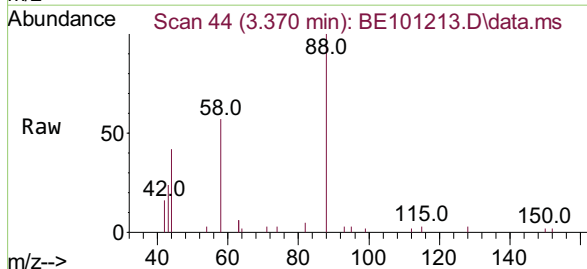


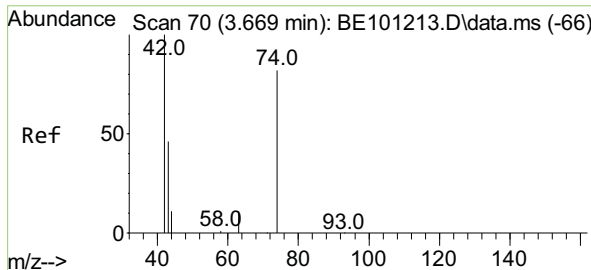

n-Nitrosodimethylamine
Concen: 0.35 ng
RT: 3.669 min Scan# 70
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00




Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	42	Resp:	2463
Ion	Ratio	Lower	Upper
42	100		
74	113.1	92.7	139.1
44	13.4	10.7	16.1

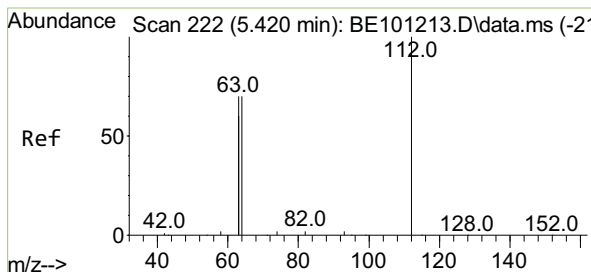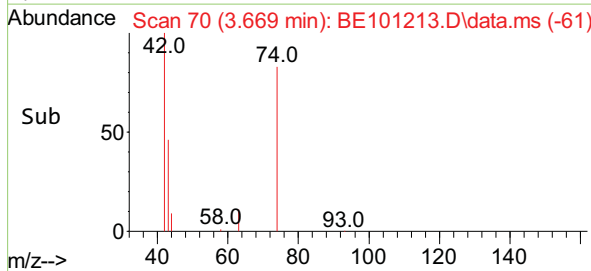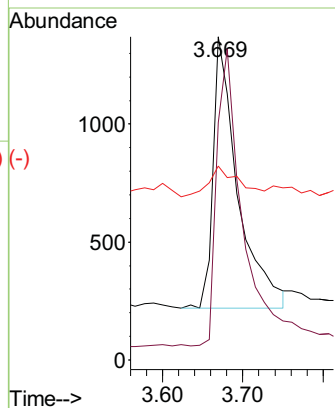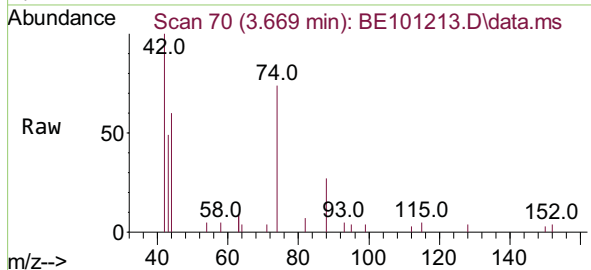

2-Fluorophenol
Concen: 0.34 ng
RT: 5.420 min Scan# 222
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Tgt Ion:	112	Resp:	3682
Ion	Ratio	Lower	Upper
112	100		
64	77.9	62.3	93.5
63	146.6	117.3	175.9


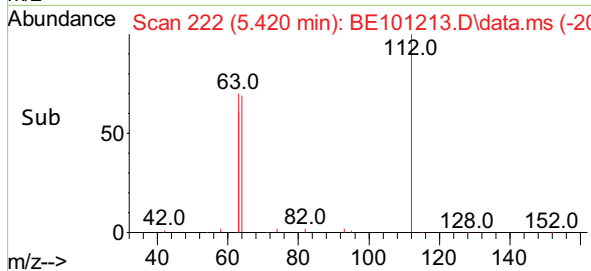
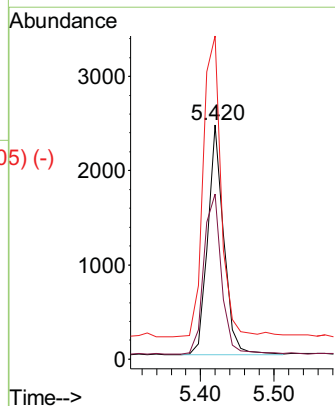
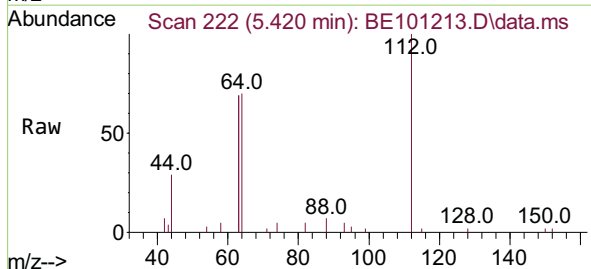


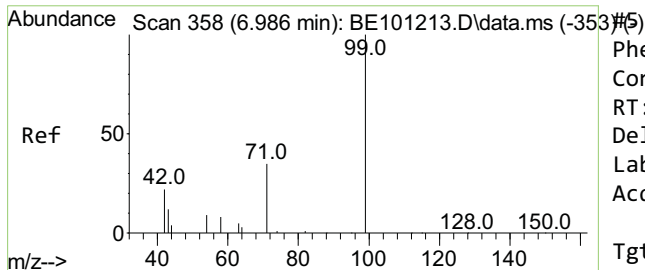

Phenol-d6
 Concen: 0.35 ng
 RT: 6.986 min Scan# 358
 Delta R.T. 0.000 min
 Lab File: BE101213.D
 Acq: 6 Apr 2021 13:00




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.4

Tgt Ion:	99	Resp:	5555
Ion	Ratio	Lower	Upper
99	100		
42	23.5	18.5	27.7
71	33.8	26.5	39.7

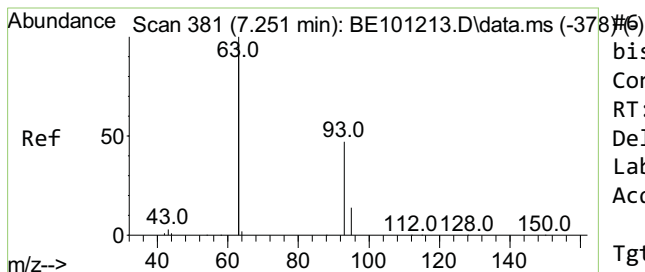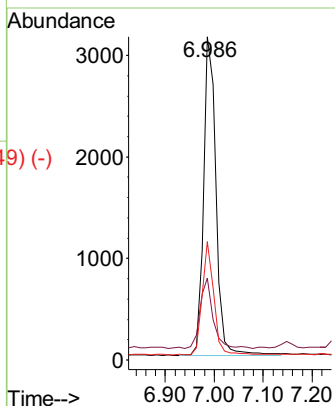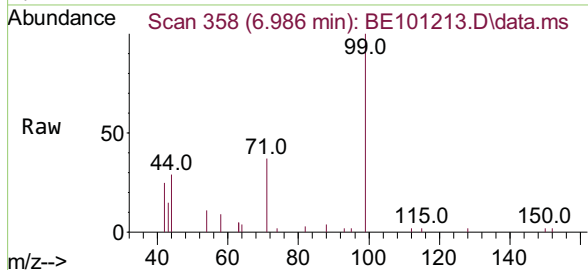


bis(2-Chloroethyl)ether
 Concen: 0.42 ng
 RT: 7.251 min Scan# 381
 Delta R.T. 0.000 min
 Lab File: BE101213.D
 Acq: 6 Apr 2021 13:00

Tgt Ion:	93	Resp:	5408
Ion	Ratio	Lower	Upper
93	100		
63	365.6	292.5	438.7
95	32.1	25.7	38.5

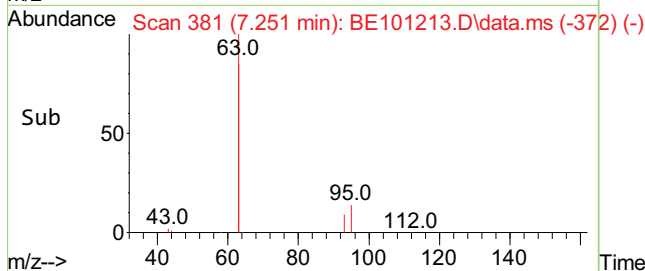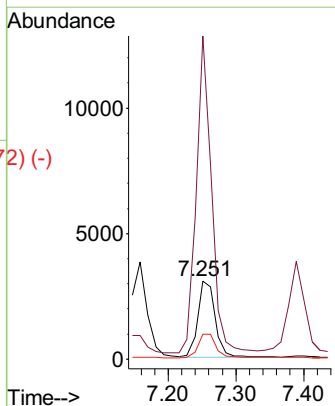




Abundance Scan 650 (10.615 min): BE101213.D\data.ms (-645) (-)

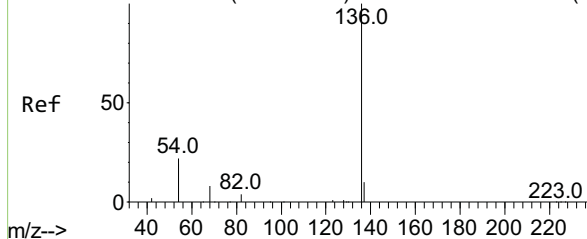


Naphthalene-d8
Concen: 0.40 ng
RT: 10.615 min Scan# 650
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	136	Resp:	17054
Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.6	13.0
54	43.4	34.7	52.1
68	8.7	7.0	10.4

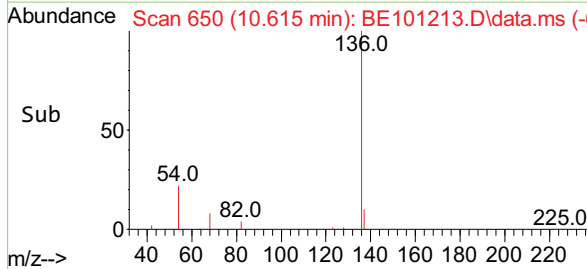
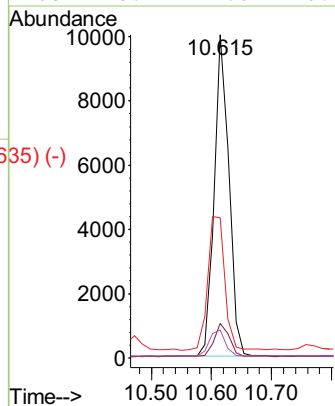
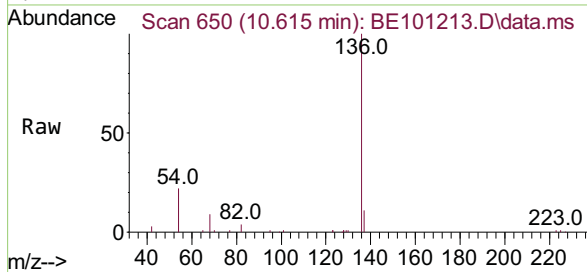


Abundance Scan 524 (8.978 min): BE101213.D\data.ms (-521) (-)

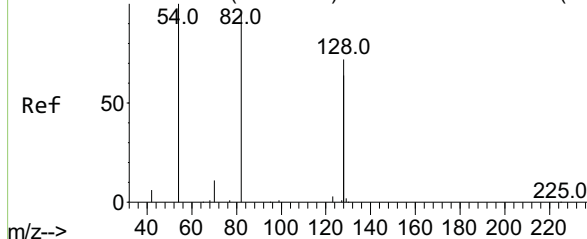


Nitrobenzene-d5
Concen: 0.36 ng
RT: 8.978 min Scan# 524
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Tgt Ion:	82	Resp:	4822
Ion	Ratio	Lower	Upper
82	100		
128	148.4	118.7	178.1
54	205.5	164.4	246.6

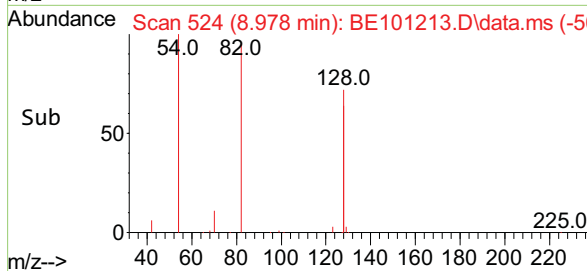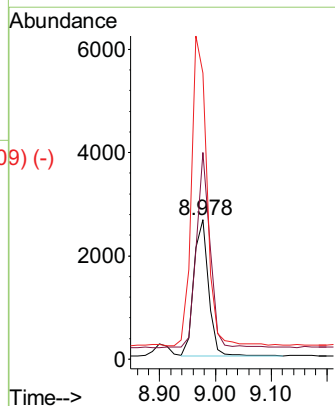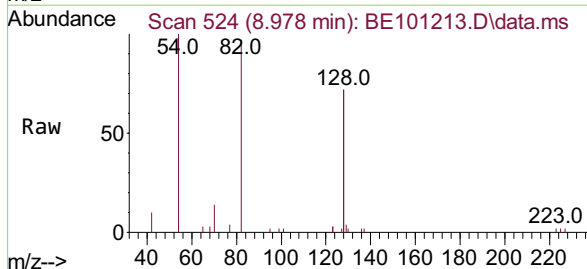



Abundance Scan 654 (10.667 min): BE101213.D\data.ms (-644) (-)

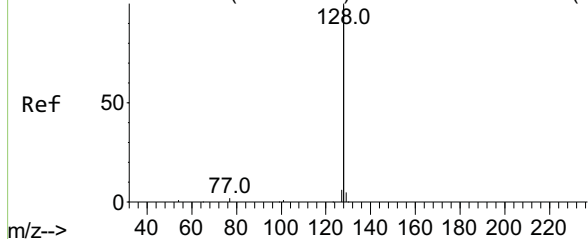


Naphthalene
Concen: 0.41 ng
RT: 10.667 min Scan# 654
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	128	Resp:	75339
Ion	Ratio	Lower	Upper
128	100		
129	2.8	2.2	3.4
127	3.2	2.6	3.8

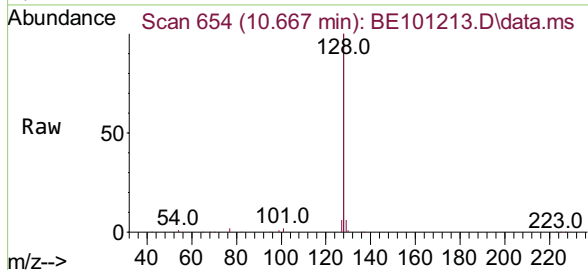

Abundance Scan 654 (10.667 min): BE101213.D\data.ms (-646) (-)


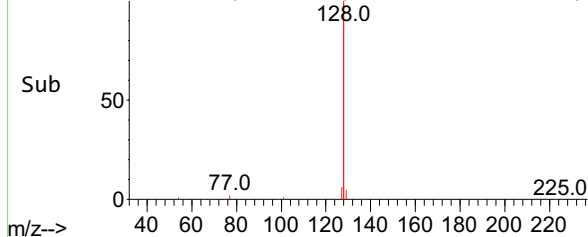


Abundance Scan 677 (10.965 min): BE101213.D\data.ms (-672) (-)

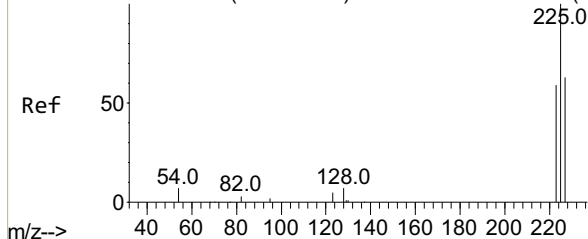



Hexachlorobutadiene
Concen: 0.41 ng
RT: 10.965 min Scan# 677
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Tgt Ion:	225	Resp:	3324
Ion	Ratio	Lower	Upper
225	100		
223	63.0	50.4	75.6
227	62.6	50.1	75.1



Abundance Scan 677 (10.965 min): BE101213.D\data.ms (-669) (-)




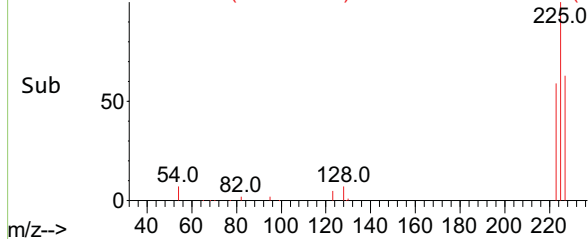


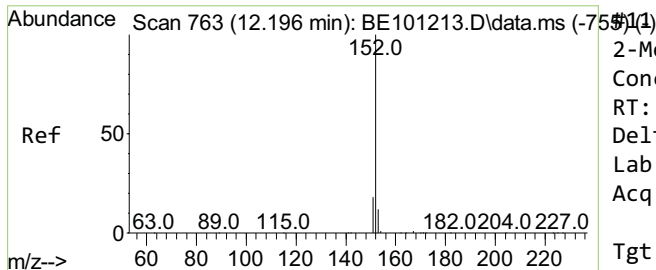

2-Methylnaphthalene-d10
 Concen: 0.41 ng
 RT: 12.196 min Scan# 763
 Delta R.T. 0.000 min
 Lab File: BE101213.D
 Acq: 6 Apr 2021 13:00




Instrument :
 BNA_E
 ClientSampled :
 SSTDICC0.4

Tgt Ion:152 Resp: 15532
 Ion Ratio Lower Upper
 152 100
 151 20.6 16.5 24.7

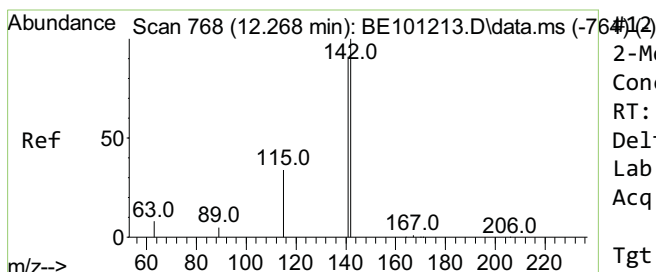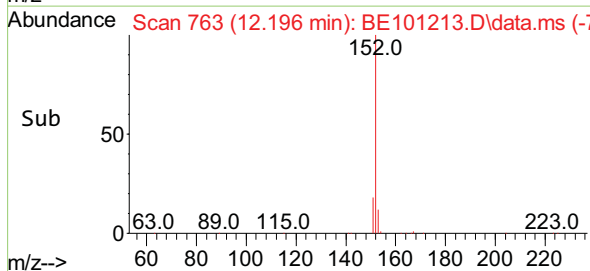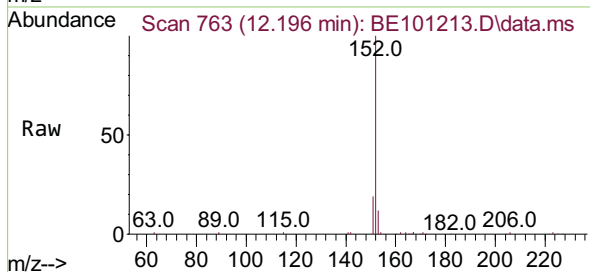


2-Methylnaphthalene
 Concen: 0.40 ng
 RT: 12.268 min Scan# 768
 Delta R.T. 0.000 min
 Lab File: BE101213.D
 Acq: 6 Apr 2021 13:00

Tgt Ion:142 Resp: 12851
 Ion Ratio Lower Upper
 142 100
 141 91.3 73.0 109.6
 115 34.8 27.8 41.8

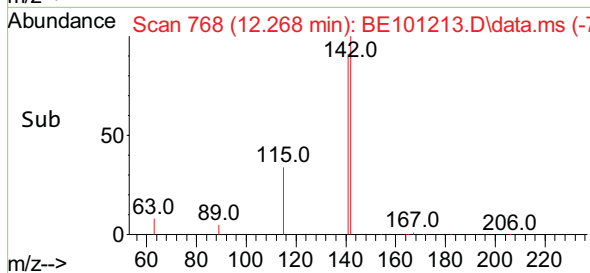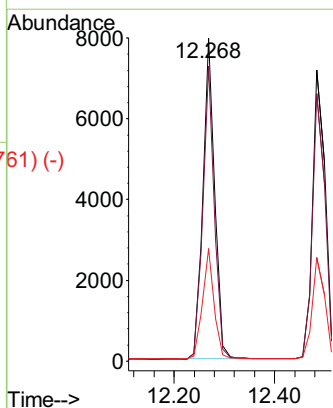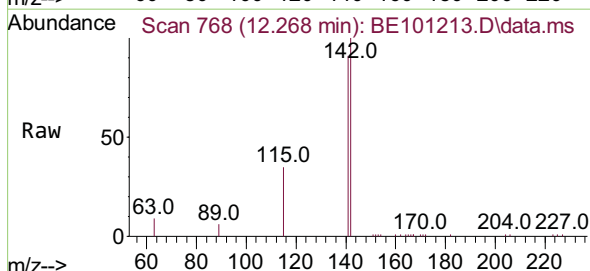




Abundance Scan 919 (14.443 min): BE101213.D\data.ms (-913)

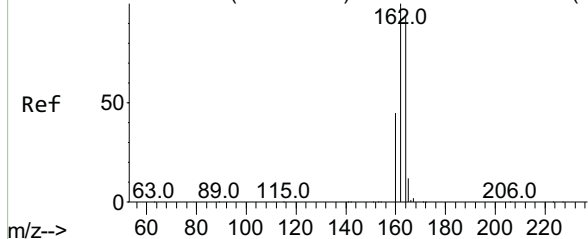


Acenaphthene-d10
Concen: 0.40 ng
RT: 14.443 min Scan# 919
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	164	Resp:	11193
Ion	Ratio	Lower	Upper
164	100		
162	106.6	85.3	127.9
160	48.9	39.1	58.7


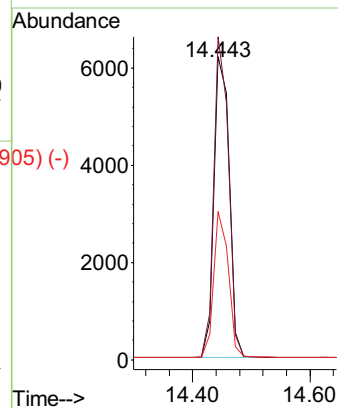
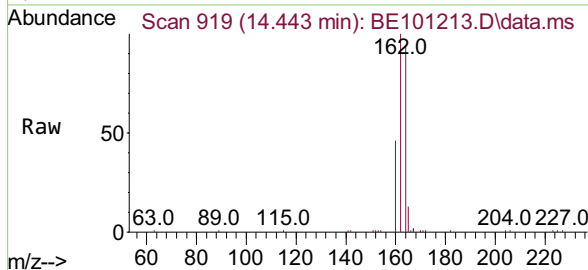



Abundance Scan 1016 (15.956 min): BE101213.D\data.ms (-1012) (-)

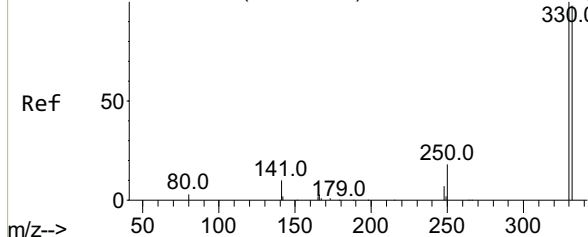

2,4,6-Tribromophenol
Concen: 0.31 ng
RT: 15.956 min Scan# 1016
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Tgt Ion:	330	Resp:	1087
Ion	Ratio	Lower	Upper
330	100		
332	97.1	77.8	116.6
141	38.0	30.4	45.6



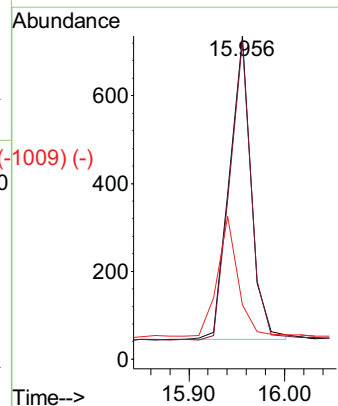



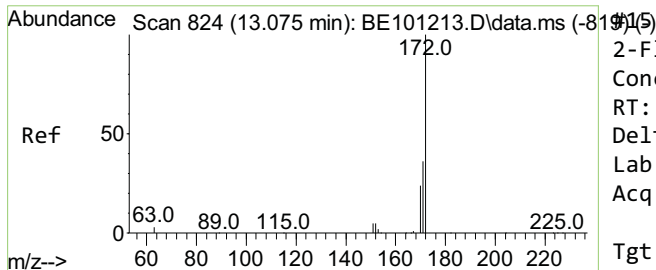

2-Fluorobiphenyl
Concen: 0.42 ng
RT: 13.075 min Scan# 824
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00




Instrument :
BNA_E
ClientSampled :
SSTDICCC0.4

Tgt Ion:	172	Resp:	17067
Ion	Ratio	Lower	Upper
172	100		
171	35.9	28.7	43.1
170	24.1	19.3	28.9

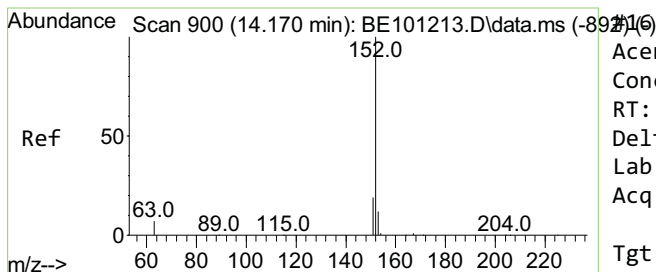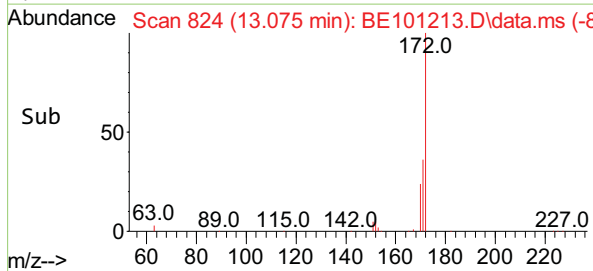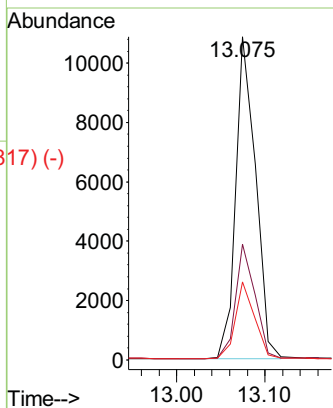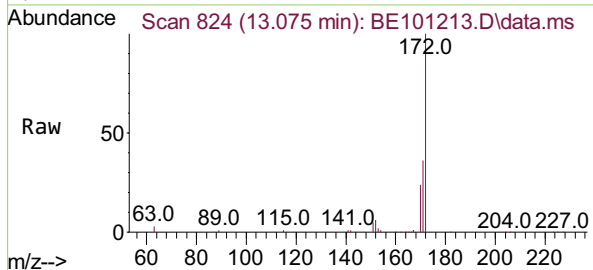


Acenaphthylene
Concen: 0.37 ng
RT: 14.170 min Scan# 900
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Tgt Ion:	152	Resp:	16563
Ion	Ratio	Lower	Upper
152	100		
151	19.2	15.4	23.2
153	12.5	10.0	15.0

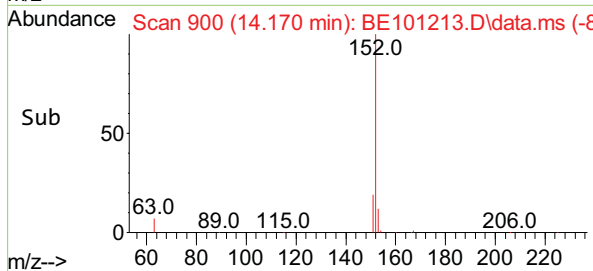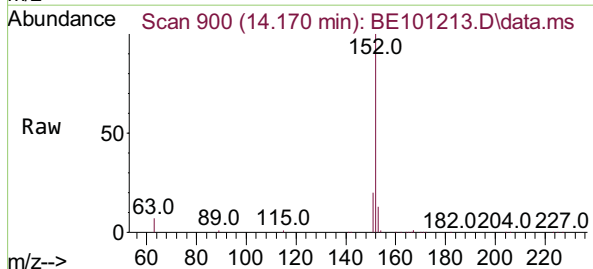



Abundance Scan 924 (14.515 min): BE101213.D\data.ms (-917) (-)

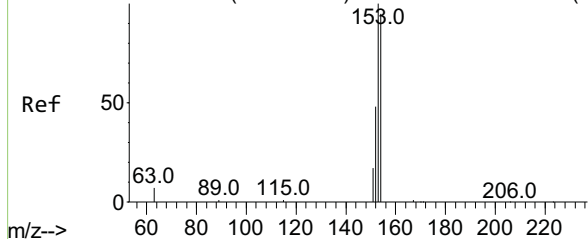


Acenaphthene
Concen: 0.40 ng
RT: 14.515 min Scan# 924
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	154	Resp:	12954
Ion Ratio	Lower	Upper	
154	100		
153	106.3	84.9	127.3
152	53.6	42.7	64.1

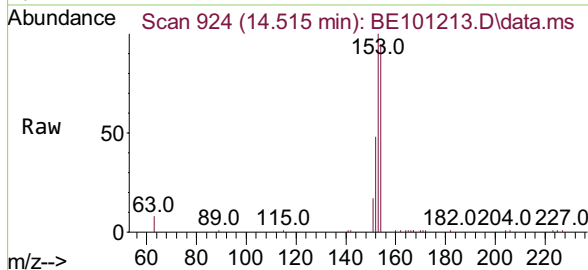

Abundance Scan 924 (14.515 min): BE101213.D\data.ms (-917) (-)


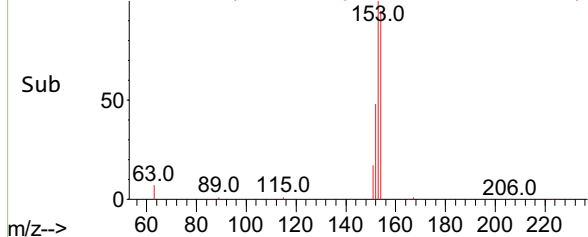


Abundance Scan 986 (15.502 min): BE101213.D\data.ms (-987) (-)

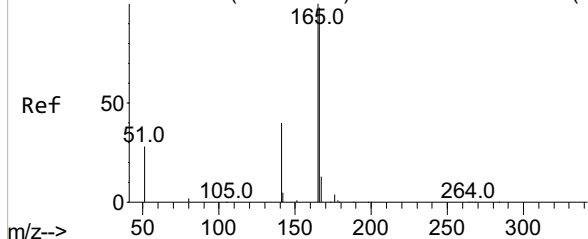


Fluorene
Concen: 0.40 ng
RT: 15.502 min Scan# 986
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Tgt Ion:	166	Resp:	16713
Ion Ratio	Lower	Upper	
166	100		
165	98.7	79.0	118.4
167	13.6	11.0	16.4




Abundance Scan 986 (15.502 min): BE101213.D\data.ms (-973) (-)

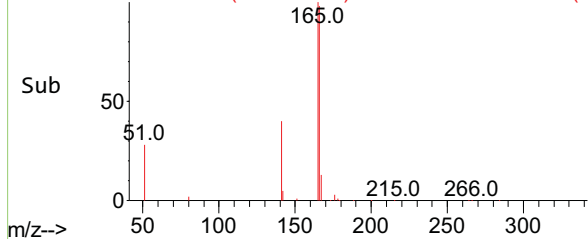




Abundance Scan 1099 (17.211 min): BE101213.D\data.ms (-1084) (-)

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.211 min Scan# 1099
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4

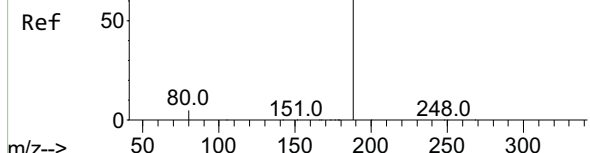




Tgt Ion:	188	Resp:	27794
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	5.7	4.6	6.8

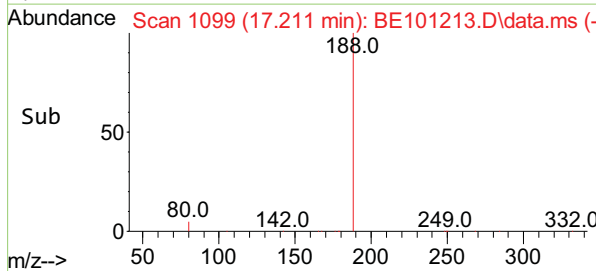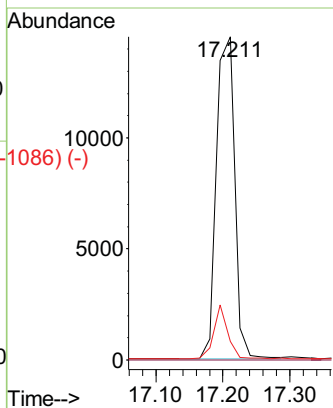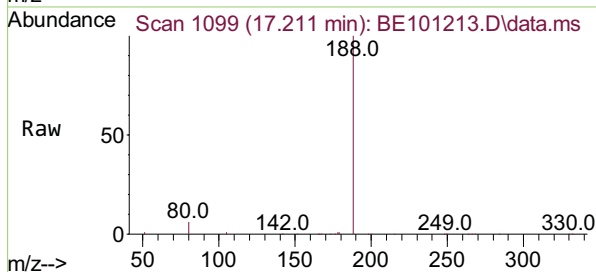


Abundance Scan 991 (15.578 min): BE101213.D\data.ms (-984) (-)

4,6-Dinitro-2-methylphenol
Concen: 0.28 ng
RT: 15.578 min Scan# 991
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Tgt Ion:	198	Resp:	1011
Ion	Ratio	Lower	Upper
198	100		
51	69.9	55.9	83.9
105	42.0	33.6	50.4

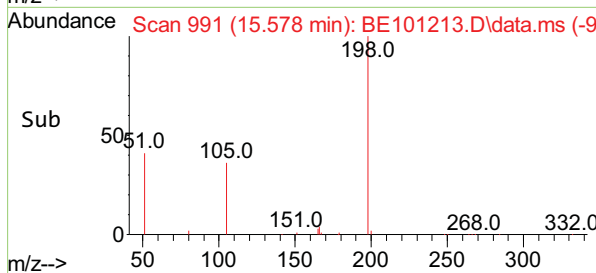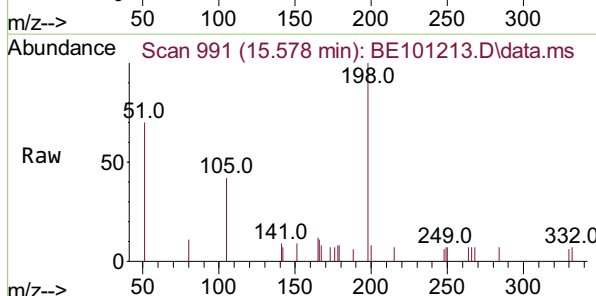



Abundance Scan 1046 (16.409 min): BE101213.D\data.ms (-1042) (-)

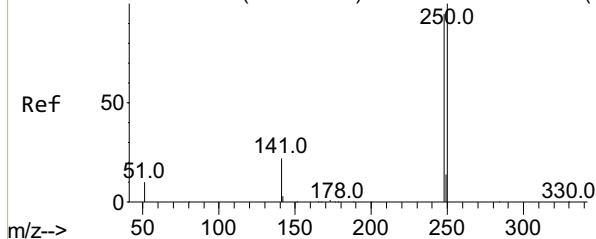


4-Bromophenyl-phenylether
Concen: 0.39 ng
RT: 16.409 min Scan# 1046
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	248	Resp:	5606
Ion	Ratio	Lower	Upper
248	100		
250	105.6	84.5	126.7
141	24.8	19.8	29.8

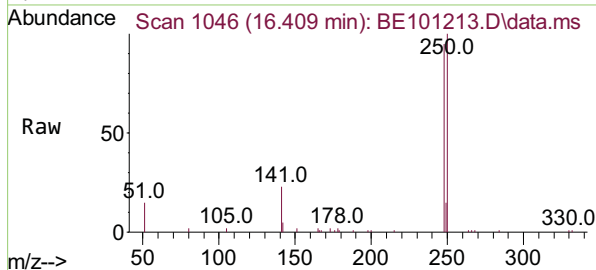

Abundance Scan 1046 (16.409 min): BE101213.D\data.ms (-1039) (-)


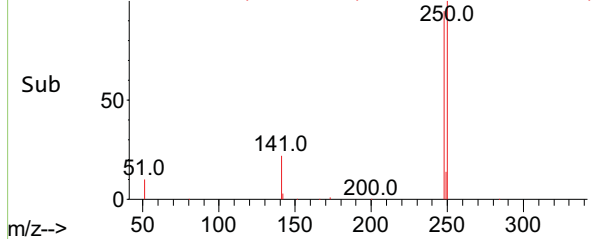


Abundance Scan 1053 (16.515 min): BE101213.D\data.ms (-1049) (-)

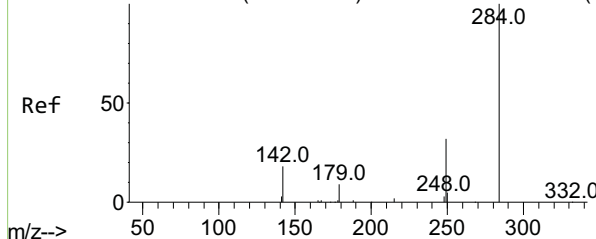


Hexachlorobenzene
Concen: 0.41 ng
RT: 16.515 min Scan# 1053
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Tgt Ion:	284	Resp:	5951
Ion	Ratio	Lower	Upper
284	100		
142	34.1	27.4	41.0
249	33.1	26.5	39.7

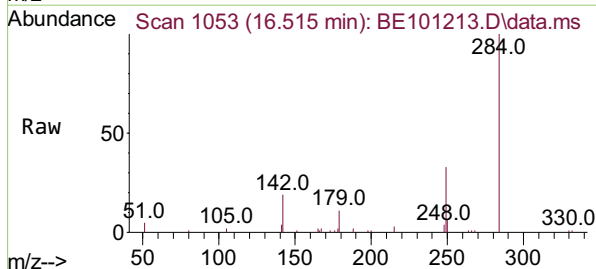


Abundance Scan 1053 (16.515 min): BE101213.D\data.ms (-1046) (-)

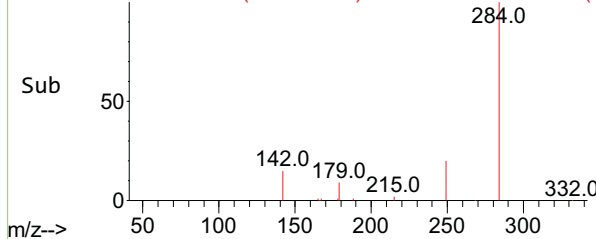




Abundance Scan 1063 (16.666 min): BE101213.D\data.ms (-1030) (-)

Atrazine
Concen: 0.30 ng
RT: 16.666 min Scan# 1063
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4

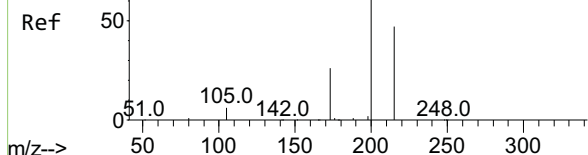


Tgt Ion:	200	Resp:	3409
Ion	Ratio	Lower	Upper
200	100		
173	27.4	21.9	32.9
215	48.2	38.6	57.8


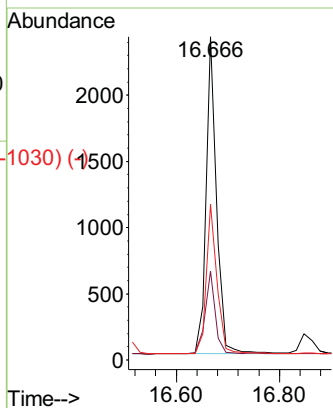
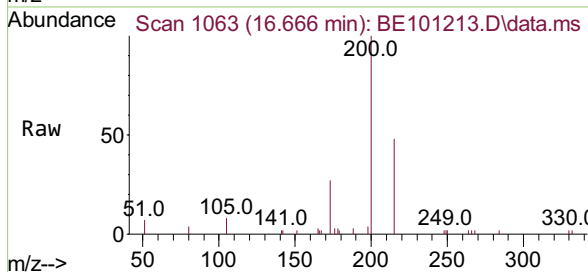



Abundance Scan 1076 (16.863 min): BE101213.D\data.ms (-1024) (-)

Pentachlorophenol
Concen: 0.25 ng
RT: 16.863 min Scan# 1076
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

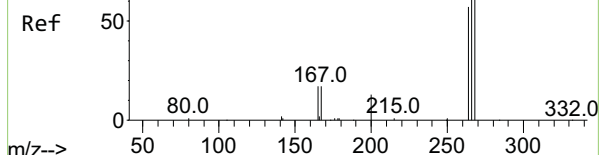

Tgt Ion:	266	Resp:	1467
Ion	Ratio	Lower	Upper
266	100		
264	61.4	49.1	73.7
268	63.3	50.6	76.0


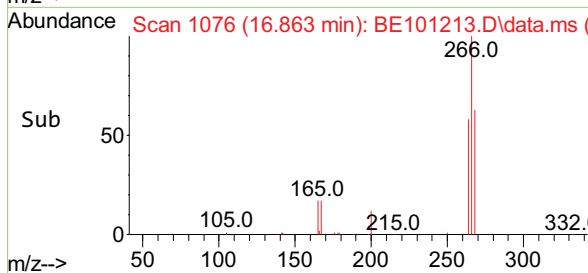




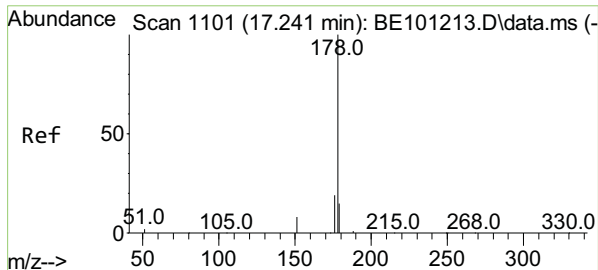

Scan 1101 (17.241 min): BE101213.D\data.ms (-1025) (-)
 Phenanthrene
 Concen: 0.40 ng
 RT: 17.241 min Scan# 1101
 Delta R.T. 0.000 min
 Lab File: BE101213.D
 Acq: 6 Apr 2021 13:00




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC0.4

Tgt Ion:	178	Resp:	33199
Ion	Ratio	Lower	Upper
178	100		
176	18.8	15.0	22.6
179	15.3	12.2	18.4

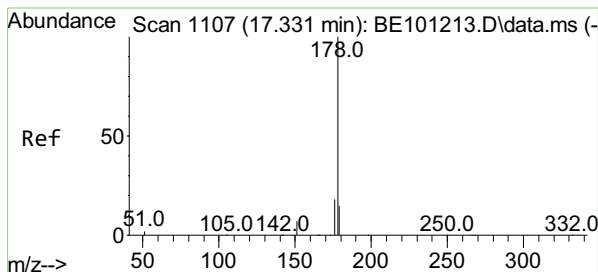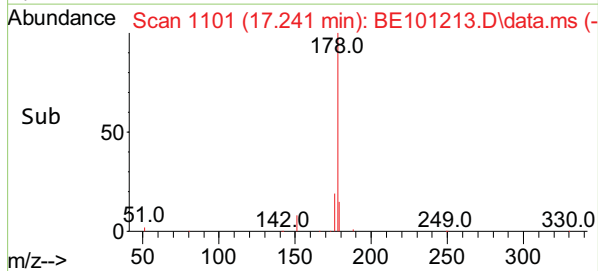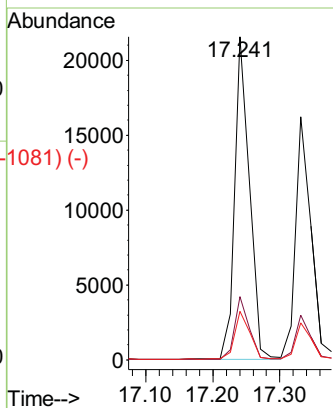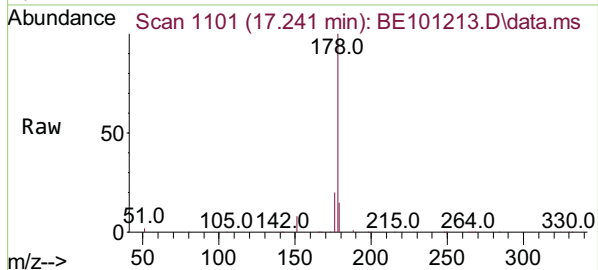

Scan 1107 (17.331 min): BE101213.D\data.ms (-1025) (-)
 Anthracene
 Concen: 0.37 ng
 RT: 17.331 min Scan# 1107
 Delta R.T. 0.000 min
 Lab File: BE101213.D
 Acq: 6 Apr 2021 13:00


Tgt Ion:	178	Resp:	26104
Ion	Ratio	Lower	Upper
178	100		
176	18.0	14.4	21.6
179	14.9	11.8	17.8

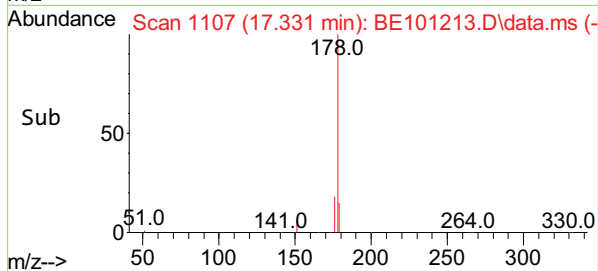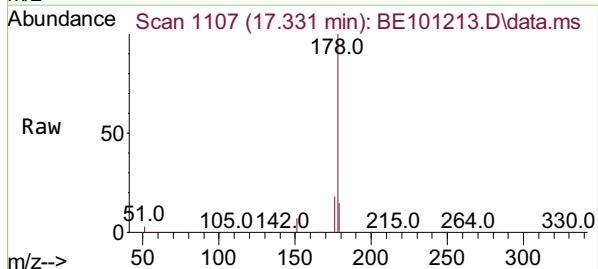




Abundance Scan 1359 (19.220 min): BE101213.D\data.ms (-1327) (-)

Fluoranthene-d10
Concen: 0.33 ng
RT: 19.220 min Scan# 1359
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4

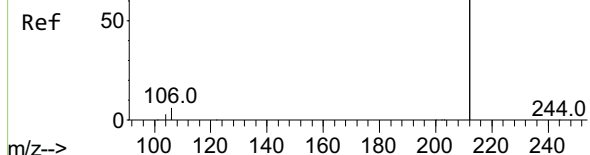





Tgt Ion:	212	Resp:	158006
Ion	Ratio	Lower	Upper
212	100		
106	3.3	2.6	4.0
104	1.8	1.4	2.2

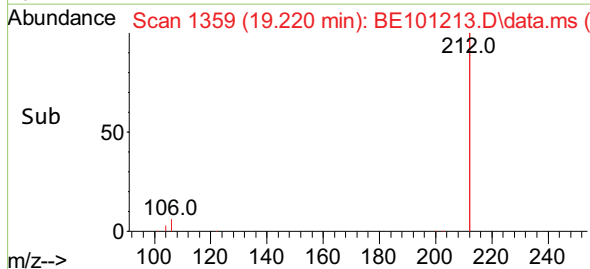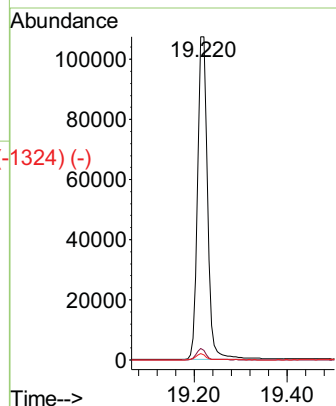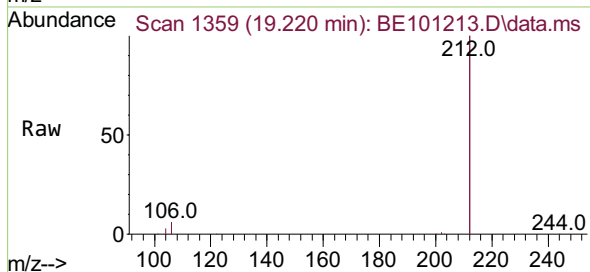

Abundance Scan 1364 (19.249 min): BE101213.D\data.ms (-1328) (-)

Fluoranthene
Concen: 0.34 ng
RT: 19.249 min Scan# 1364
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00


Tgt Ion:	202	Resp:	35153
Ion	Ratio	Lower	Upper
202	100		
101	11.4	9.1	13.7
203	17.0	13.6	20.4

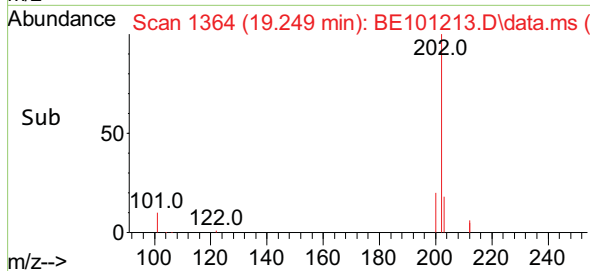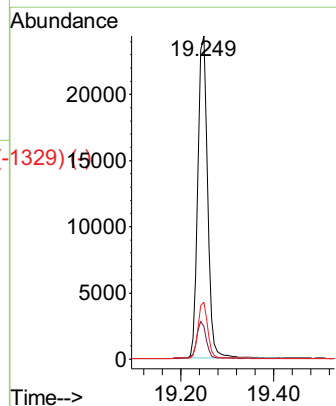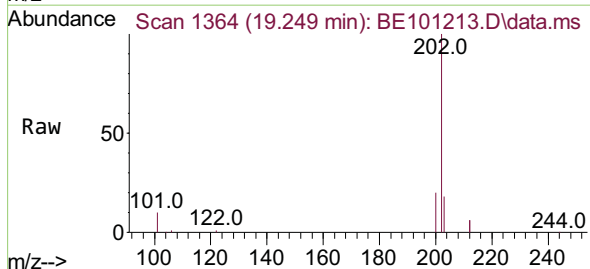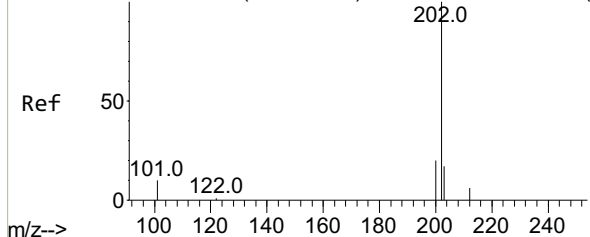




Abundance Scan 1603 (21.354 min): BE101213.D\data.ms (-1586) (-)

Chrysene-d12
Concen: 0.40 ng
RT: 21.354 min Scan# 1603
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4

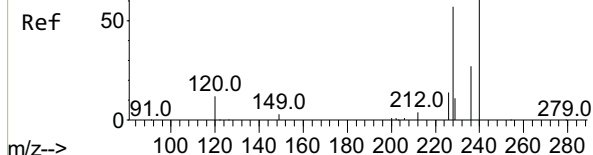


Tgt Ion:	240	Resp:	26065
Ion	Ratio	Lower	Upper
240	100		
120	12.8	10.2	15.4
236	27.1	21.7	32.5

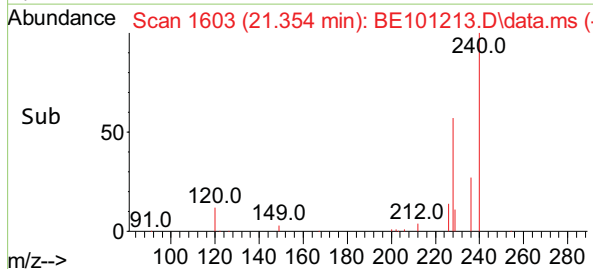

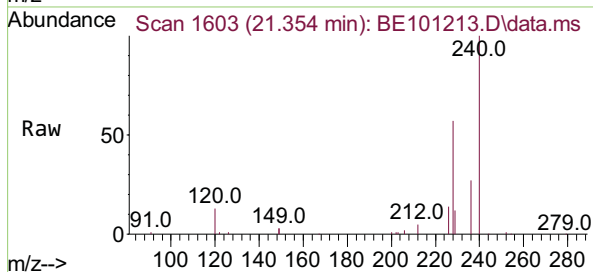


Abundance Scan 1426 (19.605 min): BE101213.D\data.ms (-1391) (-)

Pyrene
Concen: 0.44 ng
RT: 19.605 min Scan# 1426
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

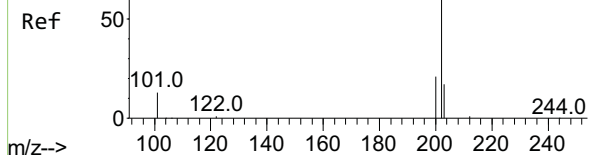


Tgt Ion:	202	Resp:	33443
Ion	Ratio	Lower	Upper
202	100		
200	20.7	16.6	24.8
203	17.3	13.8	20.8

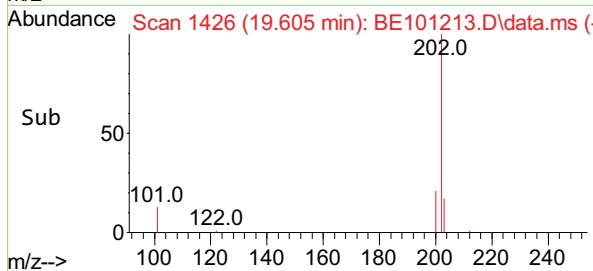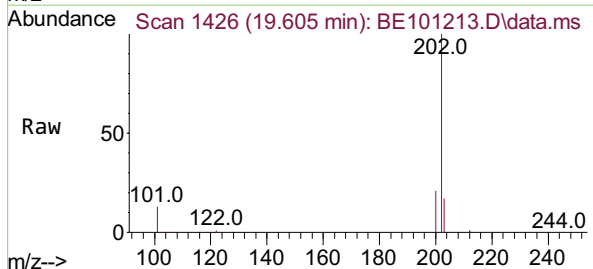




Abundance Scan 1463 (19.818 min): BE101213.D\data.ms (-1434) (-)

Terphenyl-d14
Concen: 0.42 ng
RT: 19.818 min Scan# 1463
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4

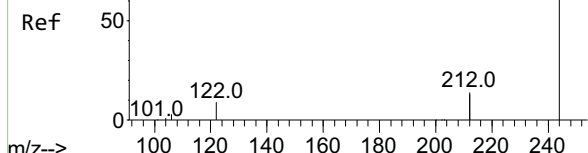


Tgt Ion:	244	Resp:	24896
Ion	Ratio	Lower	Upper
244	100		
212	27.4	21.9	32.9
122	9.1	7.3	10.9



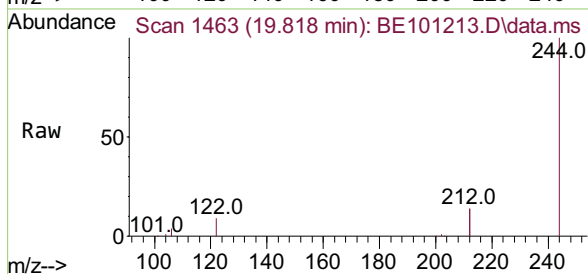



Abundance Scan 1602 (21.342 min): BE101213.D\data.ms (-1534) (-)

Benzo(a)anthracene
Concen: 0.36 ng
RT: 21.342 min Scan# 1602
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

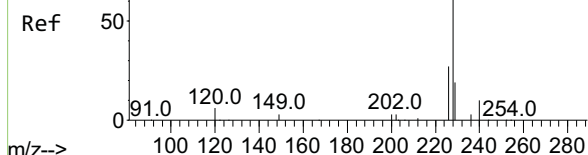

Tgt Ion:	228	Resp:	28035
Ion	Ratio	Lower	Upper
228	100		
226	26.8	21.4	32.2
229	19.6	15.7	23.5







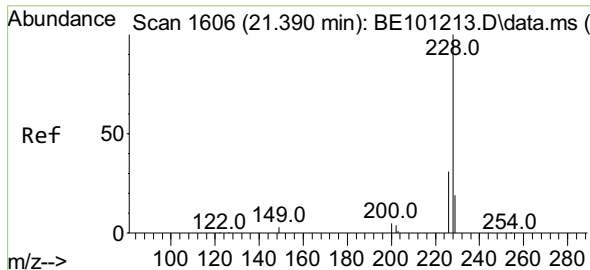

Scan 1606 (21.390 min): BE101213.D\data.ms (-1598) (-)
 Chrysene
 Concen: 0.41 ng
 RT: 21.390 min Scan# 1606
 Delta R.T. 0.000 min
 Lab File: BE101213.D
 Acq: 6 Apr 2021 13:00




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICCC0.4

Tgt Ion:	228	Resp:	35303
Ion	Ratio	Lower	Upper
228	100		
226	31.0	24.8	37.2
229	19.0	15.2	22.8

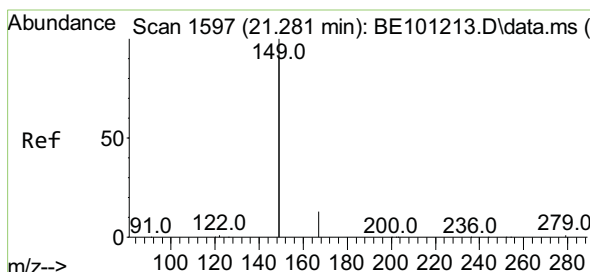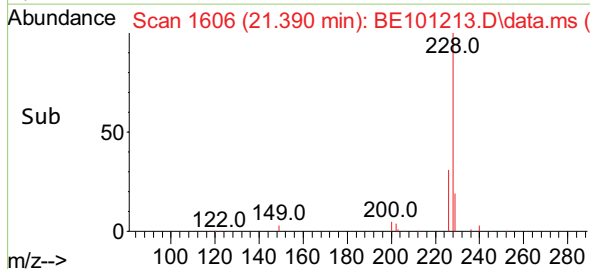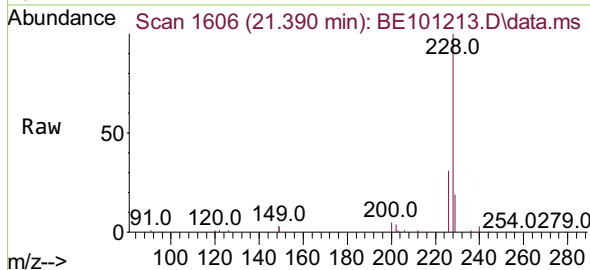


Scan 1597 (21.281 min): BE101213.D\data.ms (-1592) (-)
 Bis(2-ethylhexyl)phthalate
 Concen: 0.21 ng
 RT: 21.281 min Scan# 1597
 Delta R.T. 0.000 min
 Lab File: BE101213.D
 Acq: 6 Apr 2021 13:00

Tgt Ion:	149	Resp:	20663
Ion	Ratio	Lower	Upper
149	100		
167	6.9	5.5	8.3
279	1.2	1.0	1.4

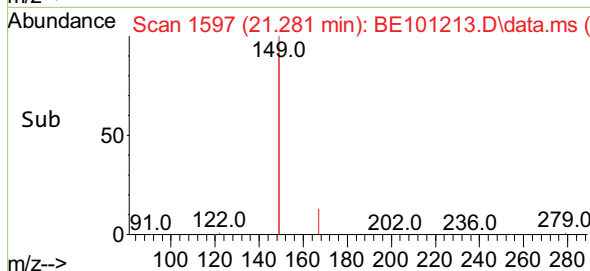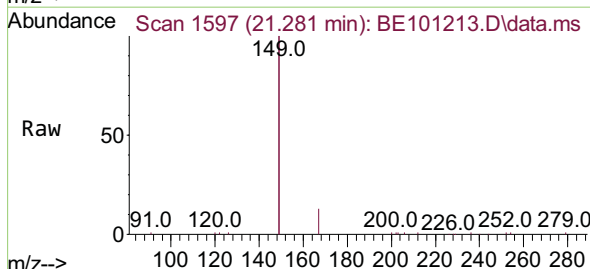


Abundance Scan 2893 (26.448 min): BE101213.D\data.ms (-2865) (-)


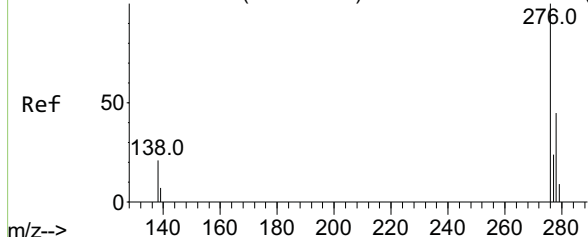


Indeno(1,2,3-cd)pyrene
Concen: 0.37 ng
RT: 26.448 min Scan# 2893
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00


Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4

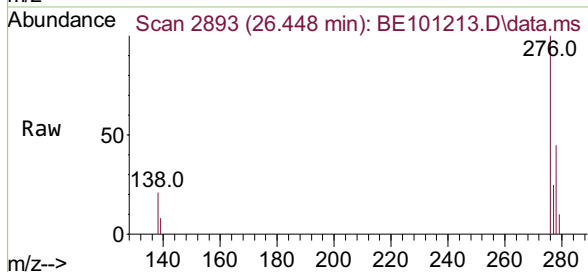


Tgt Ion	Ratio	Lower	Upper
276	100		
138	22.0	17.4	26.0
277	24.8	19.8	29.8

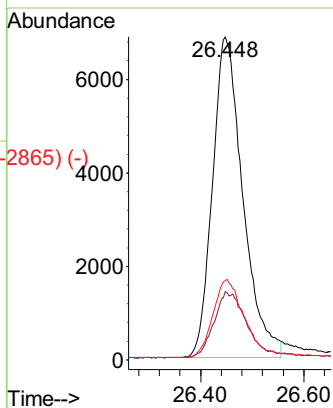



Abundance Scan 2165 (23.838 min): BE101213.D\data.ms (-2123) (-)

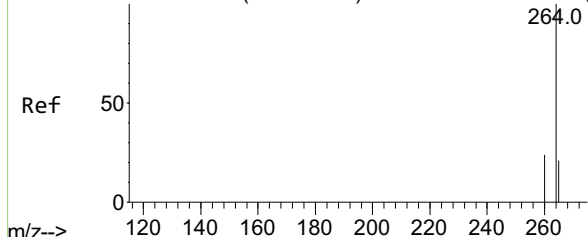

Perylene-d12
Concen: 0.40 ng
RT: 23.838 min Scan# 2165
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00




Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.1	19.3	28.9
265	28.0	22.4	33.6

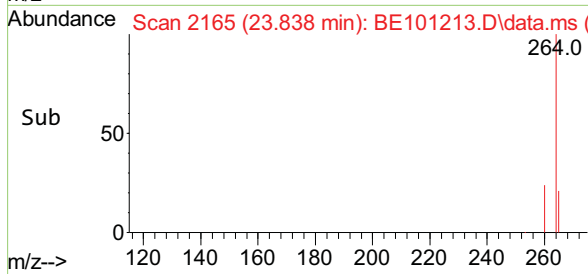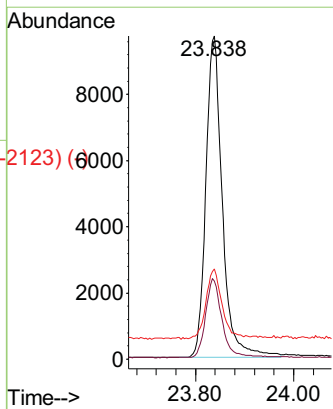




Abundance Scan 1951 (23.075 min): BE101213.D\data.ms (-1937)

Benzo(b)fluoranthene
Concen: 0.42 ng
RT: 23.075 min Scan# 1951
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4

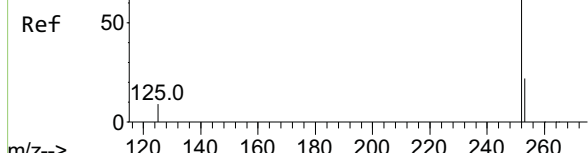





Tgt Ion:	252	Resp:	28973
Ion	Ratio	Lower	Upper
252	100		
253	22.6	18.1	27.1
125	9.5	7.6	11.4

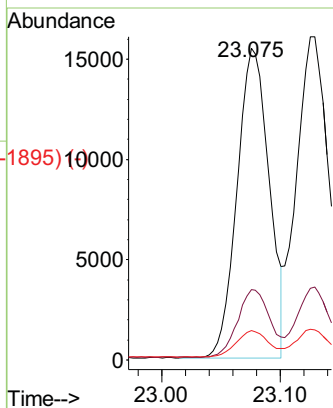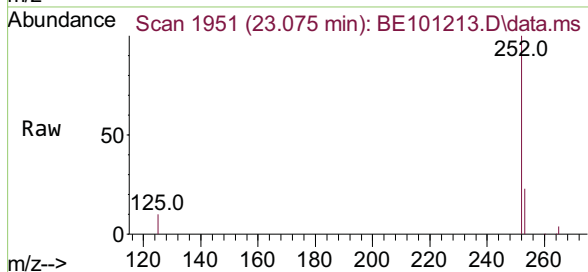


Abundance Scan 1965 (23.125 min): BE101213.D\data.ms (-1939)

Benzo(k)fluoranthene
Concen: 0.40 ng
RT: 23.125 min Scan# 1965
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Tgt Ion:	252	Resp:	31553
Ion	Ratio	Lower	Upper
252	100		
253	22.2	17.8	26.6
125	9.5	7.6	11.4

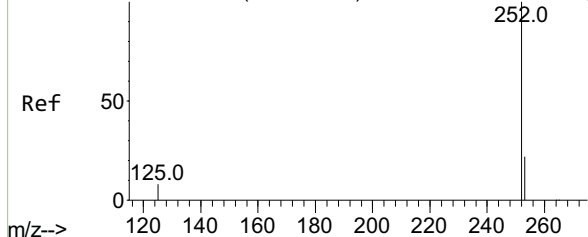




Abundance Scan 2133 (23.724 min): BE101213.D\data.ms (-287) (-)

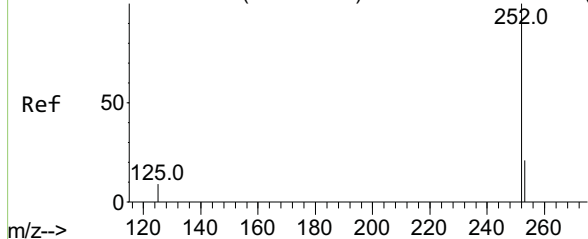


Benzo(a)pyrene
Concen: 0.39 ng
RT: 23.724 min Scan# 2133
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	252	Resp:	23705
Ion	Ratio	Lower	Upper
252	100		
253	22.5	18.0	27.0
125	10.0	8.0	12.0



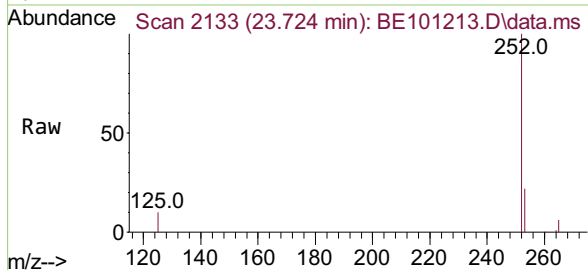


Abundance Scan 2900 (26.473 min): BE101213.D\data.ms (-287) (-)

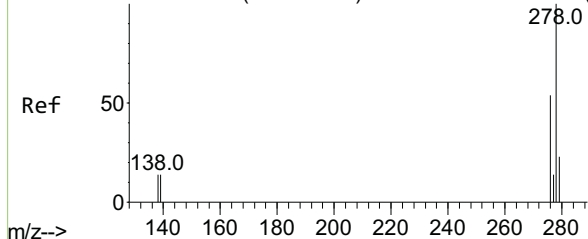


Dibenzo(a,h)anthracene
Concen: 0.40 ng
RT: 26.473 min Scan# 2900
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Tgt Ion:	278	Resp:	24168
Ion	Ratio	Lower	Upper
278	100		
139	15.2	12.2	18.2
279	24.1	19.3	28.9




Abundance Scan 3117 (27.247 min): BE101213.D\data.ms (-3061) (-)

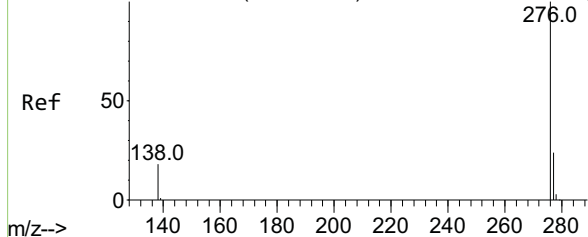

Benzo(g,h,i)perylene
Concen: 0.42 ng
RT: 27.247 min Scan# 3117
Delta R.T. 0.000 min
Lab File: BE101213.D
Acq: 6 Apr 2021 13:00

Instrument :
BNA_E
ClientSampleId :
SSTDICCC0.4

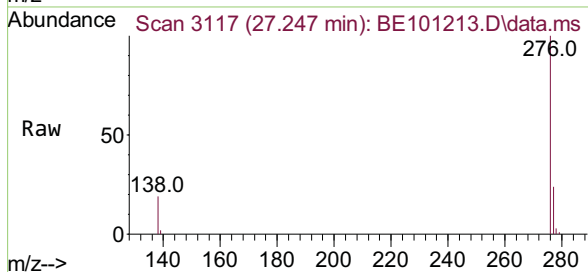

Tgt Ion:	276	Resp:	27385
Ion	Ratio	Lower	Upper
276	100		
277	24.2	19.4	29.0
138	19.0	15.2	22.8

