

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040621\
 Data File : BE101215.D
 Acq On : 6 Apr 2021 14:15
 Operator : CG/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC1.6

Quant Time: Apr 06 14:59:09 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE040621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 06 13:45:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	3949	0.40	ng	# 0.00
7) Naphthalene-d8	10.614	136	17728	0.40	ng	0.00
13) Acenaphthene-d10	14.443	164	12614	0.40	ng	0.00
19) Phenanthrene-d10	17.196	188	33318	0.40	ng	#-0.01
29) Chrysene-d12	21.366	240	34536	0.40	ng	# 0.01
36) Perylene-d12	23.838	264	24524	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.422	112	14716	1.37	ng	0.00
5) Phenol-d6	6.988	99	23283	1.47	ng	0.00
8) Nitrobenzene-d5	8.977	82	21805	1.56	ng	0.00
11) 2-Methylnaphthalene-d10	12.195	152	66974	1.69	ng	0.00
14) 2,4,6-Tribromophenol	15.956	330	6664	1.69	ng	0.00
15) 2-Fluorobiphenyl	13.074	172	73789	1.61	ng	0.00
27) Fluoranthene-d10	19.219	212	1004172	1.75	ng	0.00
31) Terphenyl-d14	19.817	244	166790	2.14	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.372	88	9376	1.34	ng	98
3) n-Nitrosodimethylamine	3.671	42	10941	1.53	ng	# 94
6) bis(2-Chloroethyl)ether	7.253	93	21929	1.69	ng	100
9) Naphthalene	10.666	128	310218	1.62	ng	100
10) Hexachlorobutadiene	10.965	225	13516	1.59	ng	98
12) 2-Methylnaphthalene	12.267	142	56327	1.69	ng	98
16) Acenaphthylene	14.169	152	85545	1.70	ng	99
17) Acenaphthene	14.515	154	61401	1.67	ng	99
18) Fluorene	15.503	166	82700	1.75	ng	99
20) 4,6-Dinitro-2-methylph...	15.578	198	7612	1.77	ng	# 73
21) 4-Bromophenyl-phenylether	16.410	248	28095	1.62	ng	97
22) Hexachlorobenzene	16.516	284	27553	1.57	ng	99
23) Atrazine	16.667	200	22324	1.67	ng	98
24) Pentachlorophenol	16.849	266	10279	1.49	ng	98
25) Phenanthrene	17.242	178	161530	1.64	ng	100
26) Anthracene	17.332	178	146311	1.72	ng	99
28) Fluoranthene	19.248	202	227062	1.81	ng	99
30) Pyrene	19.610	202	222245	2.21	ng	99
32) Benzo(a)anthracene	21.342	228	163361	1.57	ng	99
33) Chrysene	21.403	228	188994	1.65	ng	96
34) Bis(2-ethylhexyl)phtha...	21.282	149	112005	0.87	ng	100
35) Indeno(1,2,3-cd)pyrene	26.453	276	141197	1.40	ng	99
37) Benzo(b)fluoranthene	23.078	252	131990	1.76	ng	99
38) Benzo(k)fluoranthene	23.128	252	145334	1.71	ng	100
39) Benzo(a)pyrene	23.727	252	117573	1.77	ng	99
40) Dibenzo(a,h)anthracene	26.477	278	124347	1.91	ng	99
41) Benzo(g,h,i)perylene	27.251	276	129757	1.84	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040621\
Data File : BE101215.D
Acq On : 6 Apr 2021 14:15
Operator : CG/JU
Sample : SSTDIC1.6
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

Quant Time: Apr 06 14:59:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE040621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 06 13:45:08 2021
Response via : Initial Calibration




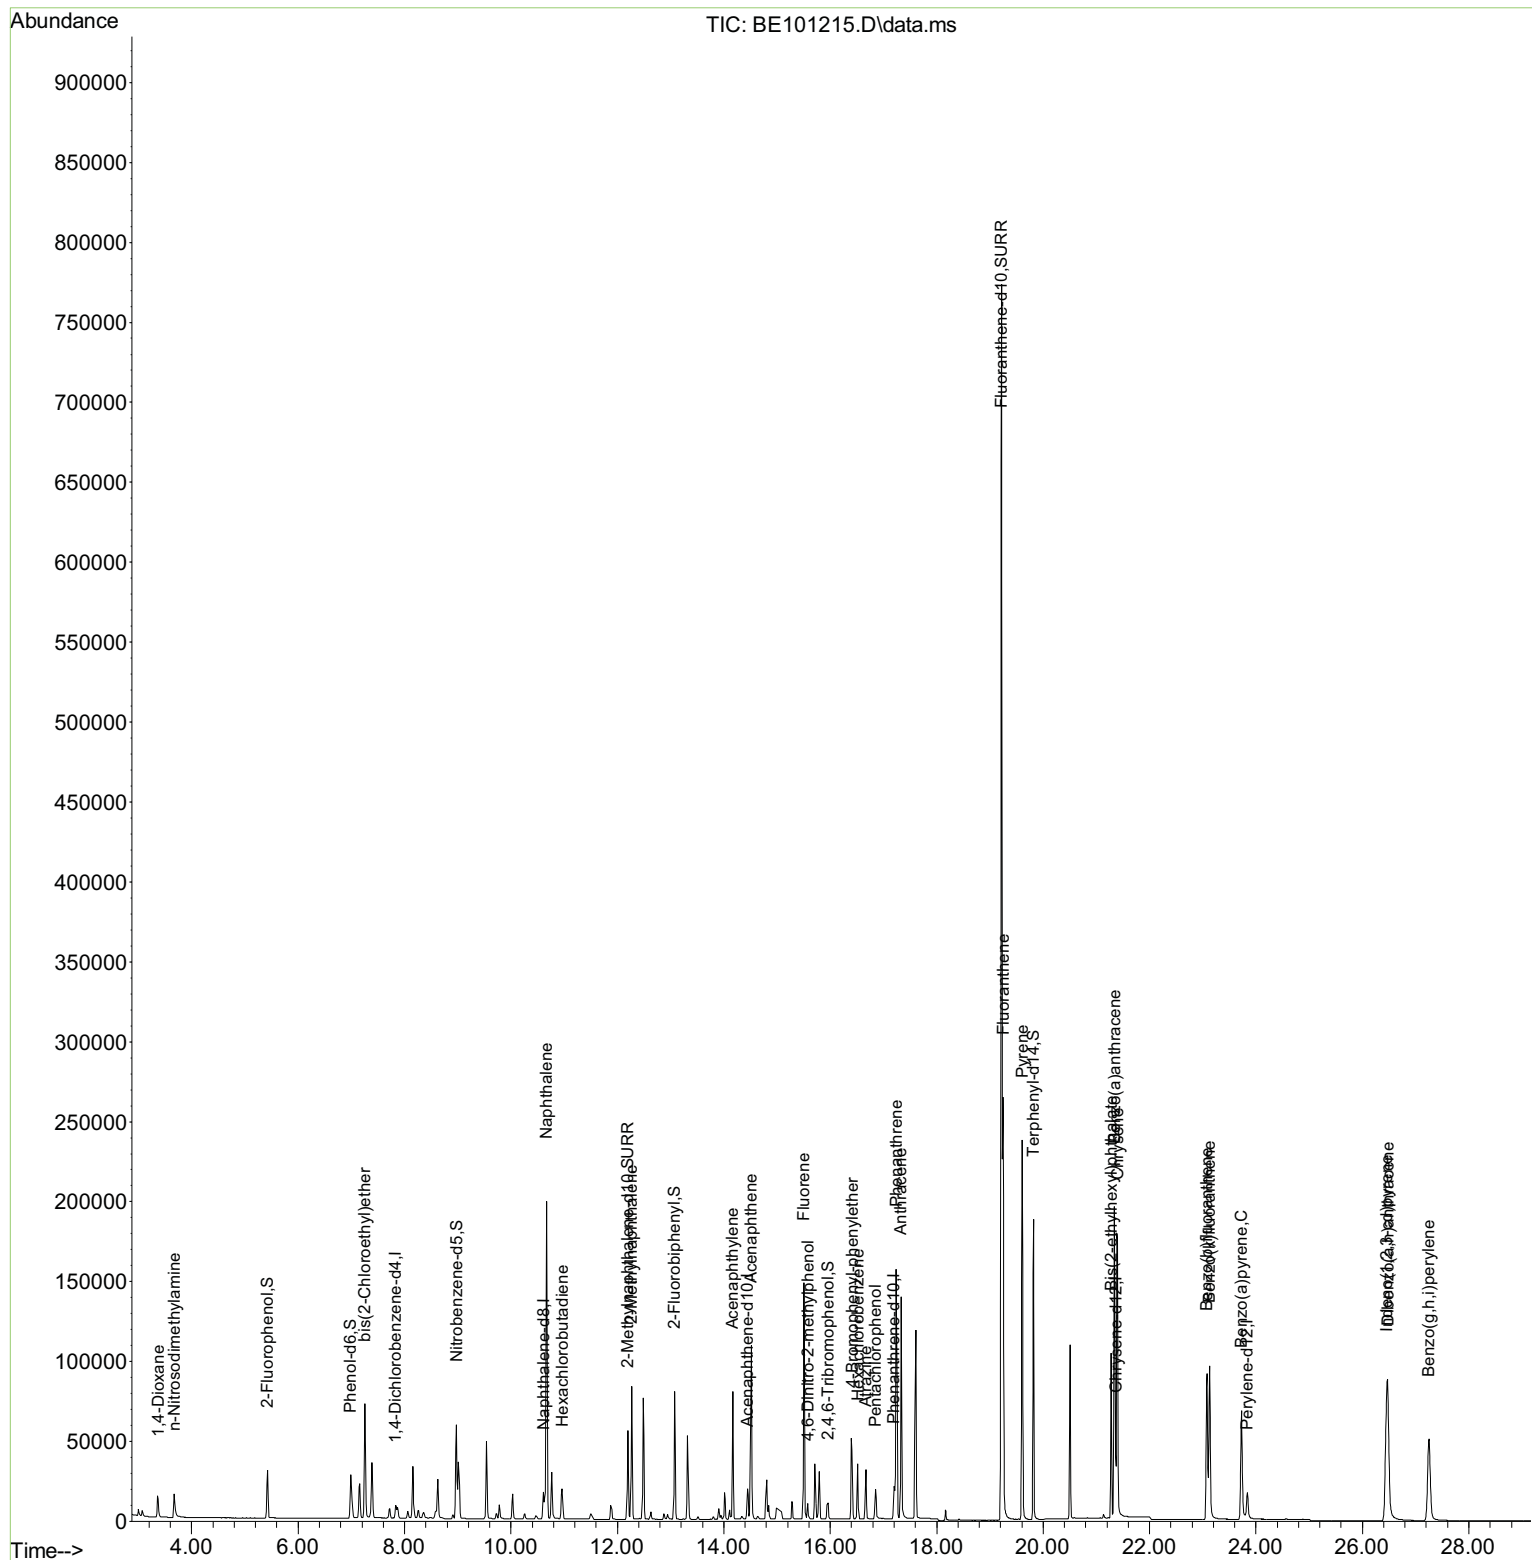


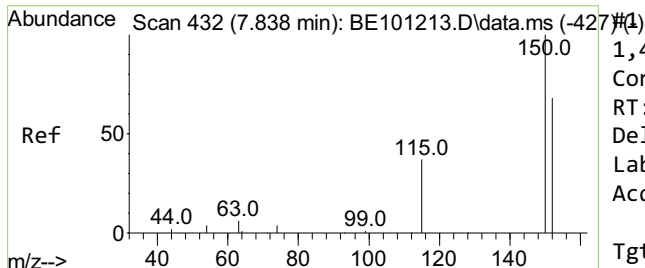

1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.829 min Scan# 431
 Delta R.T. -0.009 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:152 Resp: 3949
 Ion Ratio Lower Upper
 152 100
 150 159.5 116.9 175.3
 115 70.0 44.5 66.7#

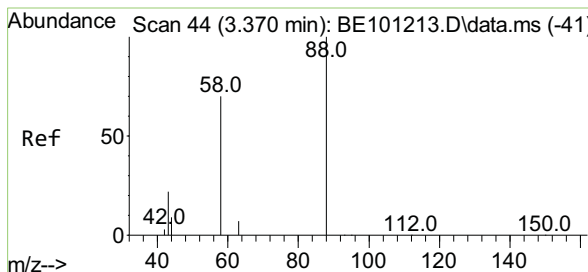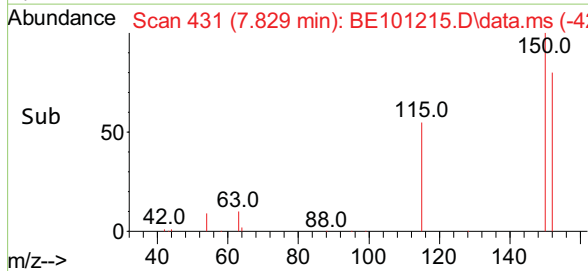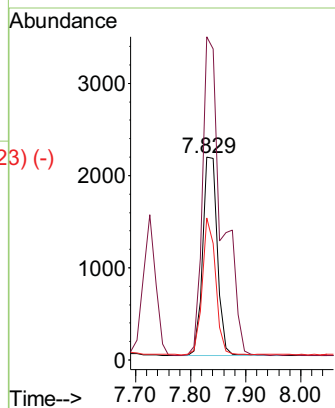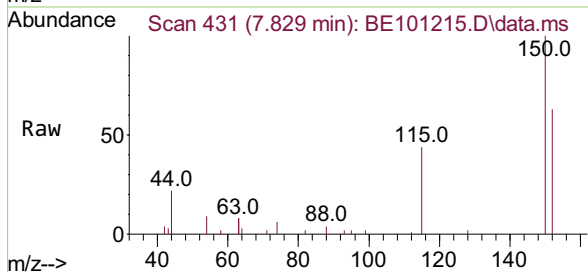

1,4-Dioxane
 Concen: 1.34 ng
 RT: 3.372 min Scan# 44
 Delta R.T. 0.002 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15

Tgt Ion: 88 Resp: 9376
 Ion Ratio Lower Upper
 88 100
 58 89.5 73.6 110.4
 43 33.9 27.6 41.4

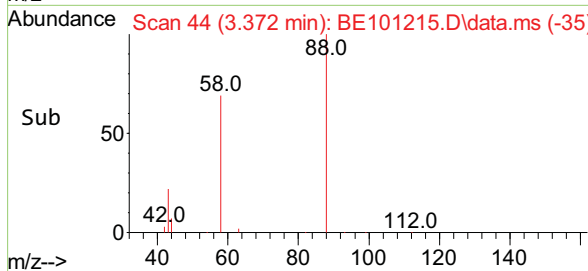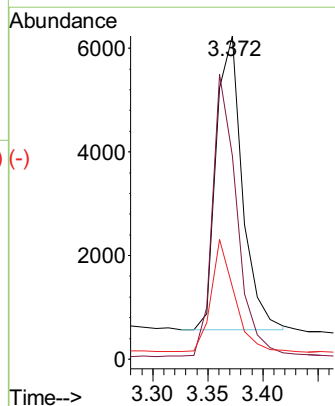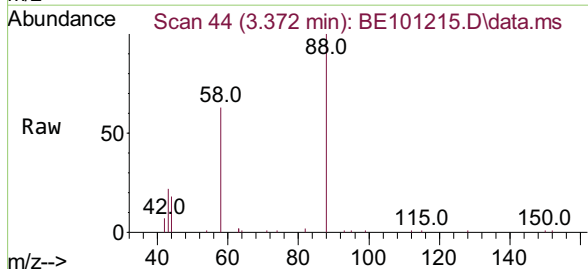




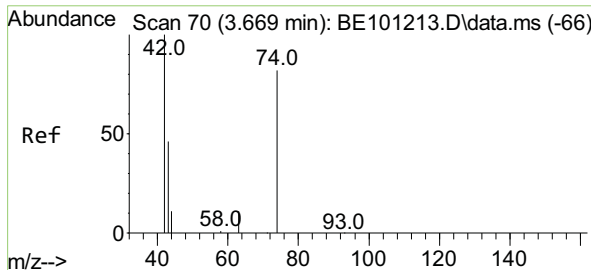


n-Nitrosodimethylamine
 Concen: 1.53 ng
 RT: 3.671 min Scan# 70
 Delta R.T. 0.002 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC1.6

Tgt Ion: 42 Resp: 10941




Ion	Ratio	Lower	Upper
42	100		
74	109.9	92.7	139.1
44	9.2	10.7	16.1#

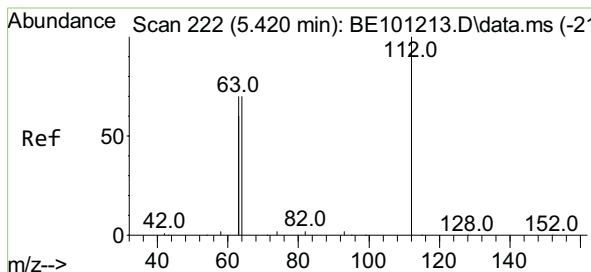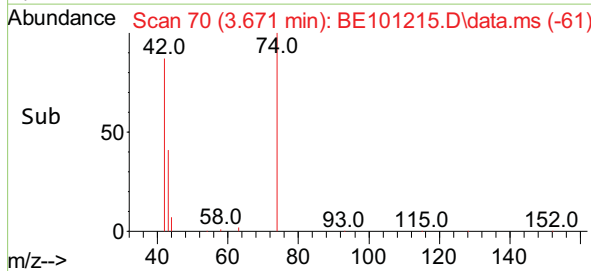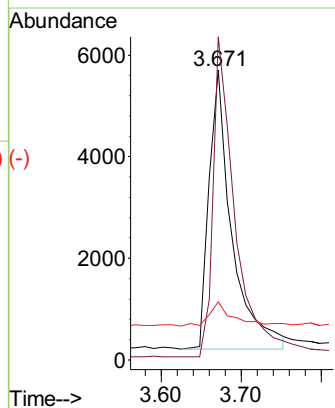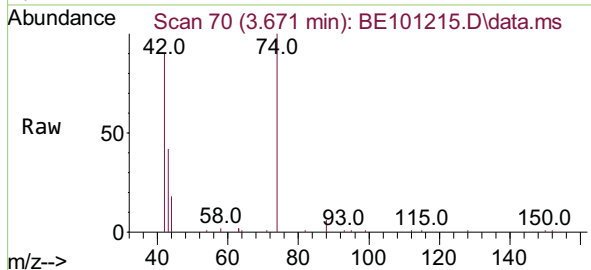


2-Fluorophenol
 Concen: 1.37 ng
 RT: 5.422 min Scan# 222
 Delta R.T. 0.002 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15

Tgt Ion: 112 Resp: 14716

Ion	Ratio	Lower	Upper
112	100		
64	75.6	62.3	93.5
63	146.9	117.3	175.9


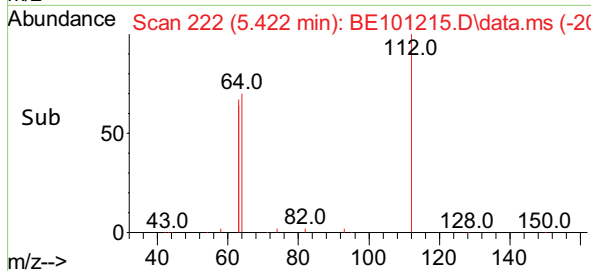
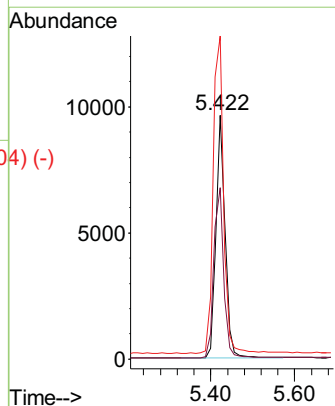
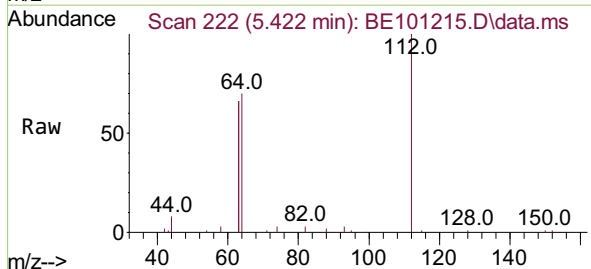


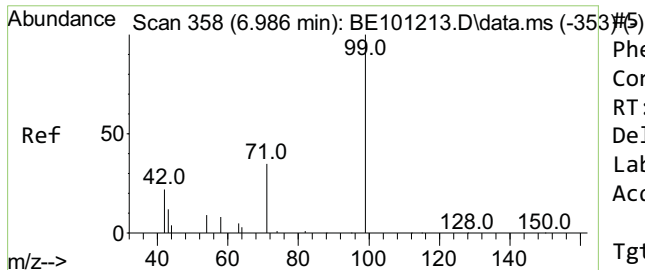

Phenol-d6
 Concen: 1.47 ng
 RT: 6.988 min Scan# 358
 Delta R.T. 0.002 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:	99	Resp:	23283
Ion	Ratio	Lower	Upper
99	100		
42	23.3	18.5	27.7
71	33.5	26.5	39.7

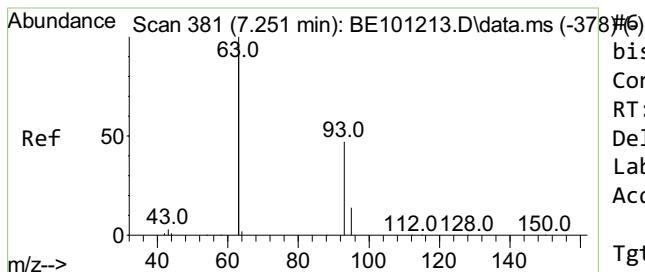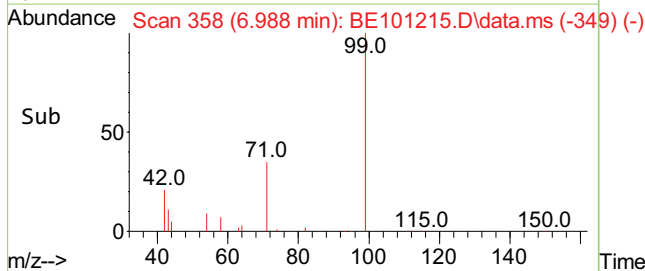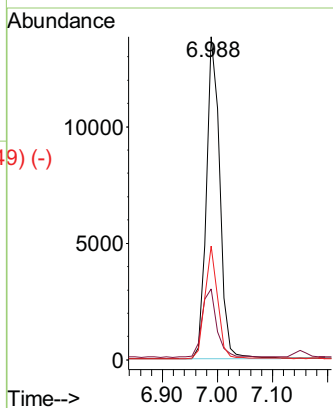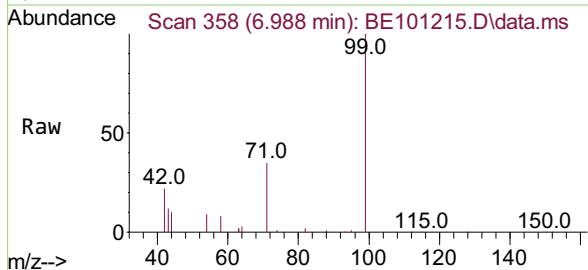


bis(2-Chloroethyl)ether
 Concen: 1.69 ng
 RT: 7.253 min Scan# 381
 Delta R.T. 0.002 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15

Tgt Ion:	93	Resp:	21929
Ion	Ratio	Lower	Upper
93	100		
63	366.3	292.5	438.7
95	32.0	25.7	38.5

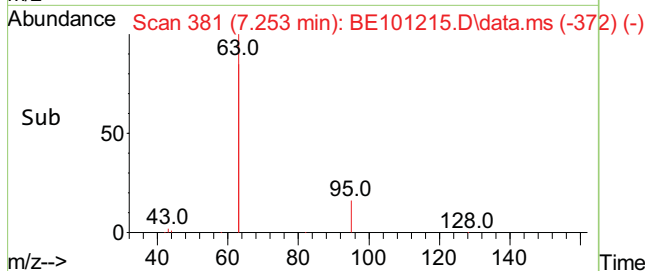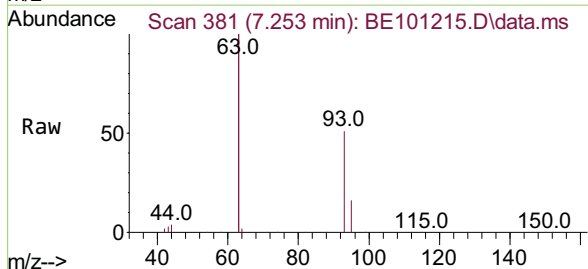




Abundance Scan 650 (10.615 min): BE101213.D\data.ms (-6457-)

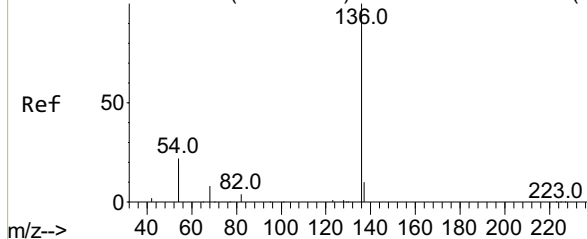


Naphthalene-d8
Concen: 0.40 ng
RT: 10.614 min Scan# 650
Delta R.T. -0.001 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

Tgt Ion:	136	Resp:	17728
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.6	13.0
54	42.3	34.7	52.1
68	8.9	7.0	10.4

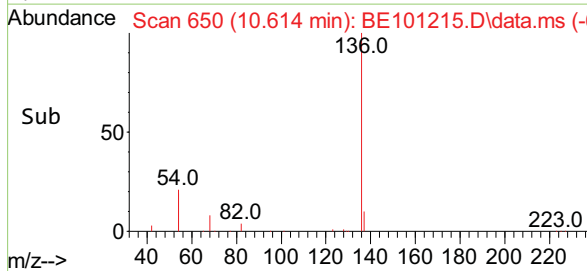
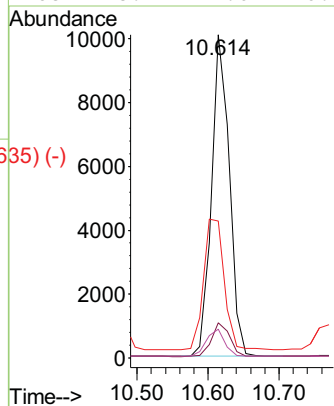
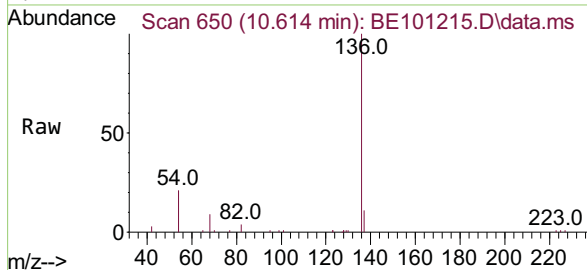


Abundance Scan 524 (8.978 min): BE101213.D\data.ms (-52178)

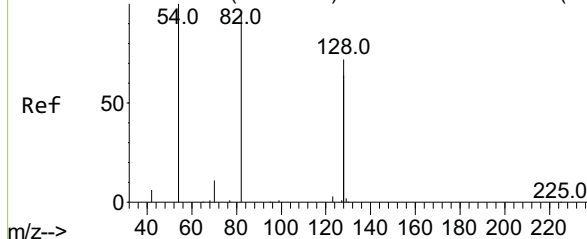


Nitrobenzene-d5
Concen: 1.56 ng
RT: 8.977 min Scan# 524
Delta R.T. -0.001 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Tgt Ion:	82	Resp:	21805
Ion	Ratio	Lower	Upper
82	100		
128	137.9	118.7	178.1
54	206.5	164.4	246.6

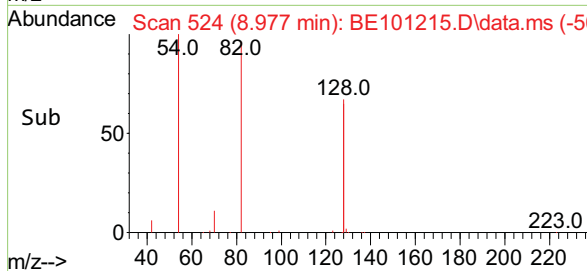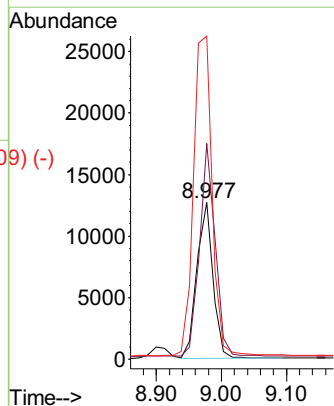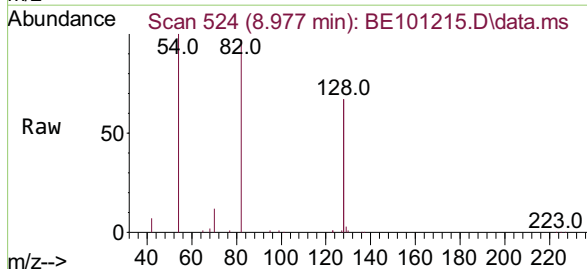



Abundance Scan 654 (10.667 min): BE101213.D\data.ms (-644) (-)




Naphthalene
Concen: 1.62 ng
RT: 10.666 min Scan# 654
Delta R.T. -0.001 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6


Tgt Ion:	128	Resp:	310218
Ion	Ratio	Lower	Upper
128	100		
129	2.7	2.2	3.4
127	3.2	2.6	3.8

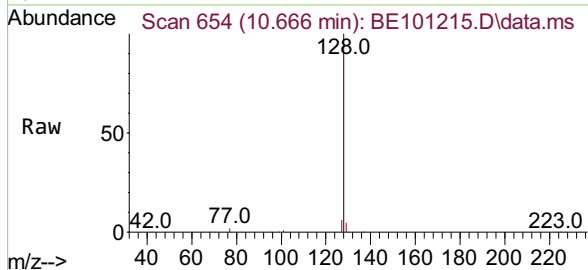

Abundance Scan 654 (10.666 min): BE101215.D\data.ms (-646) (-)


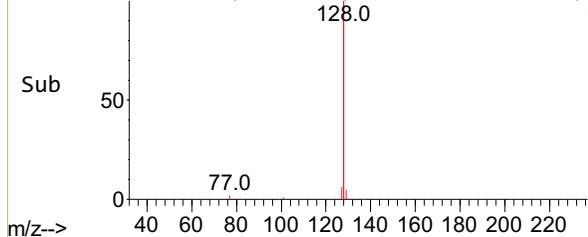


Abundance Scan 677 (10.965 min): BE101213.D\data.ms (-672) (-)





Hexachlorobutadiene
Concen: 1.59 ng
RT: 10.965 min Scan# 677
Delta R.T. -0.001 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Tgt Ion:	225	Resp:	13516
Ion	Ratio	Lower	Upper
225	100		
223	62.3	50.4	75.6
227	64.8	50.1	75.1

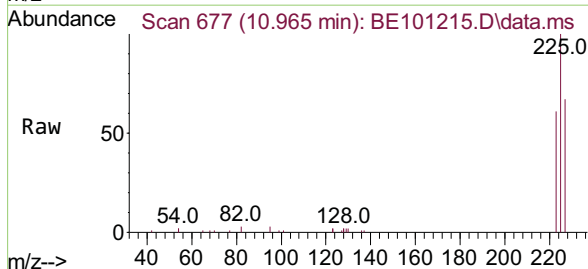

Abundance Scan 677 (10.965 min): BE101215.D\data.ms (-669) (-)







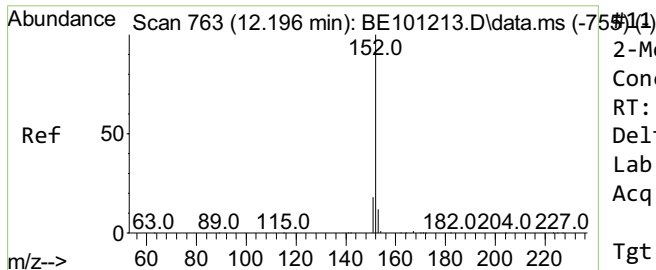

2-Methylnaphthalene-d10
 Concen: 1.69 ng
 RT: 12.195 min Scan# 763
 Delta R.T. -0.001 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:152 Resp: 66974
 Ion Ratio Lower Upper
 152 100
 151 20.4 16.5 24.7

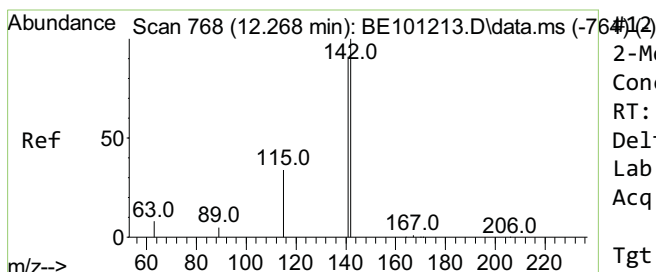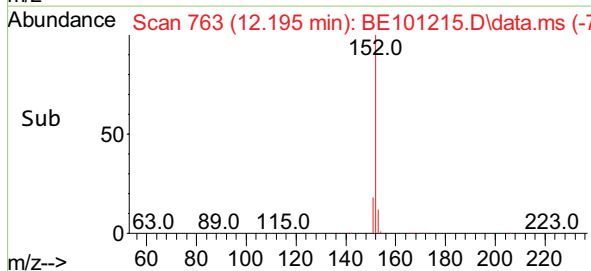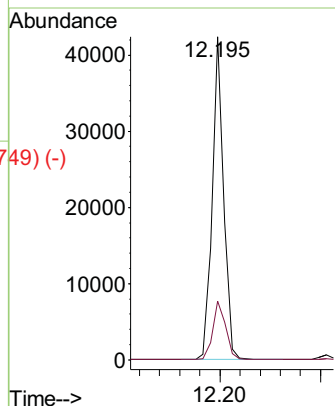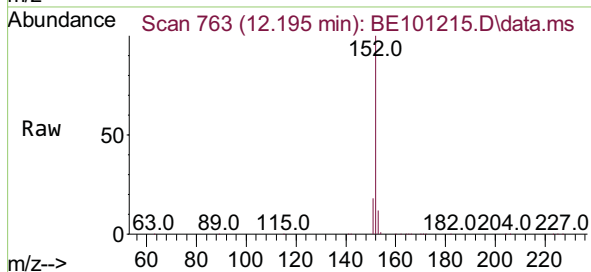

2-Methylnaphthalene
 Concen: 1.69 ng
 RT: 12.267 min Scan# 768
 Delta R.T. -0.001 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15

Tgt Ion:142 Resp: 56327
 Ion Ratio Lower Upper
 142 100
 141 89.0 73.0 109.6
 115 33.9 27.8 41.8


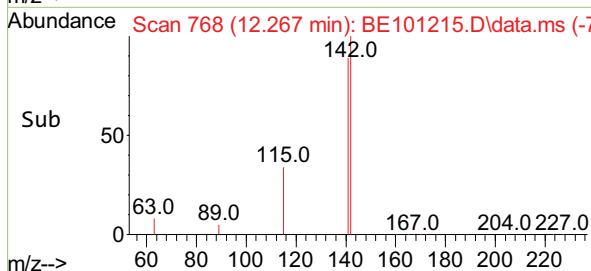
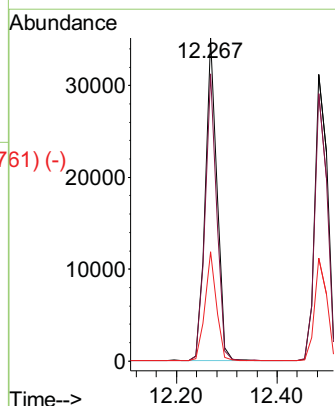
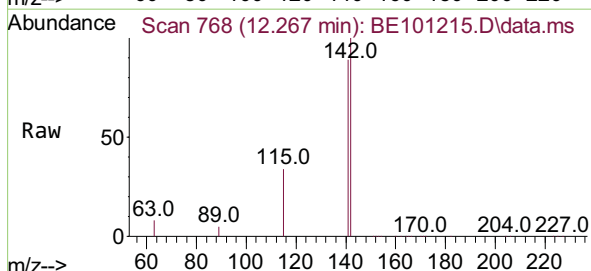


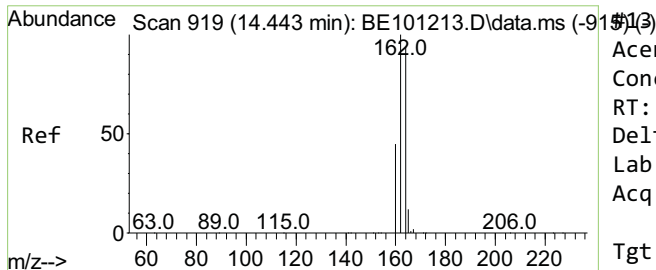

Acenaphthene-d10
 Concen: 0.40 ng
 RT: 14.443 min Scan# 919
 Delta R.T. -0.001 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:	164	Resp:	12614
Ion	Ratio	Lower	Upper
164	100		
162	106.8	85.3	127.9
160	49.6	39.1	58.7

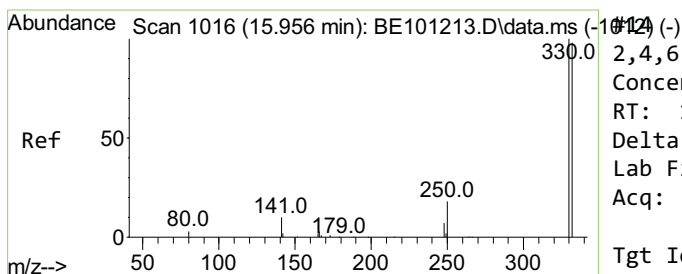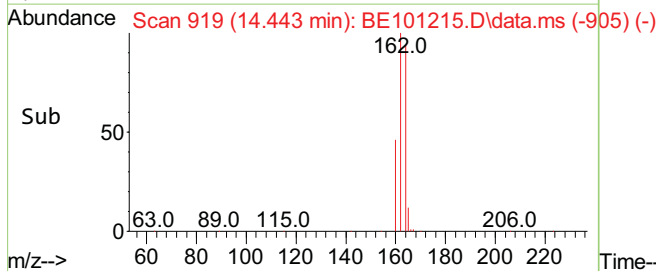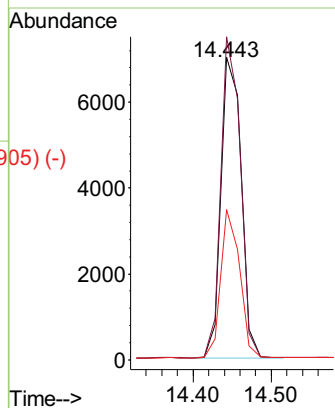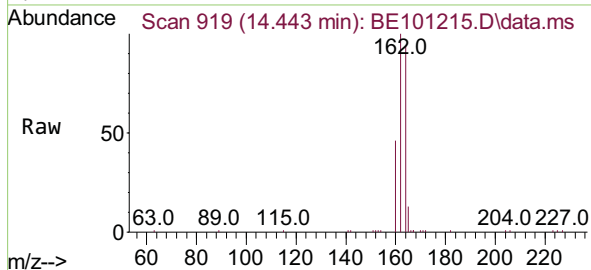

2,4,6-Tribromophenol
 Concen: 1.69 ng
 RT: 15.956 min Scan# 1016
 Delta R.T. 0.001 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15

Tgt Ion:	330	Resp:	6664
Ion	Ratio	Lower	Upper
330	100		
332	97.9	77.8	116.6
141	40.2	30.4	45.6


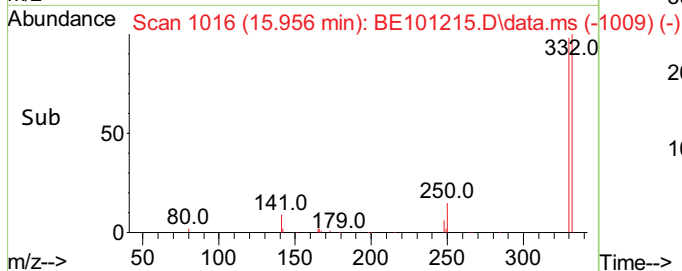
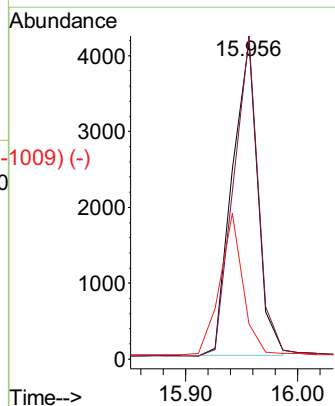
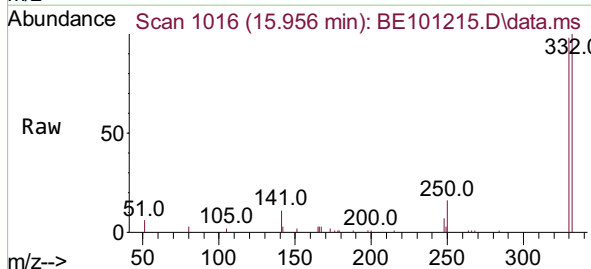


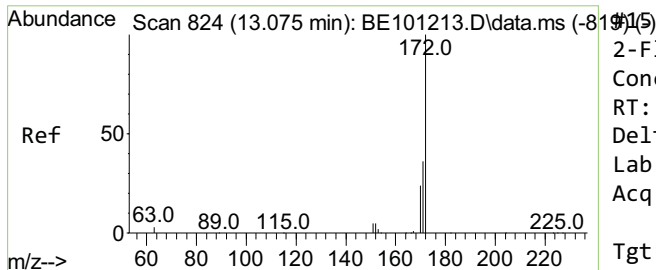

2-Fluorobiphenyl
 Concen: 1.61 ng
 RT: 13.074 min Scan# 824
 Delta R.T. -0.001 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:	172	Resp:	73789
Ion	Ratio	Lower	Upper
172	100		
171	35.1	28.7	43.1
170	23.7	19.3	28.9

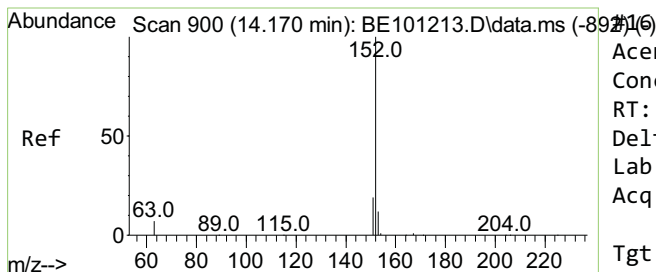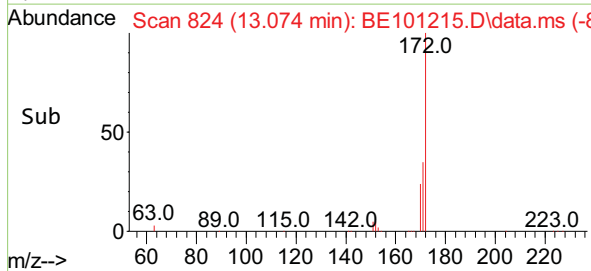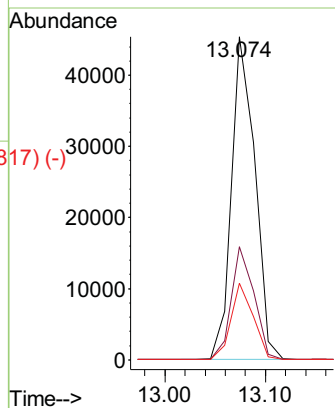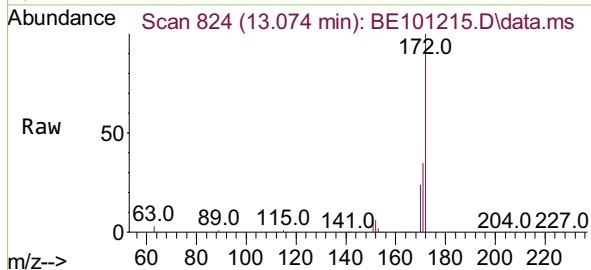


Acenaphthylene
 Concen: 1.70 ng
 RT: 14.169 min Scan# 900
 Delta R.T. -0.001 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15

Tgt Ion:	152	Resp:	85545
Ion	Ratio	Lower	Upper
152	100		
151	19.2	15.4	23.2
153	13.1	10.0	15.0

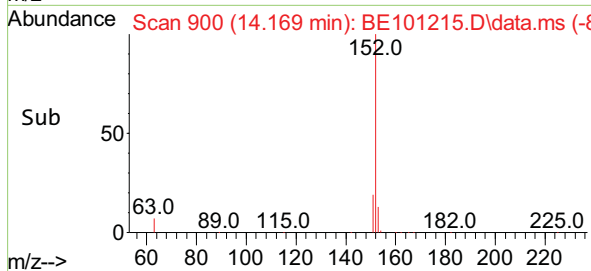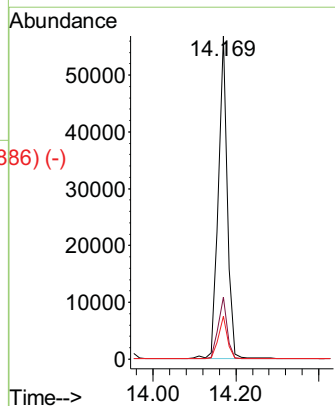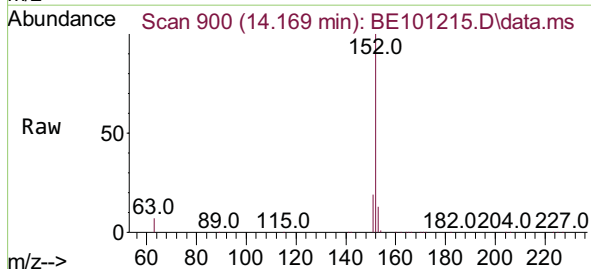




Abundance Scan 924 (14.515 min): BE101213.D\data.ms (-917) #17




Acenaphthene
Concen: 1.67 ng
RT: 14.515 min Scan# 924
Delta R.T. -0.001 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

Tgt Ion:	154	Resp:	61401
Ion	Ratio	Lower	Upper
154	100		
153	104.9	84.9	127.3
152	52.5	42.7	64.1

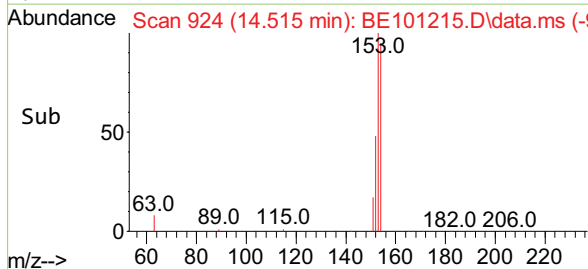
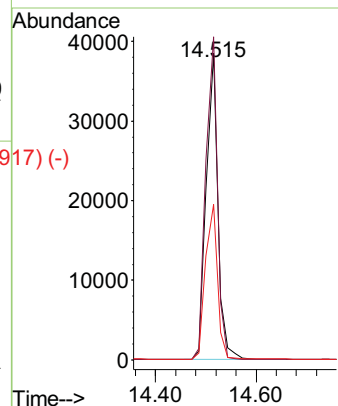
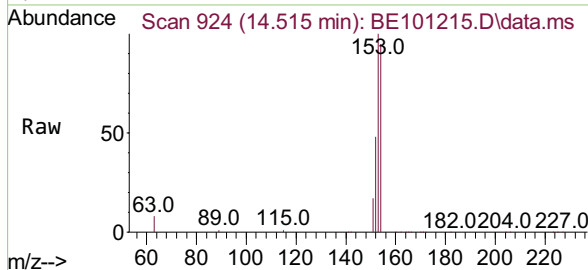


Abundance Scan 986 (15.502 min): BE101213.D\data.ms (-982) #18

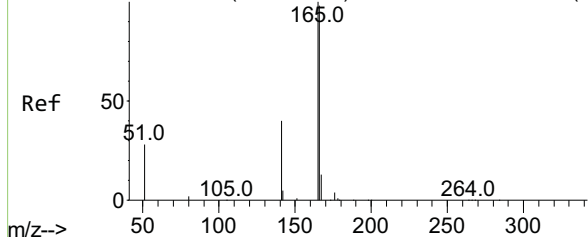

Fluorene
Concen: 1.75 ng
RT: 15.503 min Scan# 986
Delta R.T. 0.001 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15


Tgt Ion:	166	Resp:	82700
Ion	Ratio	Lower	Upper
166	100		
165	97.1	79.0	118.4
167	13.5	11.0	16.4

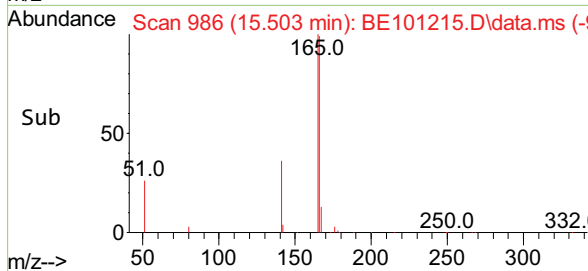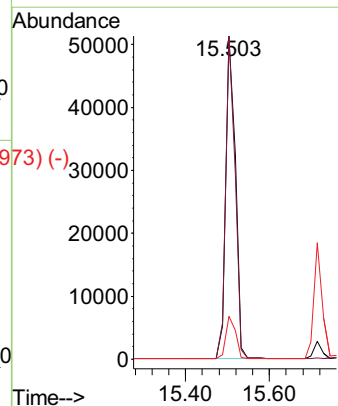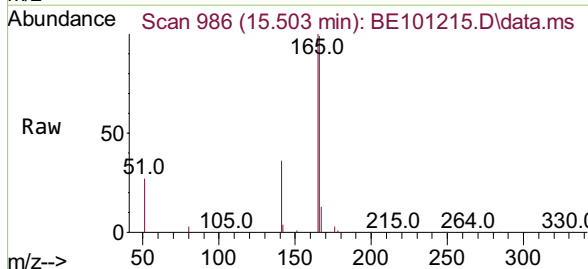




Abundance Scan 1099 (17.211 min): BE101213.D\data.ms (-1014) (-)

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.196 min Scan# 1098
Delta R.T. -0.014 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

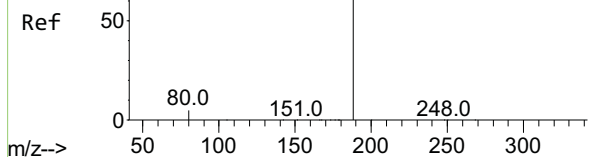




Tgt Ion:	188	Resp:	33318
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	16.8	4.6	6.8#

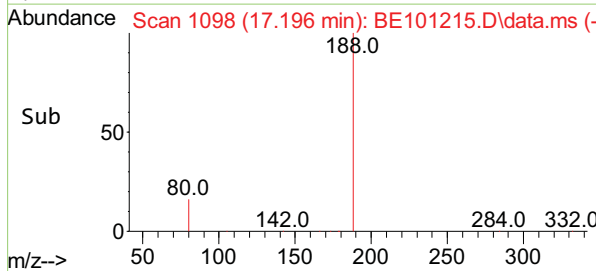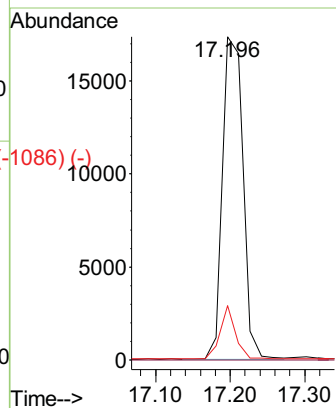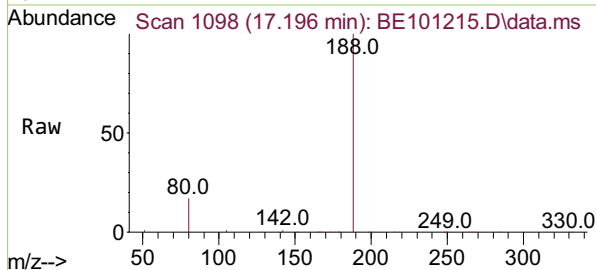


Abundance Scan 991 (15.578 min): BE101213.D\data.ms (-984) (-)

4,6-Dinitro-2-methylphenol
Concen: 1.77 ng
RT: 15.578 min Scan# 991
Delta R.T. 0.001 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Tgt Ion:	198	Resp:	7612
Ion	Ratio	Lower	Upper
198	100		
51	41.3	55.9	83.9#
105	34.0	33.6	50.4

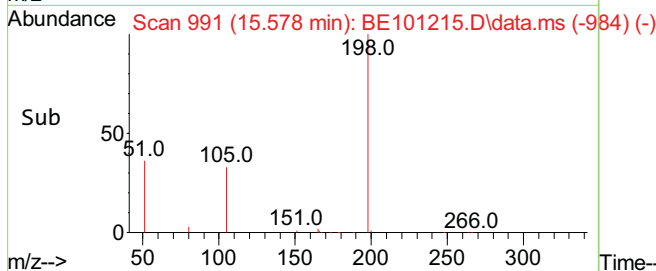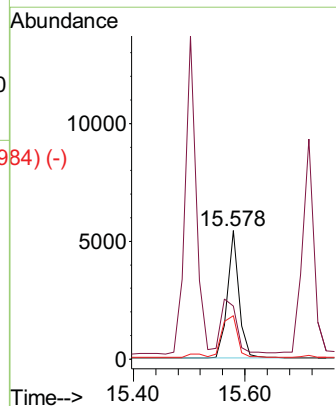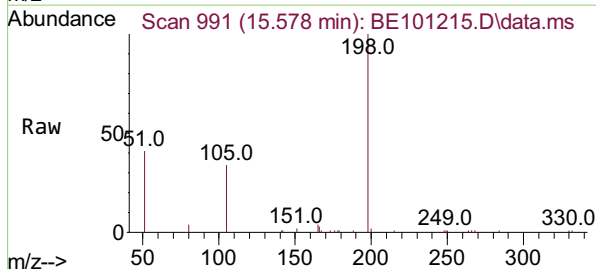




Abundance Scan 1046 (16.409 min): BE101213.D\data.ms (-1042) (-)

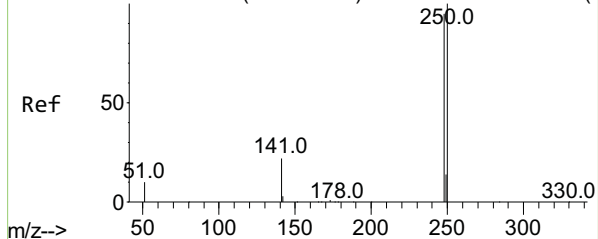


4-Bromophenyl-phenylether
Concen: 1.62 ng
RT: 16.410 min Scan# 1046
Delta R.T. 0.001 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

Tgt Ion:	248	Resp:	28095
Ion	Ratio	Lower	Upper
248	100		
250	107.3	84.5	126.7
141	20.6	19.8	29.8

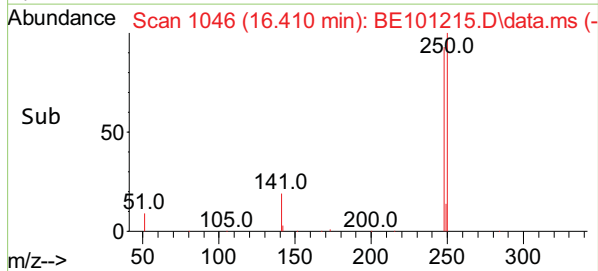
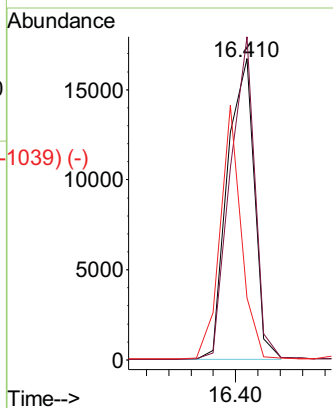
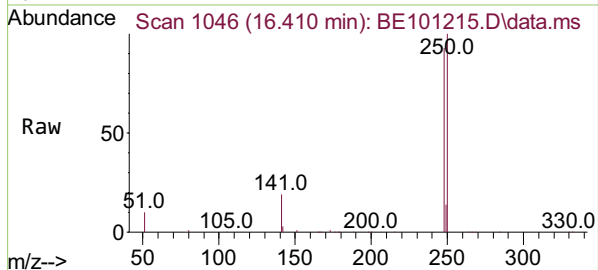


Abundance Scan 1053 (16.515 min): BE101213.D\data.ms (-1049) (-)

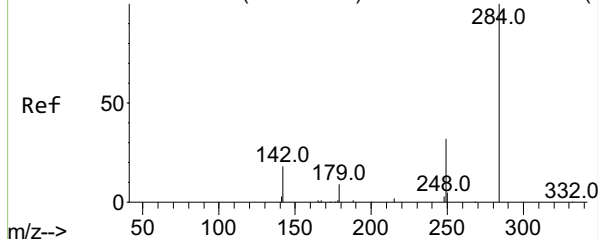

Hexachlorobenzene
Concen: 1.57 ng
RT: 16.516 min Scan# 1053
Delta R.T. 0.001 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15


Tgt Ion:	284	Resp:	27553
Ion	Ratio	Lower	Upper
284	100		
142	34.0	27.4	41.0
249	33.8	26.5	39.7

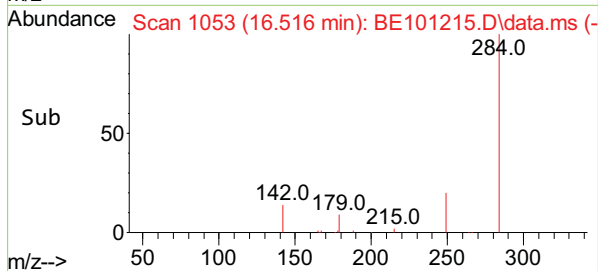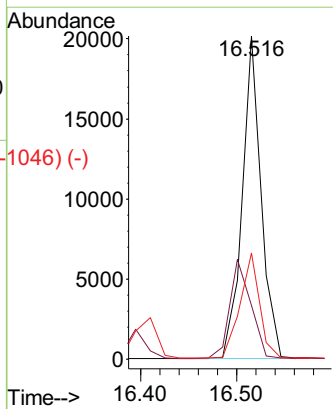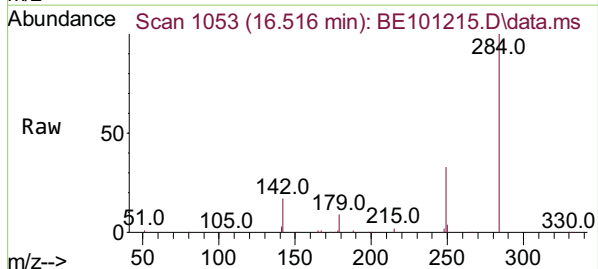




Abundance Scan 1063 (16.666 min): BE101213.D\data.ms (-1029) (-)

Atrazine
Concen: 1.67 ng
RT: 16.667 min Scan# 1063
Delta R.T. 0.001 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

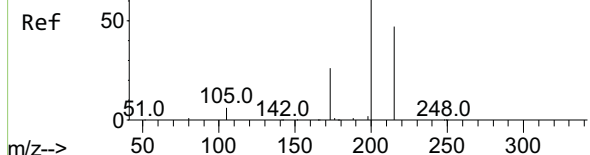


Tgt Ion:	200	Resp:	22324
Ion	Ratio	Lower	Upper
200	100		
173	25.5	21.9	32.9
215	48.7	38.6	57.8

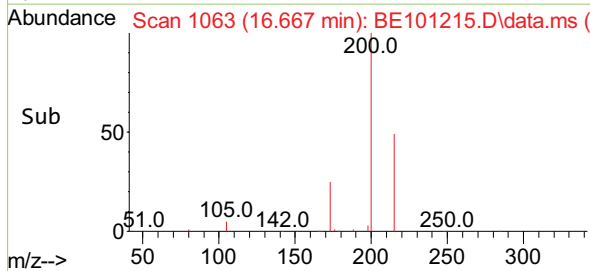
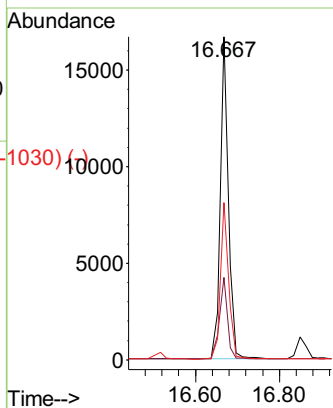
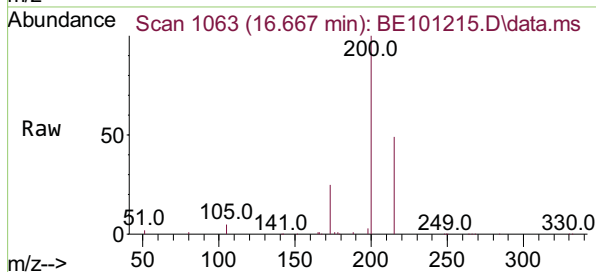



Abundance Scan 1076 (16.863 min): BE101213.D\data.ms (-1024) (-)

Pentachlorophenol
Concen: 1.49 ng
RT: 16.849 min Scan# 1075
Delta R.T. -0.014 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

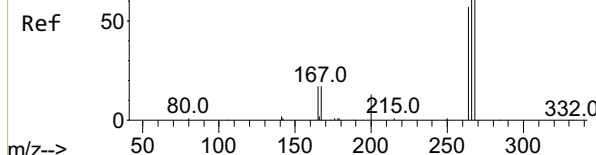

Tgt Ion:	266	Resp:	10279
Ion	Ratio	Lower	Upper
266	100		
264	62.9	49.1	73.7
268	65.3	50.6	76.0


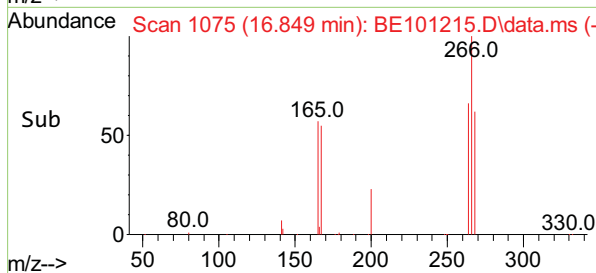

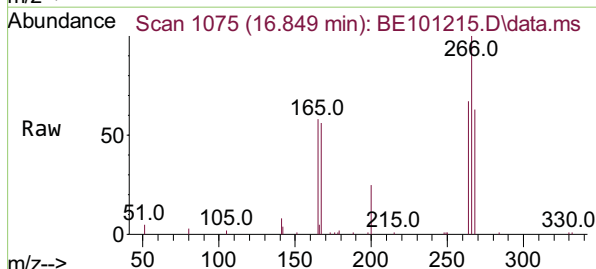


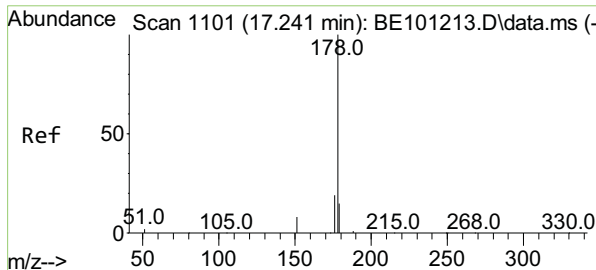

Scan 1101 (17.241 min): BE101213.D\data.ms (-1025) (-)
 Phenanthrene
 Concen: 1.64 ng
 RT: 17.242 min Scan# 1101
 Delta R.T. 0.001 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:	178	Resp:	161530
Ion	Ratio	Lower	Upper
178	100		
176	19.1	15.0	22.6
179	15.3	12.2	18.4

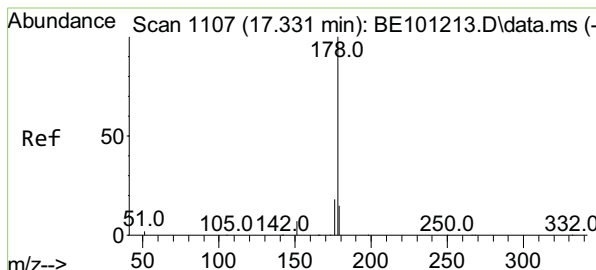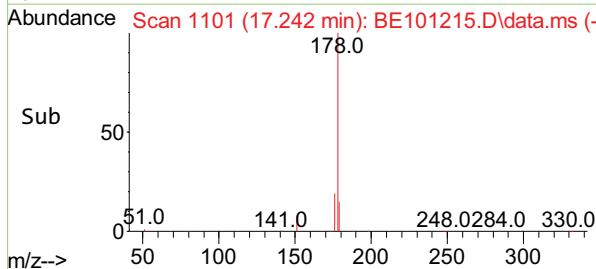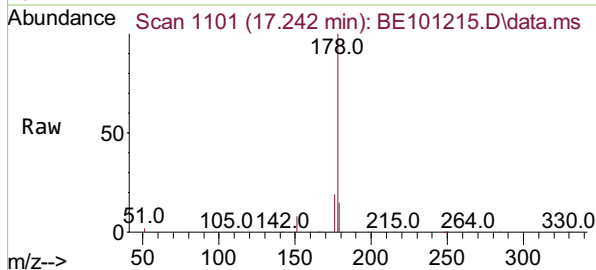

Scan 1107 (17.331 min): BE101213.D\data.ms (-1025) (-)
 Anthracene
 Concen: 1.72 ng
 RT: 17.332 min Scan# 1107
 Delta R.T. 0.001 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15


Tgt Ion:	178	Resp:	146311
Ion	Ratio	Lower	Upper
178	100		
176	18.2	14.4	21.6
179	15.2	11.8	17.8

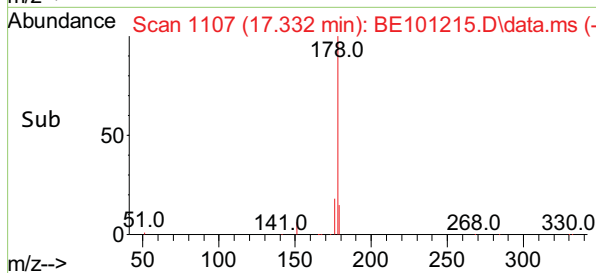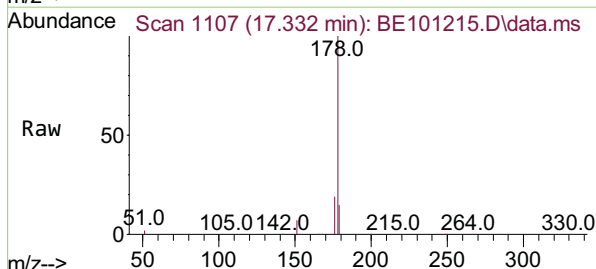

Abundance Scan 1359 (19.220 min): BE101213.D\data.ms (-1327) (-)




Fluoranthene-d10
Concen: 1.75 ng
RT: 19.219 min Scan# 1359
Delta R.T. -0.001 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

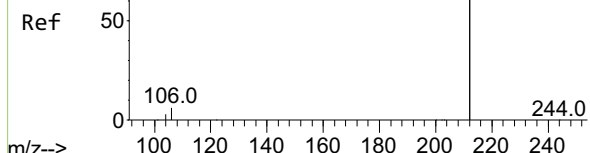

Tgt Ion:212 Resp: 1004172

Ion	Ratio	Lower	Upper
212	100		
106	3.4	2.6	4.0
104	1.9	1.4	2.2


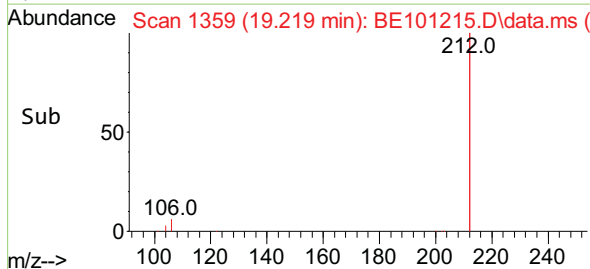

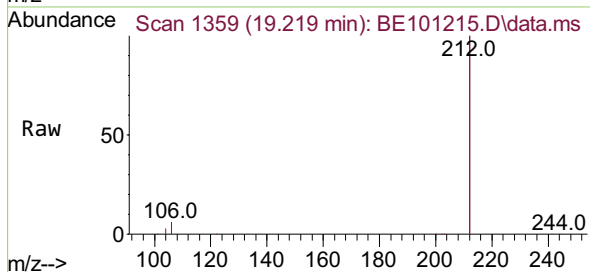



Abundance Scan 1364 (19.249 min): BE101213.D\data.ms (-1328) (-)

Fluoranthene
Concen: 1.81 ng
RT: 19.248 min Scan# 1364
Delta R.T. -0.001 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Tgt Ion:202 Resp: 227062

Ion	Ratio	Lower	Upper
202	100		
101	11.7	9.1	13.7
203	17.6	13.6	20.4

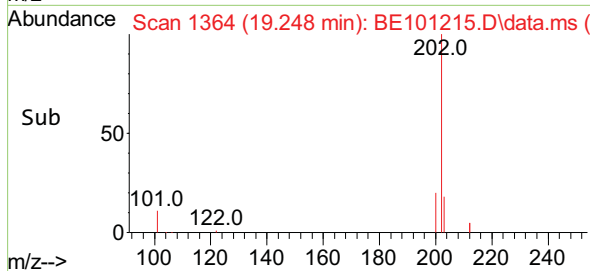

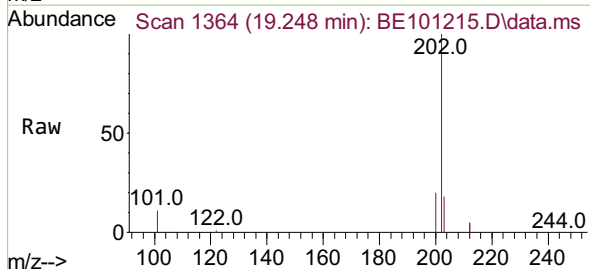
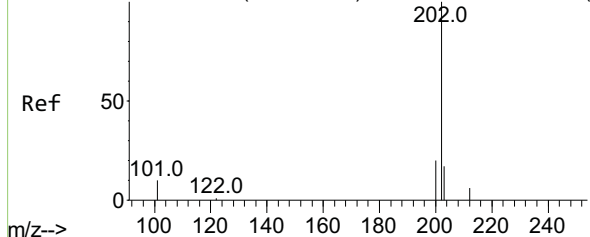


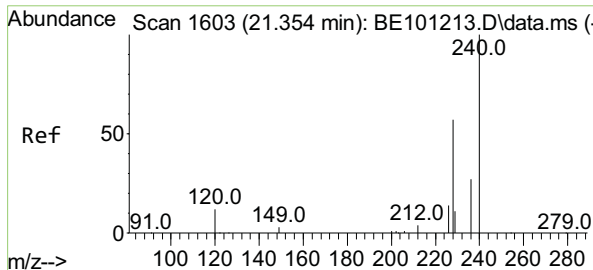

Chrysene-d12
 Concen: 0.40 ng
 RT: 21.366 min Scan# 1605
 Delta R.T. 0.012 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:	240	Resp:	34536
Ion	Ratio	Lower	Upper
240	100		
120	3.9	10.2	15.4#
236	25.2	21.7	32.5

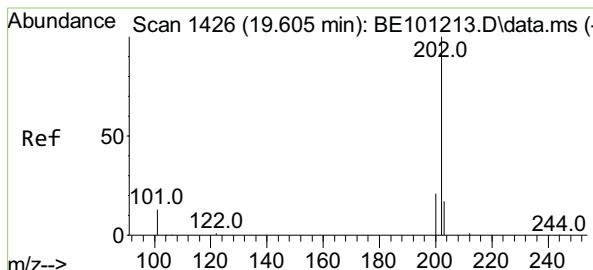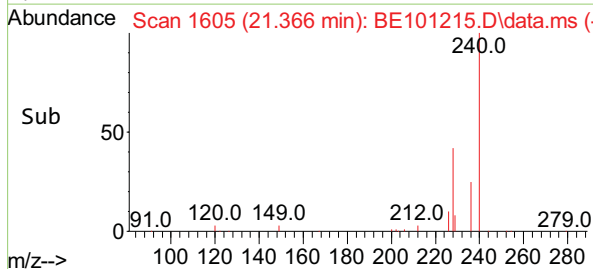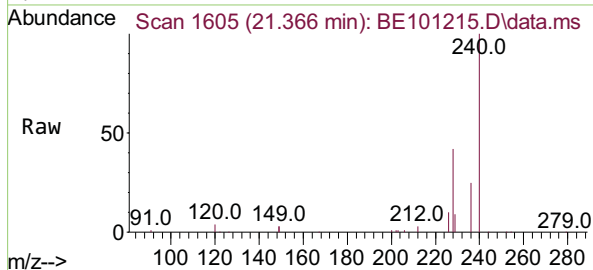

Pyrene
 Concen: 2.21 ng
 RT: 19.610 min Scan# 1427
 Delta R.T. 0.005 min
 Lab File: BE101215.D
 Acq: 6 Apr 2021 14:15

Tgt Ion:	202	Resp:	222245
Ion	Ratio	Lower	Upper
202	100		
200	20.9	16.6	24.8
203	17.8	13.8	20.8

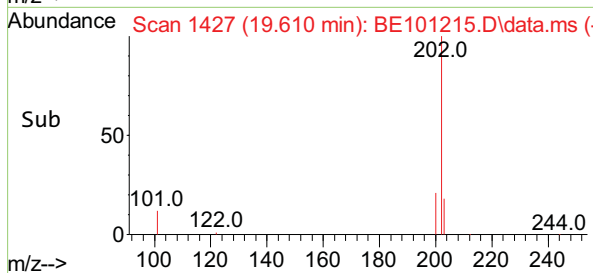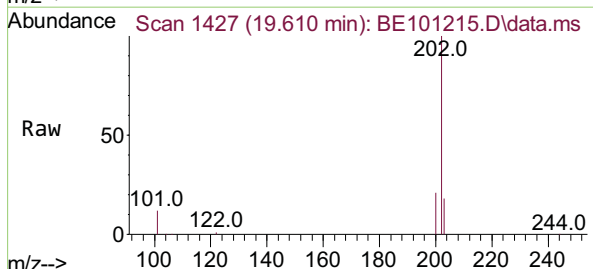

Abundance Scan 1463 (19.818 min): BE101213.D\data.ms (-1434) (-)

Terphenyl-d14

Concen: 2.14 ng

RT: 19.817 min Scan# 1463

Delta R.T. -0.001 min

Lab File: BE101215.D

Acq: 6 Apr 2021 14:15





Tgt Ion:244 Resp: 166790

Ion Ratio Lower Upper

244 100

212 27.9 21.9 32.9

122 9.9 7.3 10.9

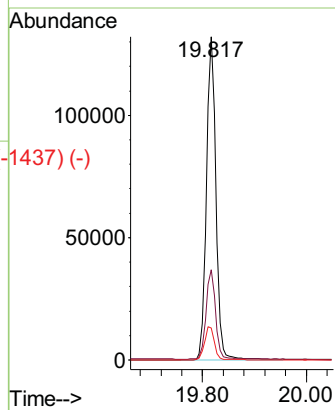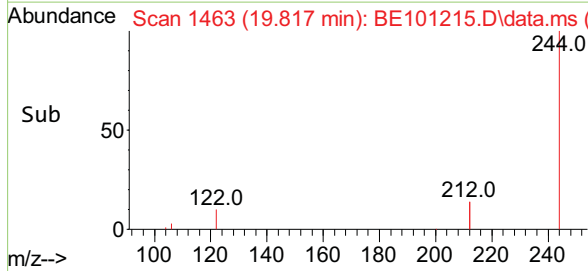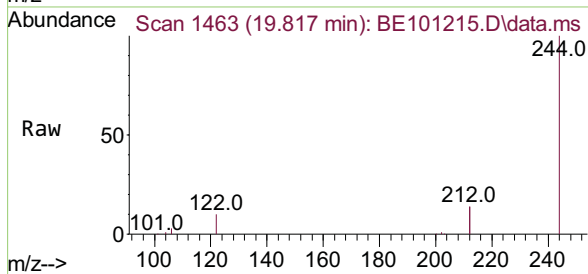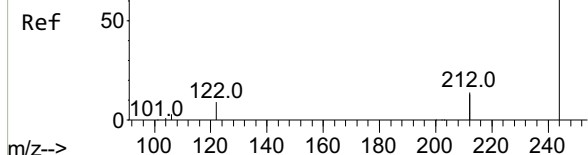

Abundance Scan 1602 (21.342 min): BE101213.D\data.ms (-1534) (-)

Benzo(a)anthracene

Concen: 1.57 ng

RT: 21.342 min Scan# 1603

Delta R.T. 0.000 min

Lab File: BE101215.D

Acq: 6 Apr 2021 14:15




Tgt Ion:228 Resp: 163361

Ion Ratio Lower Upper

228 100

226 27.4 21.4 32.2

229 19.6 15.7 23.5

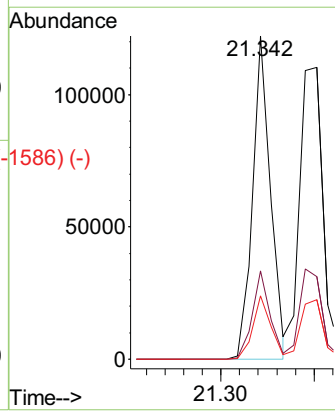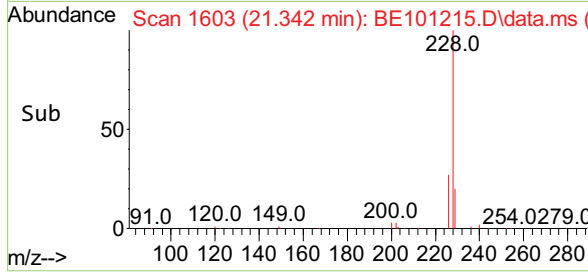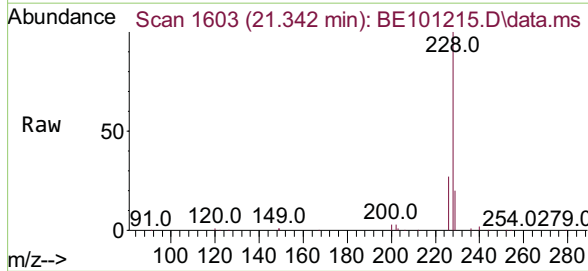


Instrument :

BNA_E


ClientSampleId :

SSTDICC1.6



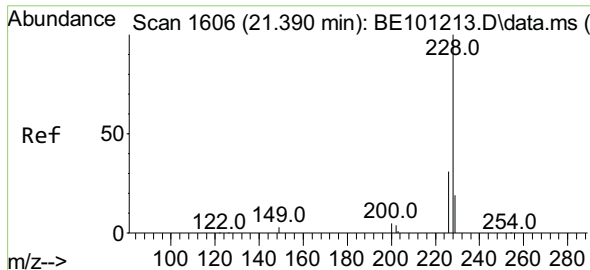


#324 (-)
Chrysene
Concen: 1.65 ng
RT: 21.403 min Scan# 1608
Delta R.T. 0.012 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15


Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

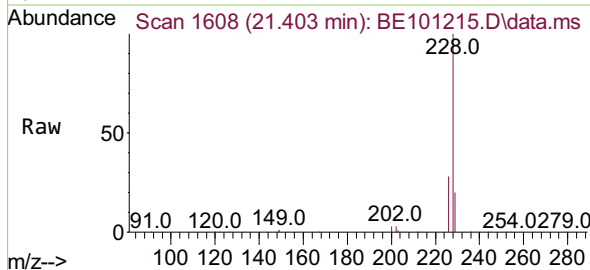



Tgt Ion:	228	Resp:	188994
Ion	Ratio	Lower	Upper
228	100		
226	28.3	24.8	37.2
229	20.4	15.2	22.8

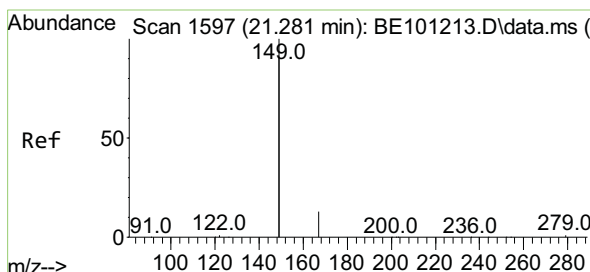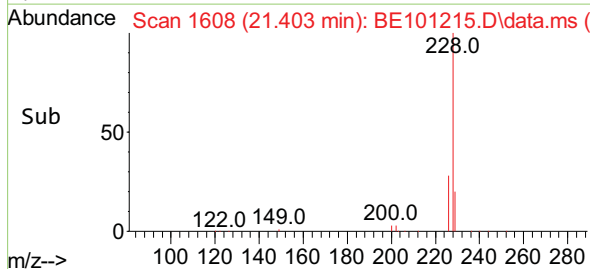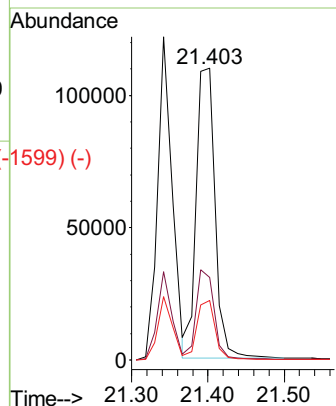


#324 (-)
Bis(2-ethylhexyl)phthalate
Concen: 0.87 ng
RT: 21.282 min Scan# 1598
Delta R.T. 0.000 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

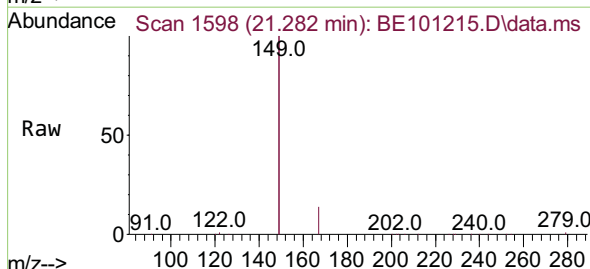

Tgt Ion:	149	Resp:	112005
Ion	Ratio	Lower	Upper
149	100		
167	6.9	5.5	8.3
279	1.1	1.0	1.4

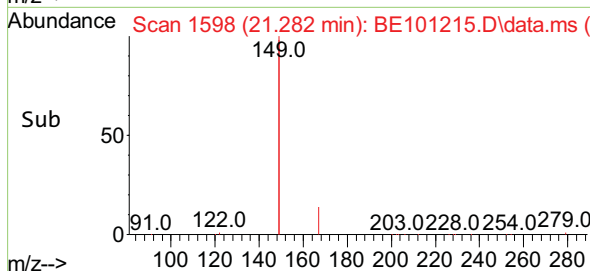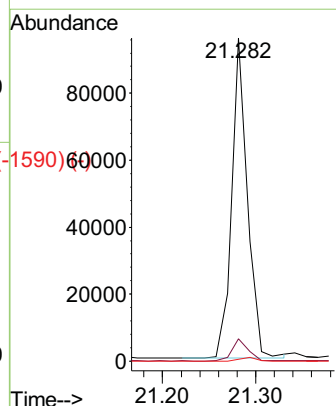



Abundance Scan 2893 (26.448 min): BE101213.D\data.ms (-2885) (-)

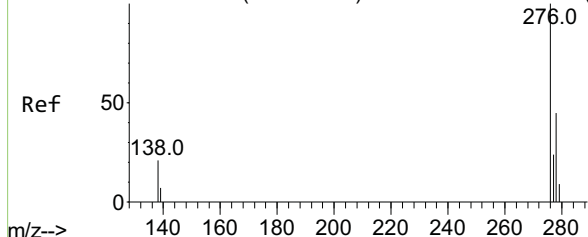


Indeno(1,2,3-cd)pyrene
Concen: 1.40 ng
RT: 26.453 min Scan# 2895
Delta R.T. 0.004 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6


Tgt Ion:	276	Resp:	141197
Ion	Ratio	Lower	Upper
276	100		
138	22.0	17.4	26.0
277	25.1	19.8	29.8

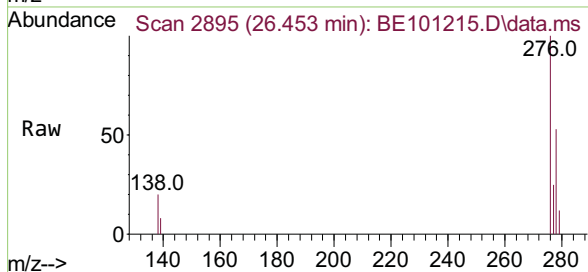

Abundance Scan 2895 (26.453 min): BE101215.D\data.ms (-2866) (-)





Abundance Scan 2165 (23.838 min): BE101213.D\data.ms (-2186) (-)

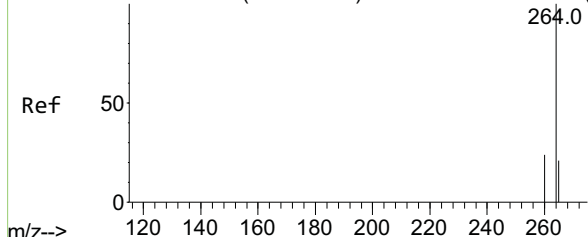


Perylene-d12
Concen: 0.40 ng
RT: 23.838 min Scan# 2166
Delta R.T. -0.000 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15


Tgt Ion:	264	Resp:	24524
Ion	Ratio	Lower	Upper
264	100		
260	24.7	19.3	28.9
265	27.1	22.4	33.6

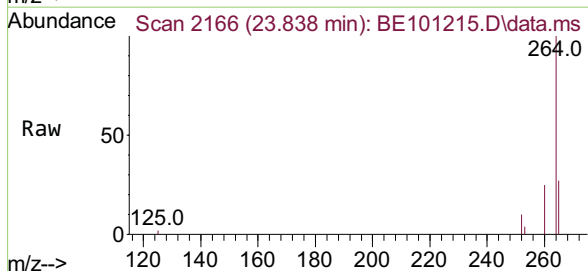

Abundance Scan 2166 (23.838 min): BE101215.D\data.ms (-2124) (-)





Abundance Scan 1951 (23.075 min): BE101213.D\data.ms (-1937) (-)




Benzo(b)fluoranthene
Concen: 1.76 ng
RT: 23.078 min Scan# 1953
Delta R.T. 0.003 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Tgt Ion:	252	Resp:	131990
Ion	Ratio	Lower	Upper
252	100		
253	22.2	18.1	27.1
125	8.6	7.6	11.4


Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

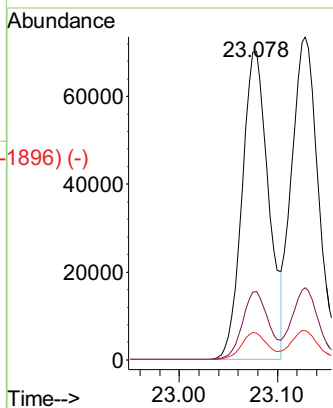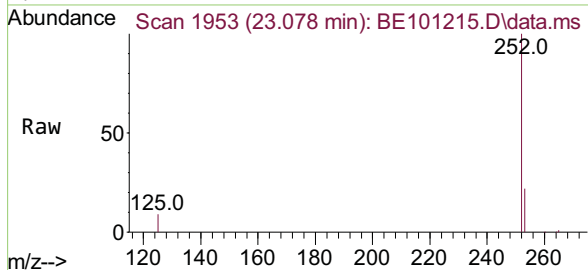

Abundance Scan 1953 (23.078 min): BE101215.D\data.ms (-1896) (-)





Abundance Scan 1965 (23.125 min): BE101213.D\data.ms (-1938) (-)




Benzo(k)fluoranthene
Concen: 1.71 ng
RT: 23.128 min Scan# 1967
Delta R.T. 0.003 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15


Tgt Ion:	252	Resp:	145334
Ion	Ratio	Lower	Upper
252	100		
253	22.3	17.8	26.6
125	9.1	7.6	11.4

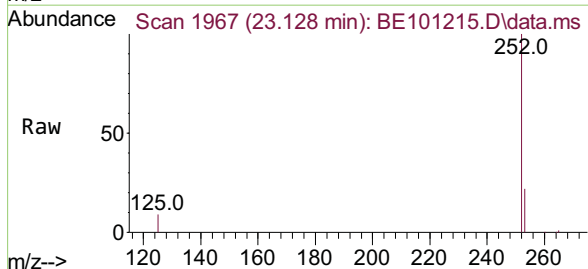

Abundance Scan 1967 (23.128 min): BE101215.D\data.ms (-1882) (-)






Abundance Scan 2133 (23.724 min): BE101213.D\data.ms (-2#89) (-)




Benzo(a)pyrene
Concen: 1.77 ng
RT: 23.727 min Scan# 2135
Delta R.T. 0.003 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

Tgt Ion:252 Resp: 117573
Ion Ratio Lower Upper
252 100
253 22.1 18.0 27.0
125 9.8 8.0 12.0

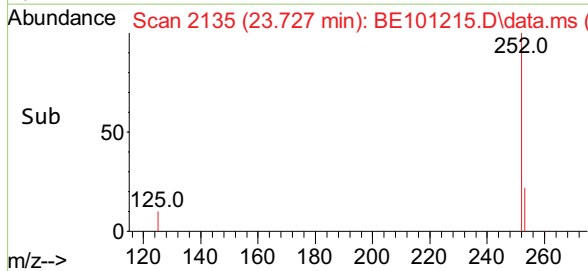
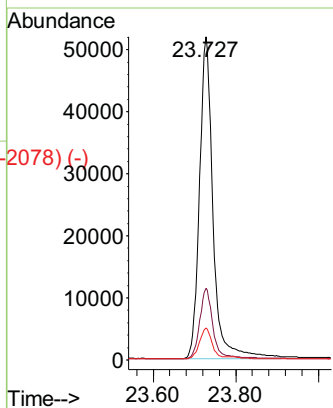
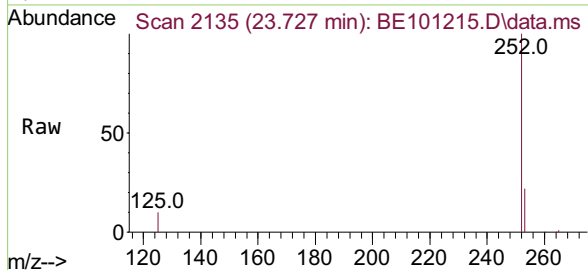


Abundance Scan 2900 (26.473 min): BE101213.D\data.ms (-2#90) (-)




Dibenzo(a,h)anthracene
Concen: 1.91 ng
RT: 26.477 min Scan# 2902
Delta R.T. 0.004 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Tgt Ion:278 Resp: 124347
Ion Ratio Lower Upper
278 100
139 14.7 12.2 18.2
279 23.8 19.3 28.9

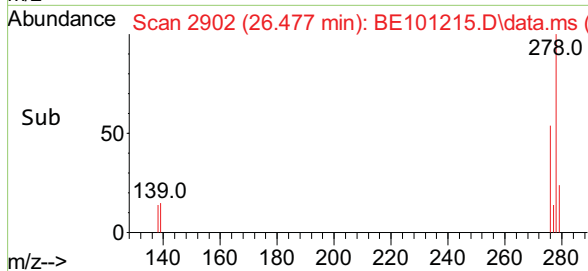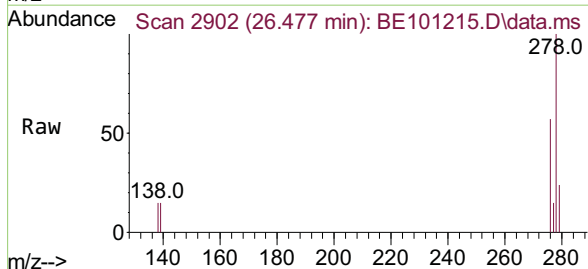


Abundance Scan 3117 (27.247 min): BE101213.D\data.ms (-3062) (-)

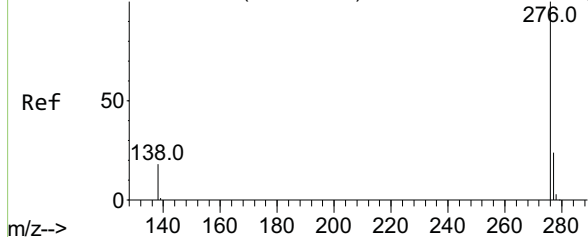


Benzo(g,h,i)perylene
Concen: 1.84 ng
RT: 27.251 min Scan# 3119
Delta R.T. 0.004 min
Lab File: BE101215.D
Acq: 6 Apr 2021 14:15

Instrument :
BNA_E
ClientSampleId :
SSTDICC1.6

Abundance Scan 3119 (27.251 min): BE101215.D\data.ms

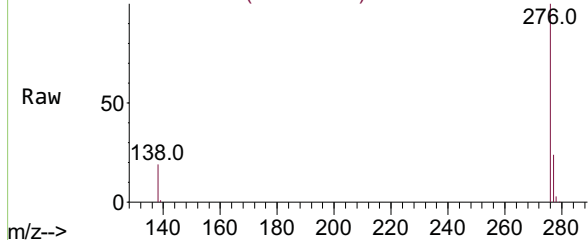

Tgt Ion:	276	Resp:	129757
Ion	Ratio	Lower	Upper
276	100		
277	23.9	19.4	29.0
138	18.7	15.2	22.8

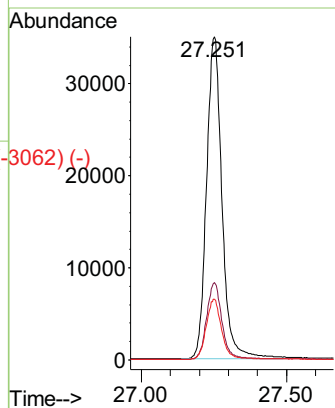

Abundance Scan 3119 (27.251 min): BE101215.D\data.ms (-3062) (-)

