
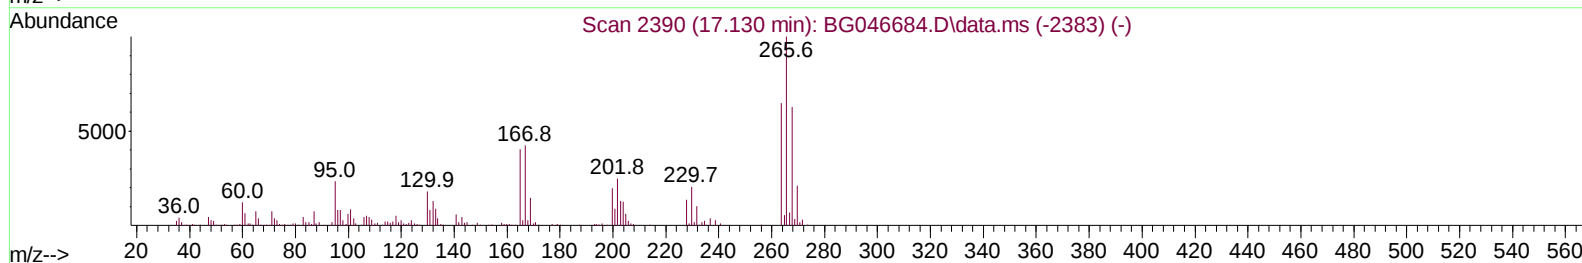
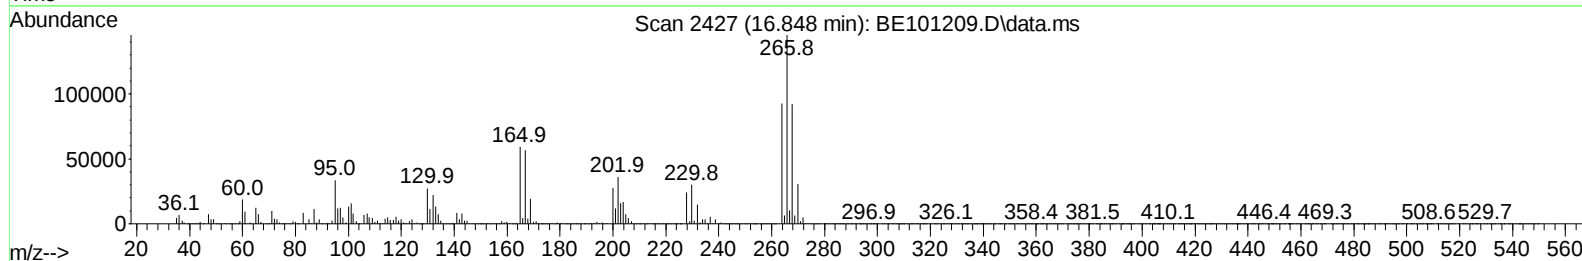


Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE040621\  
Data File : BE101209.D  
Acq On : 6 Apr 2021 9:28  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 11:20:59 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 31 10:54:22 2021  
Response via : Initial Calibration

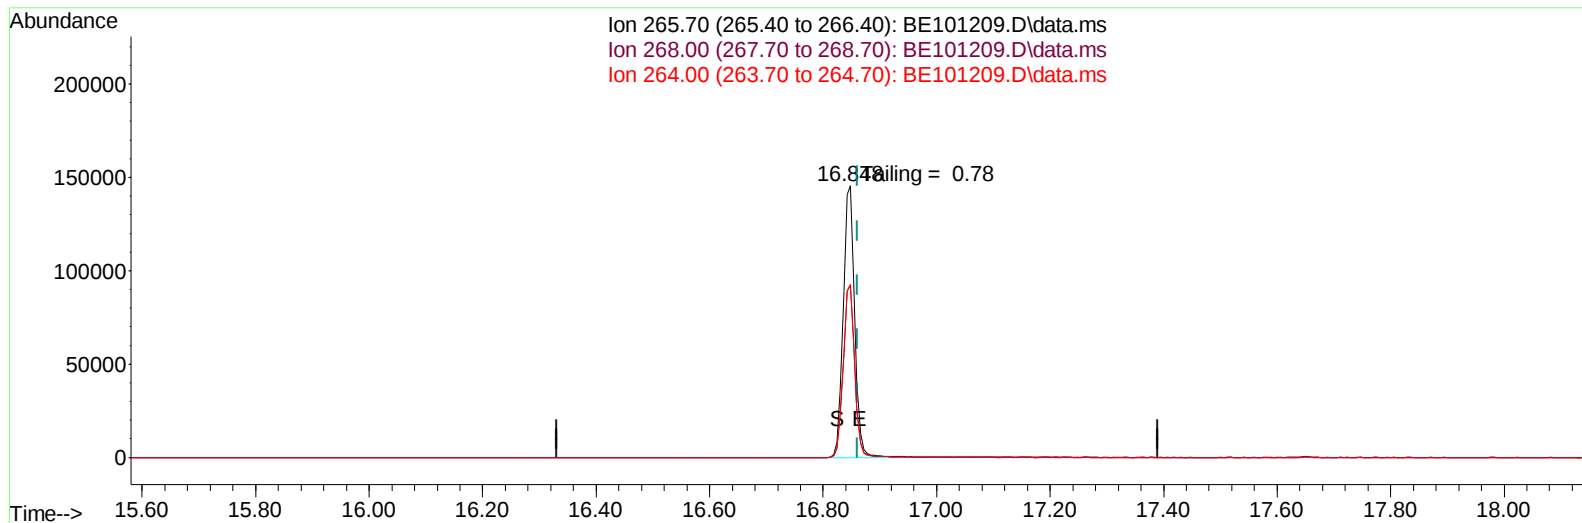




TIC: BE101209.D\data.ms

**(70) Pentachlorophenol (C)****16.848min (-0.012) 1461502.03 ng****response 206451**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.26  |
| 264.00 | 61.60  | 63.88  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE040621\  
Data File : BE101209.D  
Acq On : 6 Apr 2021 9:28  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 11:20:59 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 31 10:54:22 2021  
Response via : Initial Calibration

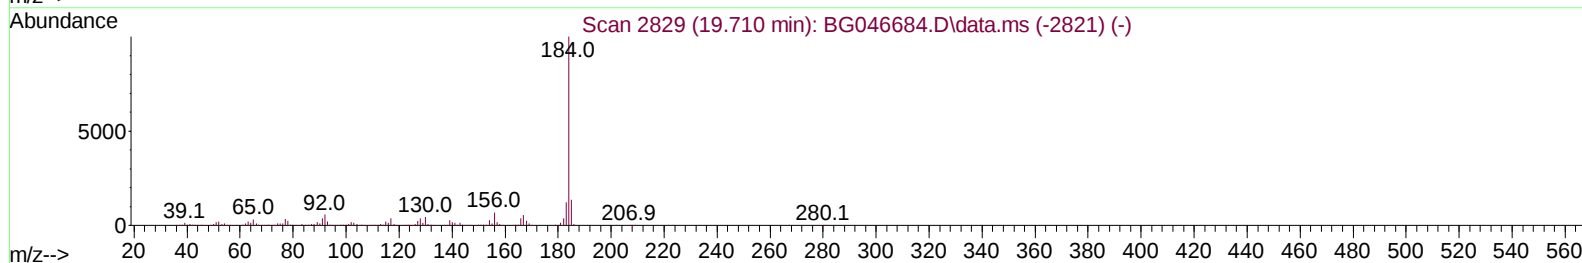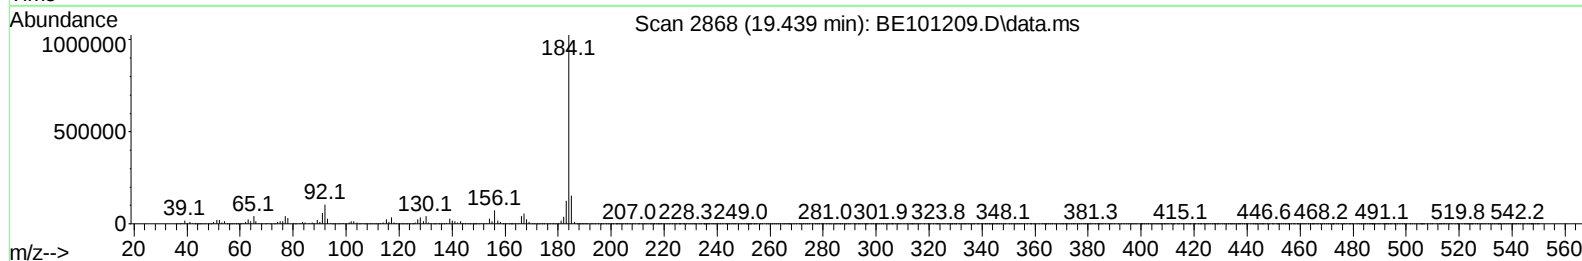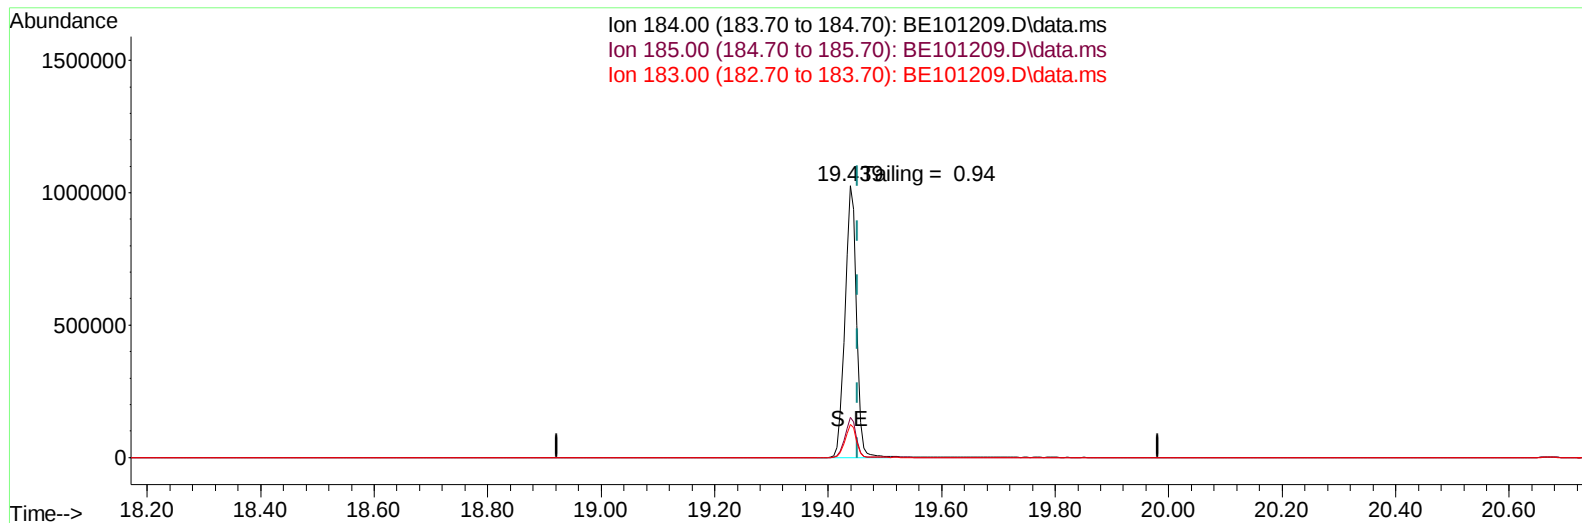

TIC: BE101209.D\data.ms

**(77) Benzidine****19.439min (-0.012) 4345.06 ng****response 1457513**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.80  |
| 183.00 | 13.20  | 12.20  |
| 0.00   | 0.00   | 0.00   |