

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040621\
 Data File : BE101217.D
 Acq On : 6 Apr 2021 15:30
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC5.0

Quant Time: Apr 06 16:13:02 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE040621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 06 13:45:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.839	152	3952	0.40	ng	0.00
7) Naphthalene-d8	10.614	136	17139	0.40	ng	0.00
13) Acenaphthene-d10	14.442	164	13505	0.40	ng	0.00
19) Phenanthrene-d10	17.196	188	34327	0.40	ng	#-0.01
29) Chrysene-d12	21.355	240	49259	0.40	ng	0.00
36) Perylene-d12	23.837	264	28712	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.421	112	41923	3.90	ng	0.00
5) Phenol-d6	6.987	99	72869	4.59	ng	0.00
8) Nitrobenzene-d5	8.977	82	71476	5.29	ng	0.00
11) 2-Methylnaphthalene-d10	12.194	152	200437	5.23	ng	0.00
14) 2,4,6-Tribromophenol	0.000	330	0d	0.00	ng	
15) 2-Fluorobiphenyl	13.073	172	214639	4.37	ng	0.00
27) Fluoranthene-d10	19.220	212	3177773	5.38	ng	0.00
31) Terphenyl-d14	19.818	244	557776	5.02	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.370	88	24103	3.44	ng	98
3) n-Nitrosodimethylamine	3.670	42	30769	4.31	ng	# 98
6) bis(2-Chloroethyl)ether	7.252	93	61341	4.73	ng	100
9) Naphthalene	10.666	128	886218	4.77	ng	100
10) Hexachlorobutadiene	10.965	225	38163	4.64	ng	99
12) 2-Methylnaphthalene	12.266	142	170915	5.32	ng	97
16) Acenaphthylene	14.168	152	284079	5.29	ng	99
17) Acenaphthene	14.514	154	197092	5.02	ng	96
18) Fluorene	15.503	166	262261	5.18	ng	99
21) 4-Bromophenyl-phenylether	16.410	248	86240	4.82	ng	98
22) Hexachlorobenzene	16.516	284	83692	4.63	ng	99
24) Pentachlorophenol	16.848	266	45452	6.39	ng	98
25) Phenanthrene	17.242	178	489376	4.82	ng	99
26) Anthracene	17.332	178	472209	5.39	ng	98
28) Fluoranthene	19.249	202	705307	5.46	ng	98
30) Pyrene	19.605	202	715063	4.99	ng	98
32) Benzo(a)anthracene	21.343	228	707408	4.76	ng	98
33) Chrysene	21.392	228	746099	4.55	ng	99
35) Indeno(1,2,3-cd)pyrene	26.449	276	462964	3.21	ng	99
37) Benzo(b)fluoranthene	23.078	252	506481	5.75	ng	99
38) Benzo(k)fluoranthene	23.128	252	563906	5.68	ng	99
39) Benzo(a)pyrene	23.726	252	439507	5.64	ng	100
40) Dibenzo(a,h)anthracene	26.477	278	410032	5.38	ng	99
41) Benzo(g,h,i)perylene	27.251	276	410189	4.97	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040621\
Data File : BE101217.D
Acq On : 6 Apr 2021 15:30
Operator : CG/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0

Quant Time: Apr 06 16:13:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE040621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 06 13:45:08 2021
Response via : Initial Calibration




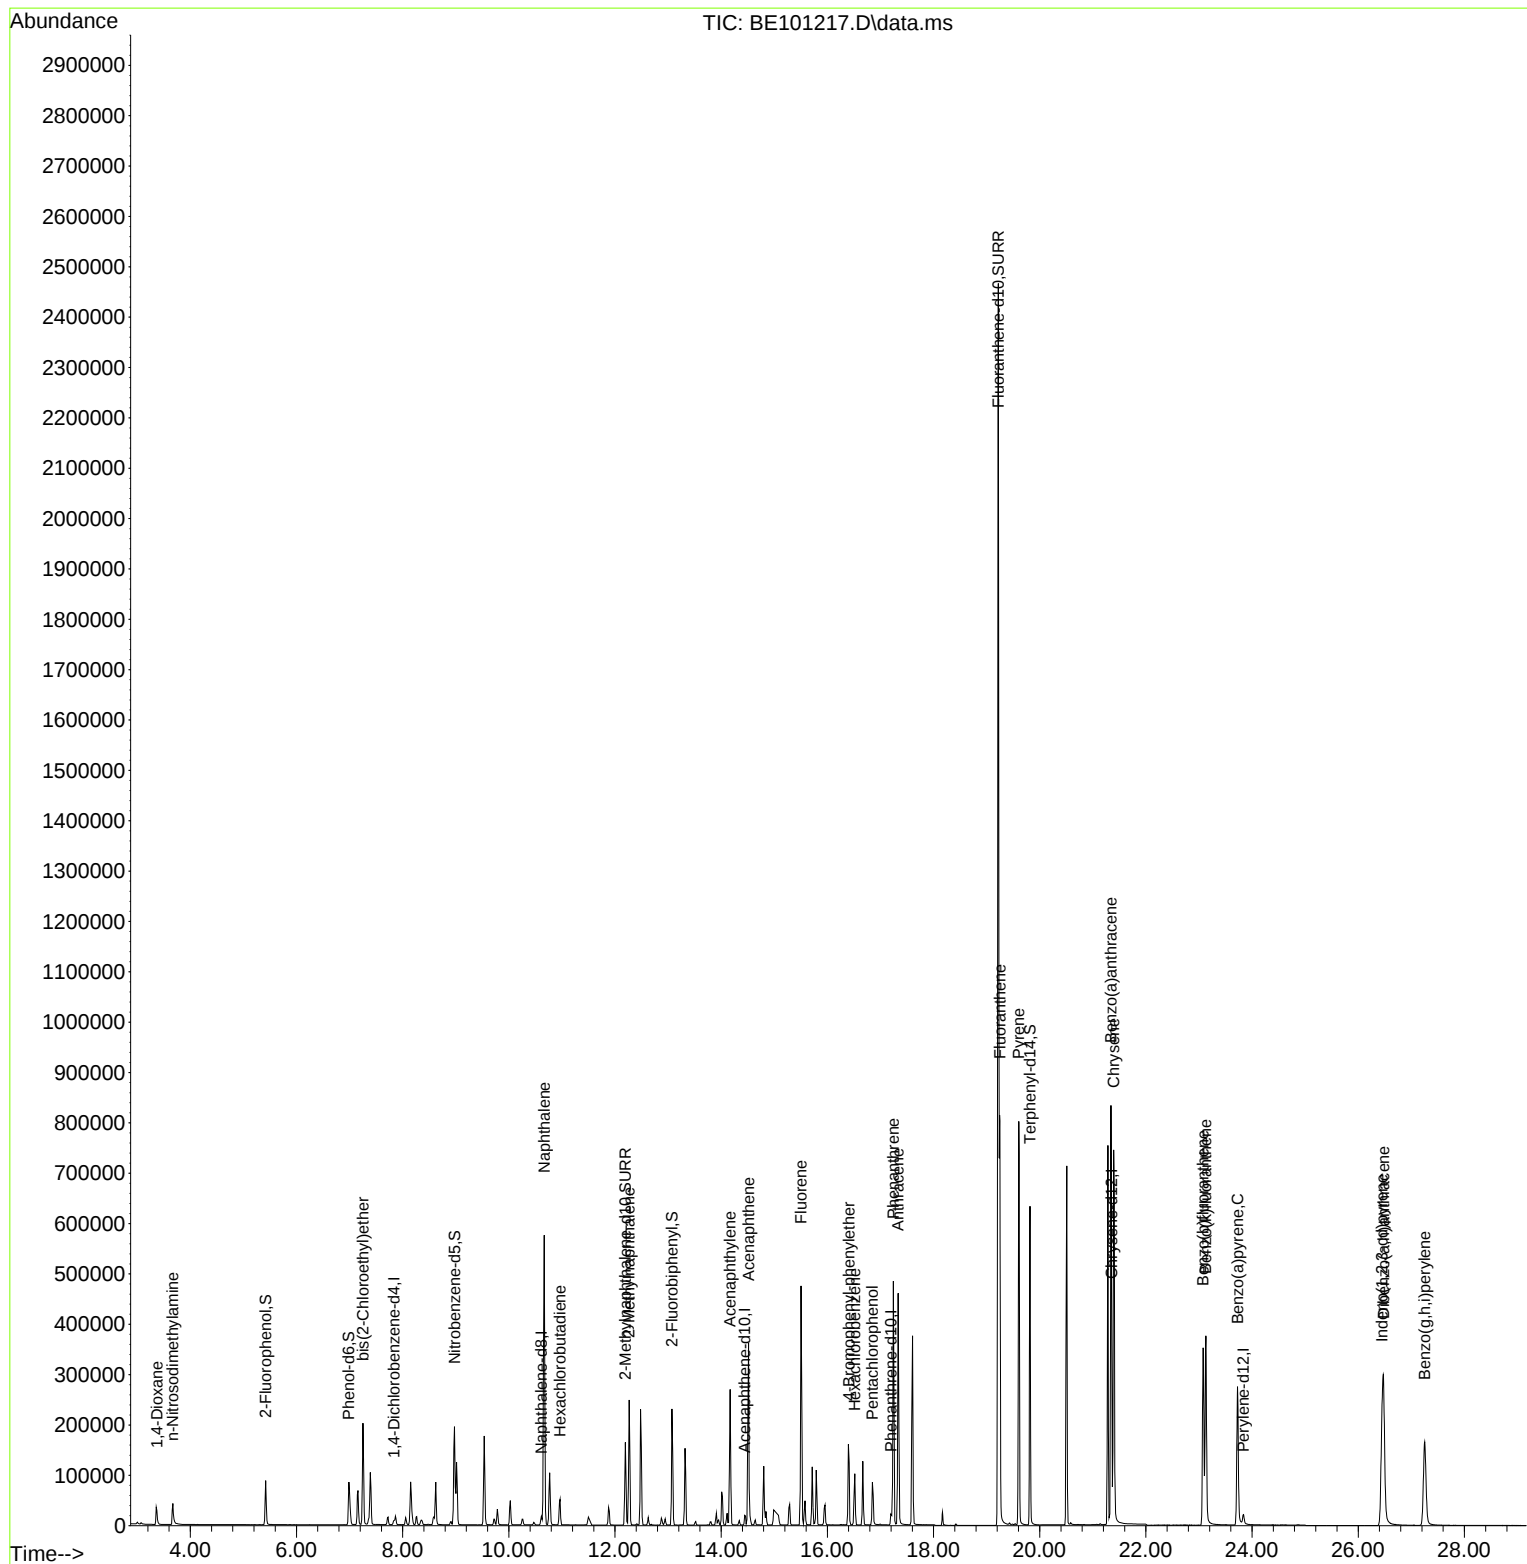




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.839 min Scan# 432
 Delta R.T. 0.001 min
 Lab File: BE101217.D
 Acq: 6 Apr 2021 15:30




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:152 Resp: 3952
 Ion Ratio Lower Upper
 152 100
 150 151.8 116.9 175.3
 115 57.0 44.5 66.7

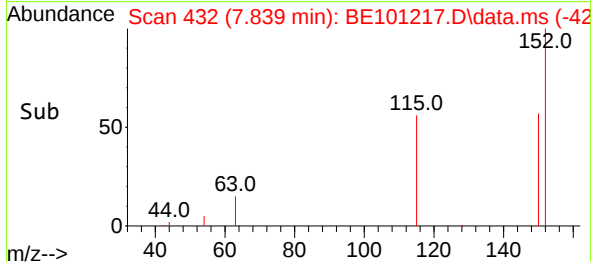

#2
 1,4-Dioxane
 Concen: 3.44 ng
 RT: 3.370 min Scan# 44
 Delta R.T. 0.001 min
 Lab File: BE101217.D
 Acq: 6 Apr 2021 15:30

Tgt Ion: 88 Resp: 24103
 Ion Ratio Lower Upper
 88 100
 58 89.4 73.6 110.4
 43 33.7 27.6 41.4


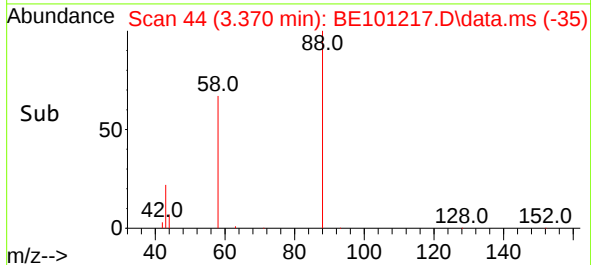




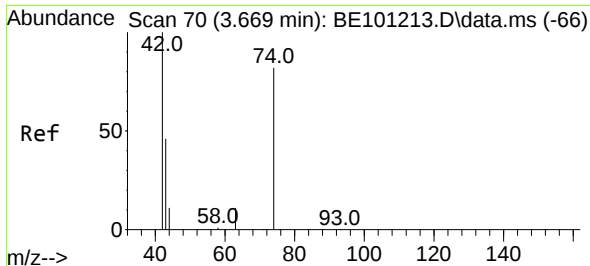

#3
n-Nitrosodimethylamine
Concen: 4.31 ng
RT: 3.670 min Scan# 70
Delta R.T. 0.001 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion: 42 Resp: 30769
Ion Ratio Lower Upper
42 100
74 115.1 92.7 139.1
44 7.5 10.7 16.1#

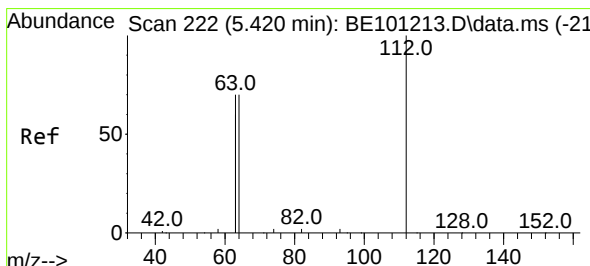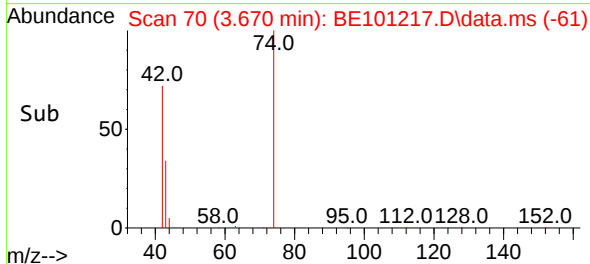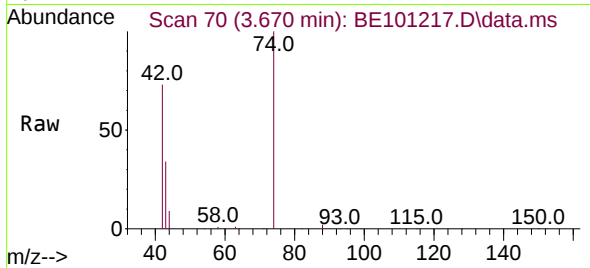

#4
2-Fluorophenol
Concen: 3.90 ng
RT: 5.421 min Scan# 222
Delta R.T. 0.001 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30

Tgt Ion: 112 Resp: 41923
Ion Ratio Lower Upper
112 100
64 76.9 62.3 93.5
63 149.2 117.3 175.9


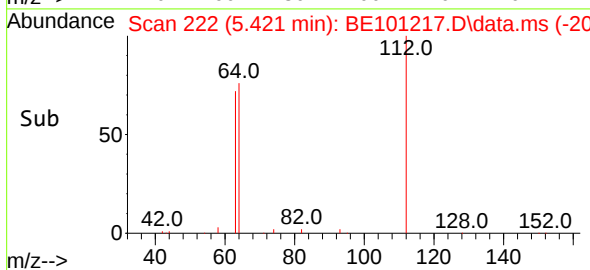

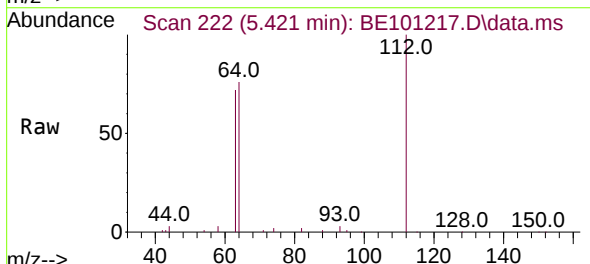




#5
Phenol-d6
Concen: 4.59 ng
RT: 6.987 min Scan# 358
Delta R.T. 0.001 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 72869
Ion Ratio Lower Upper
99 100
42 23.1 18.5 27.7
71 33.7 26.5 39.7

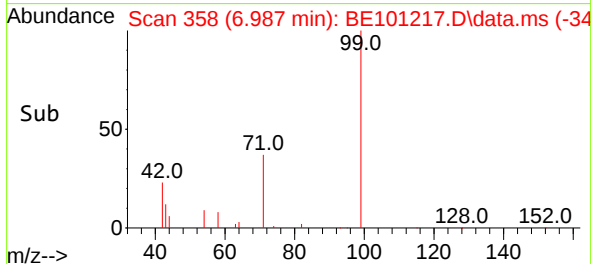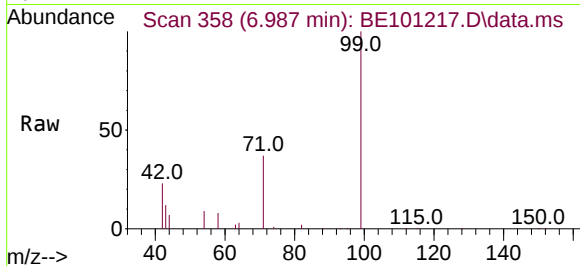

#6
bis(2-Chloroethyl)ether
Concen: 4.73 ng
RT: 7.252 min Scan# 381
Delta R.T. 0.001 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30

Tgt Ion: 93 Resp: 61341
Ion Ratio Lower Upper
93 100
63 365.6 292.5 438.7
95 32.6 25.7 38.5


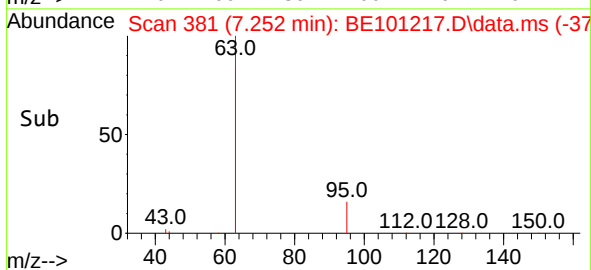

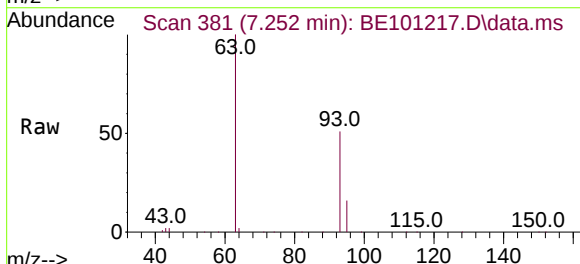




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.614 min Scan# 650
Delta R.T. -0.001 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	17139
Ion Ratio	Lower	Upper	
136	100		
137	11.1	8.6	13.0
54	45.3	34.7	52.1
68	9.5	7.0	10.4

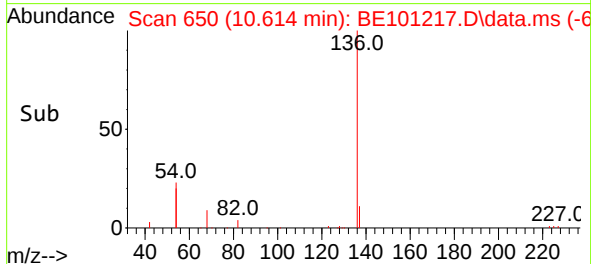

#8
Nitrobenzene-d5
Concen: 5.29 ng
RT: 8.977 min Scan# 524
Delta R.T. -0.001 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30

Tgt Ion:	82	Resp:	71476
Ion Ratio	Lower	Upper	
82	100		
128	147.7	118.7	178.1
54	200.3	164.4	246.6


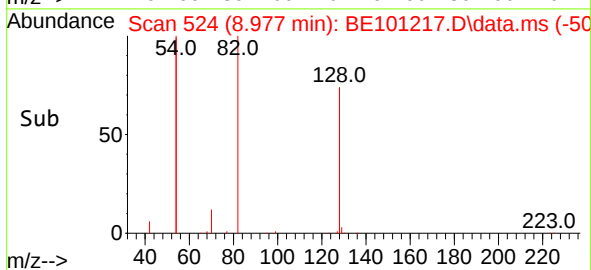

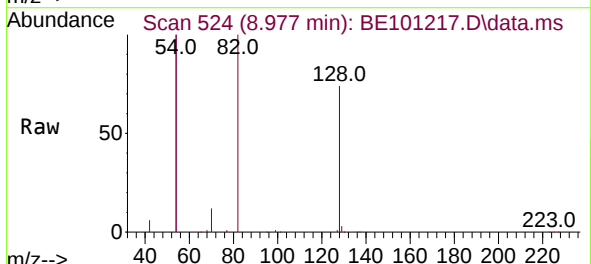




#9
Naphthalene
Concen: 4.77 ng
RT: 10.666 min Scan# 654
Delta R.T. -0.001 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:128 Resp: 886218
Ion Ratio Lower Upper
128 100
129 2.9 2.2 3.4
127 3.2 2.6 3.8

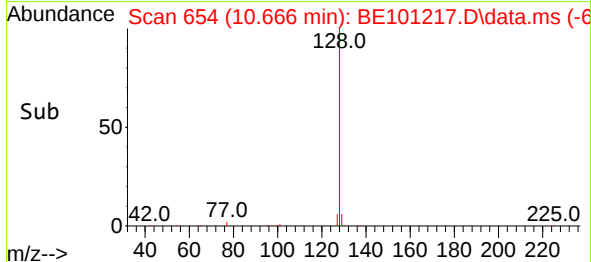

#10
Hexachlorobutadiene
Concen: 4.64 ng
RT: 10.965 min Scan# 677
Delta R.T. -0.001 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30

Tgt Ion:225 Resp: 38163
Ion Ratio Lower Upper
225 100
223 62.8 50.4 75.6
227 64.4 50.1 75.1




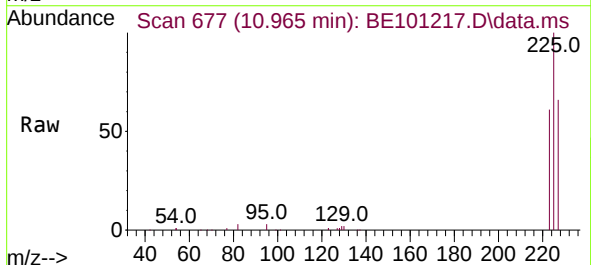




#11
2-Methylnaphthalene-d10
Concen: 5.23 ng
RT: 12.194 min Scan# 763
Delta R.T. -0.002 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 200437
Ion Ratio Lower Upper
152 100
151 20.5 16.5 24.7

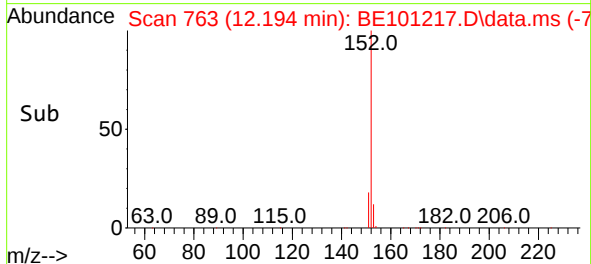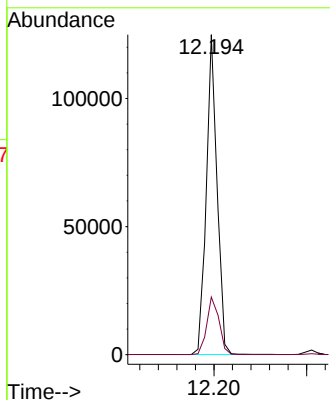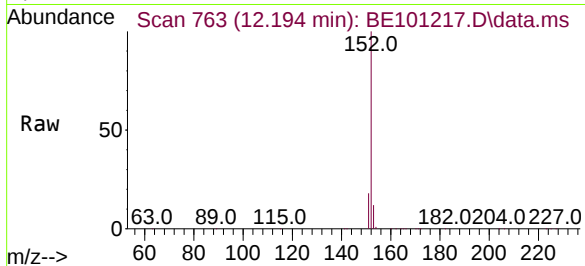

#12
2-Methylnaphthalene
Concen: 5.32 ng
RT: 12.266 min Scan# 768
Delta R.T. -0.002 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30

Tgt Ion:142 Resp: 170915
Ion Ratio Lower Upper
142 100
141 88.2 73.0 109.6
115 33.7 27.8 41.8



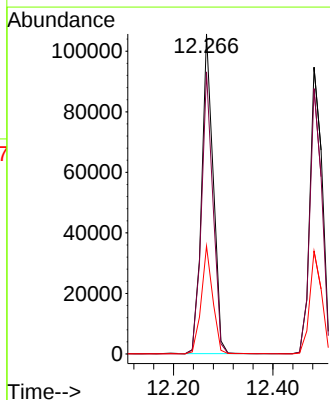
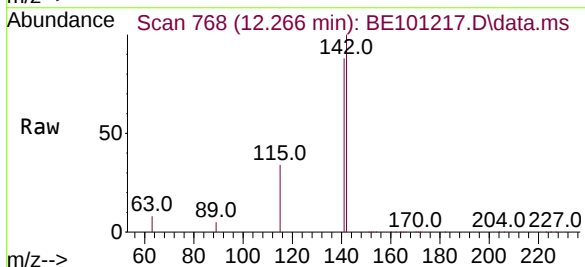


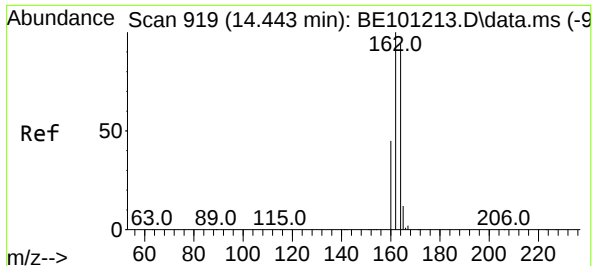

#13
 Acenaphthene-d10
 Concen: 0.40 ng
 RT: 14.442 min Scan# 919
 Delta R.T. -0.002 min
 Lab File: BE101217.D
 Acq: 6 Apr 2021 15:30

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:164	Resp:	13505
Ion	Ratio	Lower Upper
164	100	
162	107.4	85.3 127.9
160	48.6	39.1 58.7

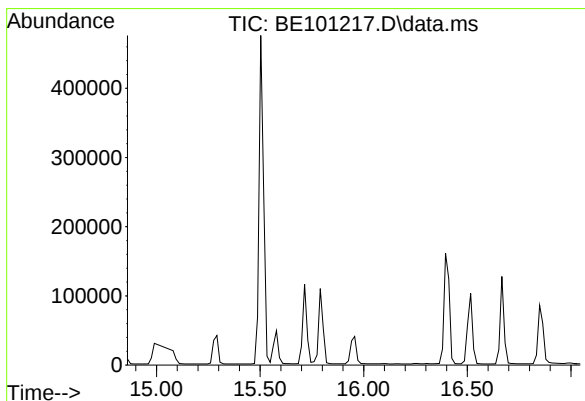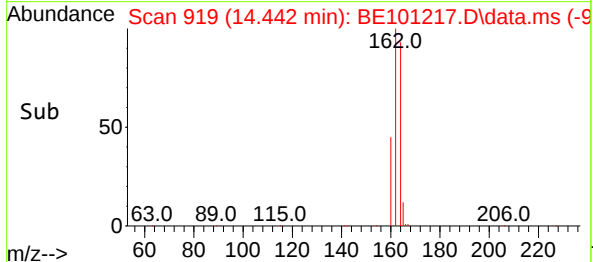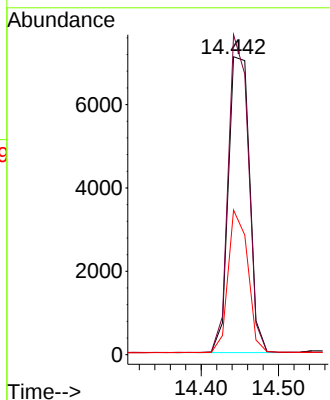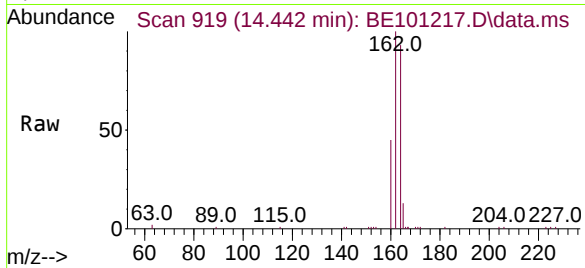


#14
 2,4,6-Tribromophenol
 Concen: 0.00 ng
 Expected RT: 15.96 min

Lab File: BE101217.D
 Acq: 6 Apr 2021 15:30

Tgt Ion: 330	
Sig	Exp Ratio
330	100
332	97.2
141	38.0




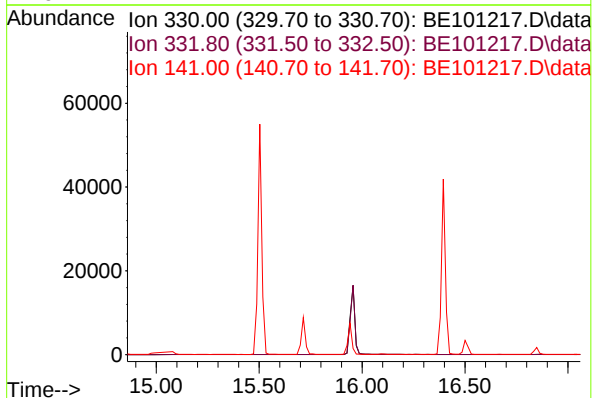


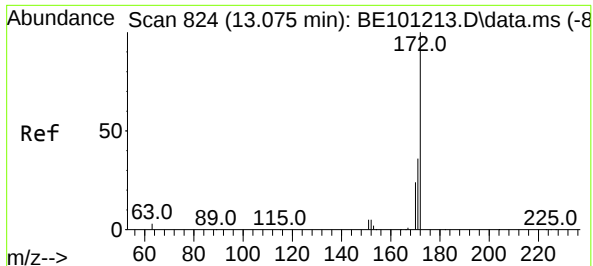

#15
2-Fluorobiphenyl
Concen: 4.37 ng
RT: 13.073 min Scan# 824
Delta R.T. -0.002 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:172 Resp: 214639
Ion Ratio Lower Upper
172 100
171 36.0 28.7 43.1
170 24.7 19.3 28.9

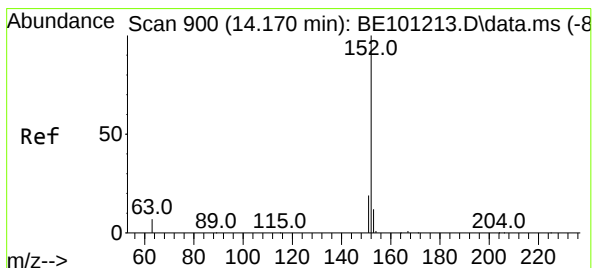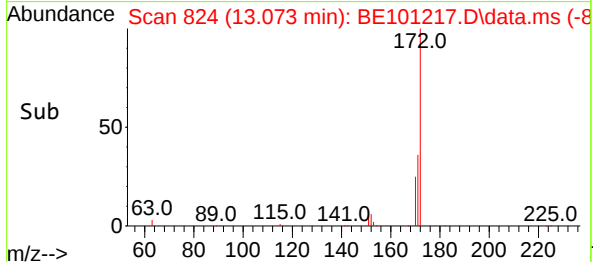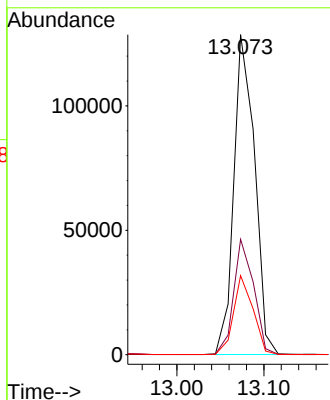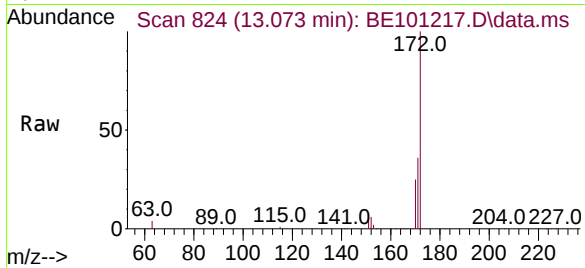

#16
Acenaphthylene
Concen: 5.29 ng
RT: 14.168 min Scan# 900
Delta R.T. -0.002 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30

Tgt Ion:152 Resp: 284079
Ion Ratio Lower Upper
152 100
151 19.5 15.4 23.2
153 13.2 10.0 15.0


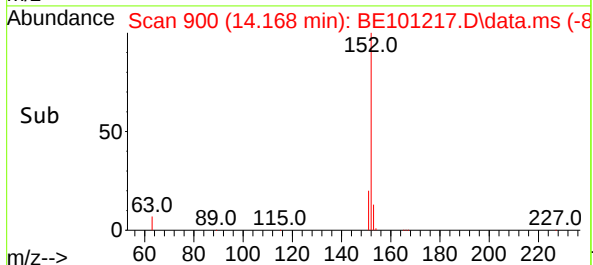
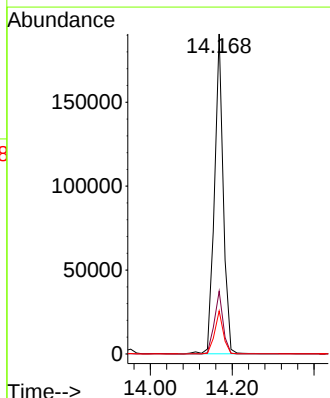
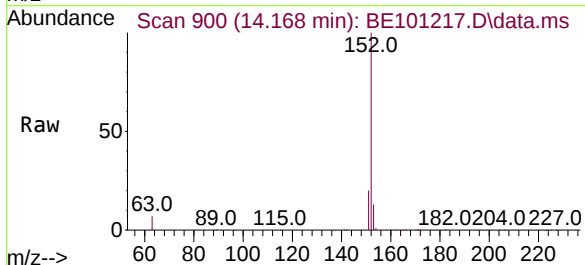


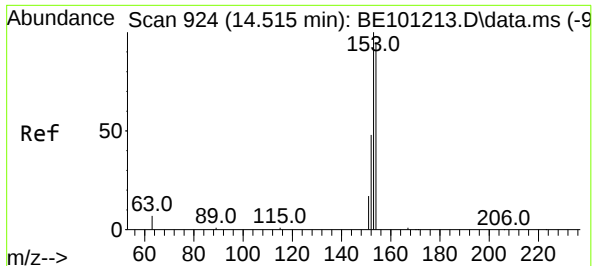

#17
Acenaphthene
Concen: 5.02 ng
RT: 14.514 min Scan# 924
Delta R.T. -0.002 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 197092
Ion Ratio Lower Upper
154 100
153 102.5 84.9 127.3
152 50.2 42.7 64.1

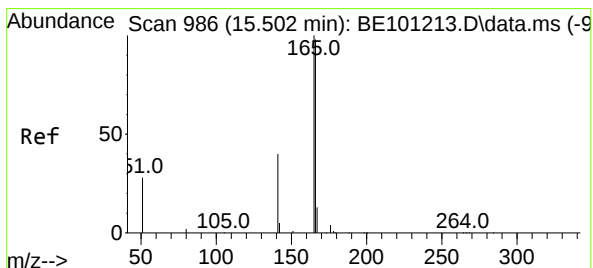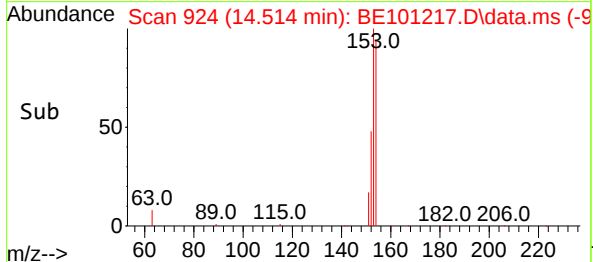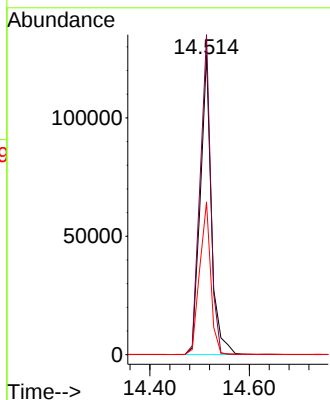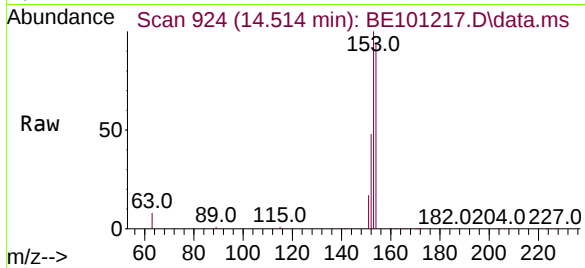

#18
Fluorene
Concen: 5.18 ng
RT: 15.503 min Scan# 986
Delta R.T. 0.001 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30

Tgt Ion:166 Resp: 262261
Ion Ratio Lower Upper
166 100
165 97.9 79.0 118.4
167 13.6 11.0 16.4


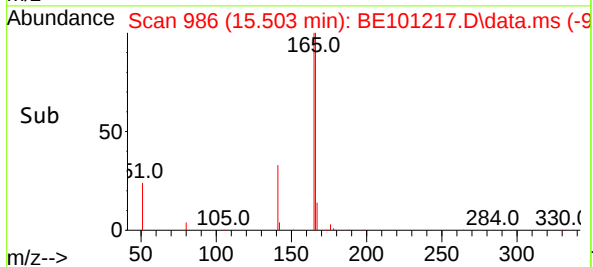
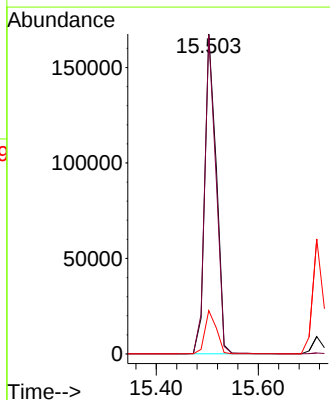
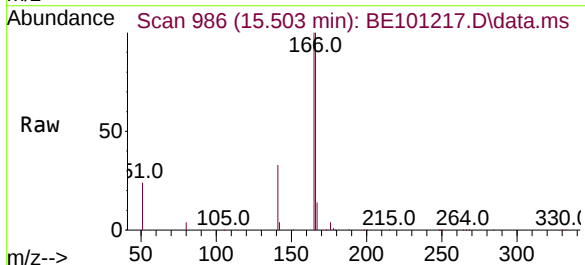




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.196 min Scan# 1098
Delta R.T. -0.014 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:188 Resp: 34327
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 17.7 4.6 6.8#

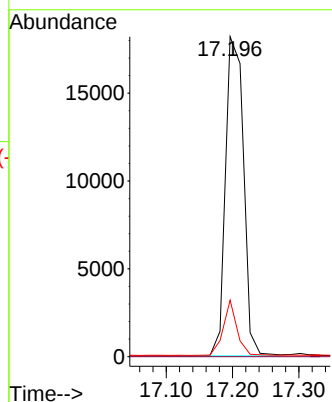

#21
4-Bromophenyl-phenylether
Concen: 4.82 ng
RT: 16.410 min Scan# 1046
Delta R.T. 0.001 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30

Tgt Ion:248 Resp: 86240
Ion Ratio Lower Upper
248 100
250 106.5 84.5 126.7
141 21.1 19.8 29.8









#22
Hexachlorobenzene
Concen: 4.63 ng
RT: 16.516 min Scan# 1053
Delta R.T. 0.001 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:284 Resp: 83692
Ion Ratio Lower Upper
284 100
142 34.4 27.4 41.0
249 34.3 26.5 39.7

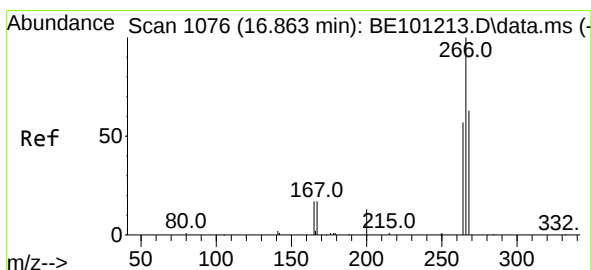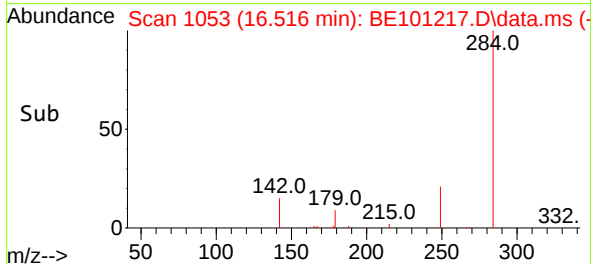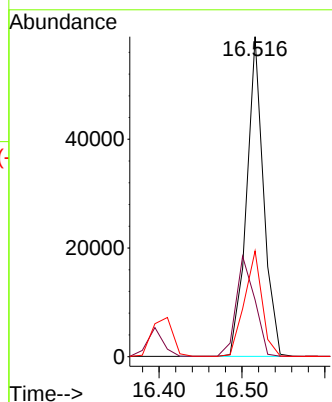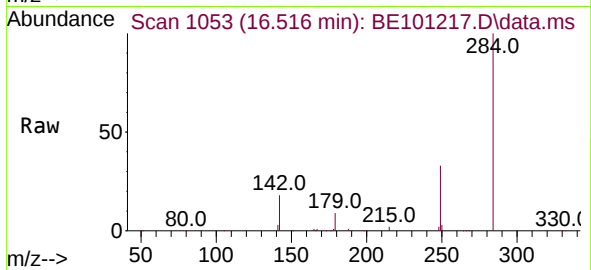

#24
Pentachlorophenol
Concen: 6.39 ng
RT: 16.848 min Scan# 1075
Delta R.T. -0.014 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30

Tgt Ion:266 Resp: 45452
Ion Ratio Lower Upper
266 100
264 63.0 49.1 73.7
268 64.2 50.6 76.0


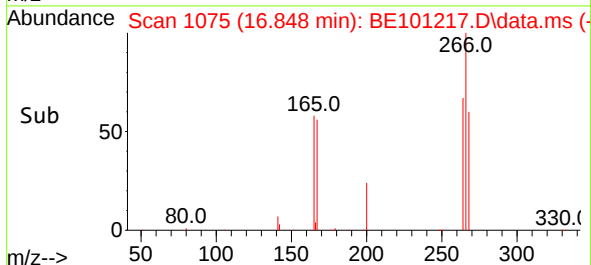




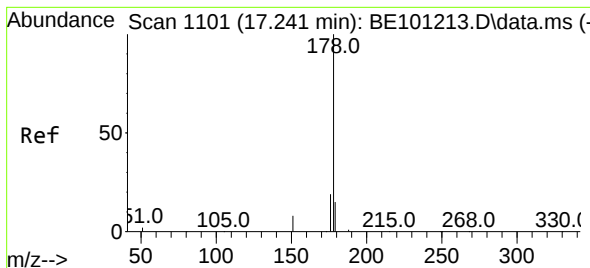

#25
Phenanthrene
Concen: 4.82 ng
RT: 17.242 min Scan# 1101
Delta R.T. 0.001 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 489376
Ion Ratio Lower Upper
178 100
176 19.3 15.0 22.6
179 15.8 12.2 18.4

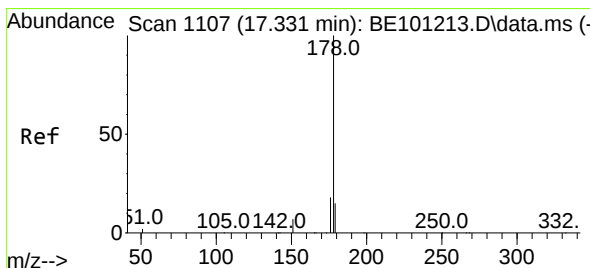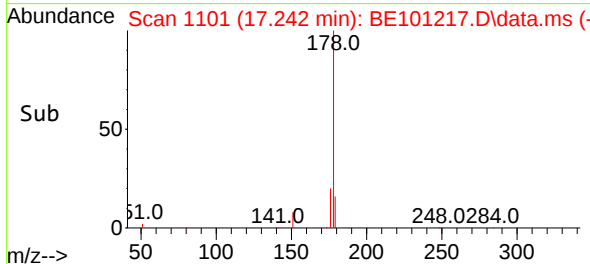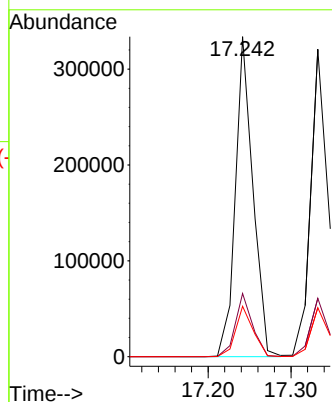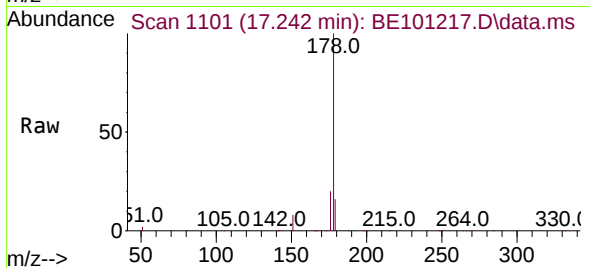

#26
Anthracene
Concen: 5.39 ng
RT: 17.332 min Scan# 1107
Delta R.T. 0.001 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30

Tgt Ion:178 Resp: 472209
Ion Ratio Lower Upper
178 100
176 18.6 14.4 21.6
179 15.9 11.8 17.8


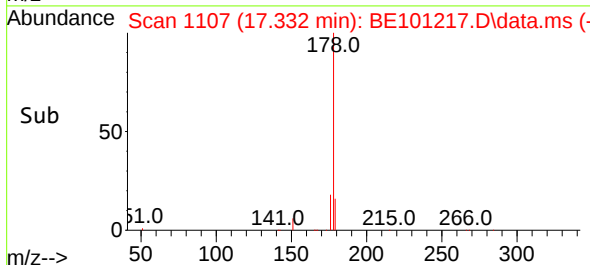

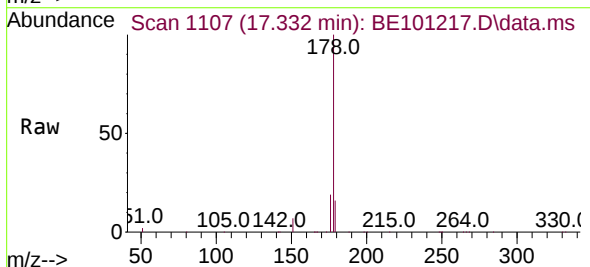




#27
Fluoranthene-d10
Concen: 5.38 ng
RT: 19.220 min Scan# 1359
Delta R.T. 0.000 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 3177773
Ion Ratio Lower Upper
212 100
106 3.5 2.6 4.0
104 1.9 1.4 2.2

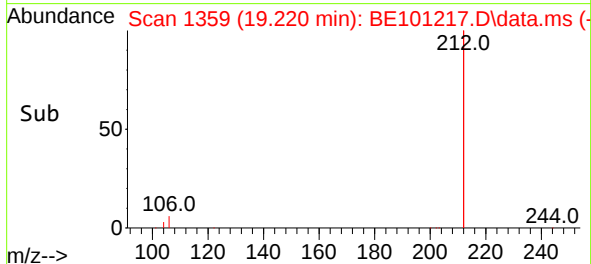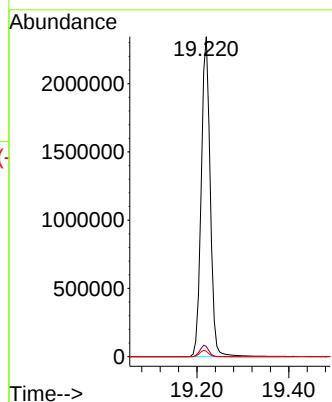

#28
Fluoranthene
Concen: 5.46 ng
RT: 19.249 min Scan# 1364
Delta R.T. 0.000 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30

Tgt Ion:202 Resp: 705307
Ion Ratio Lower Upper
202 100
101 12.1 9.1 13.7
203 18.2 13.6 20.4



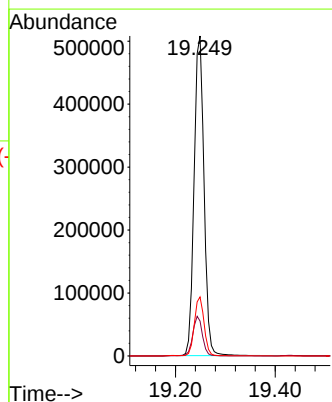



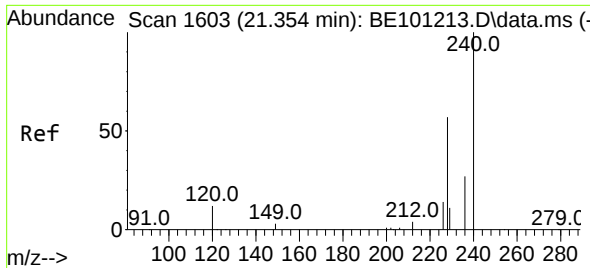

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.355 min Scan# 1604
Delta R.T. 0.002 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:240 Resp: 49259
Ion Ratio Lower Upper
240 100
120 11.9 10.2 15.4
236 27.2 21.7 32.5

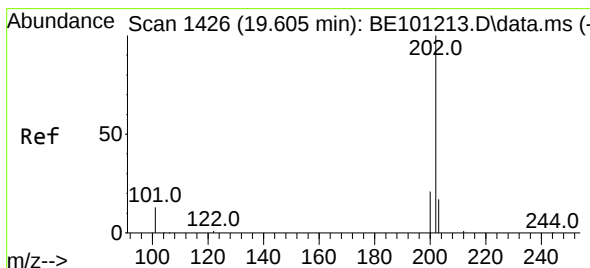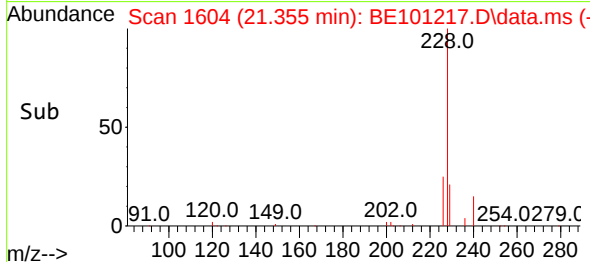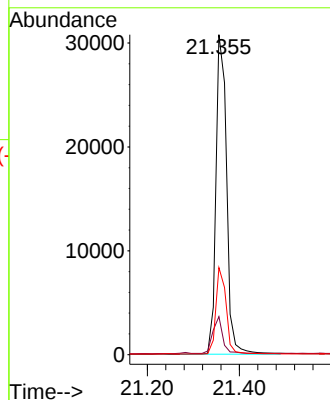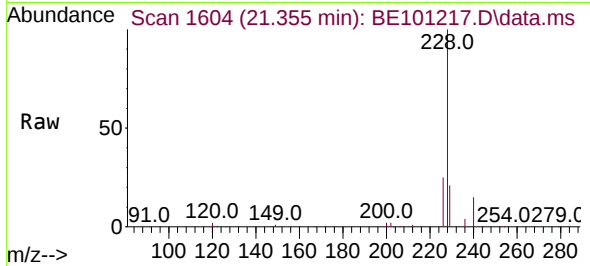

#30
Pyrene
Concen: 4.99 ng
RT: 19.605 min Scan# 1426
Delta R.T. 0.000 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30

Tgt Ion:202 Resp: 715063
Ion Ratio Lower Upper
202 100
200 21.4 16.6 24.8
203 18.3 13.8 20.8


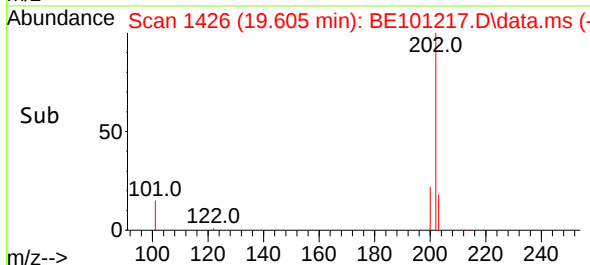
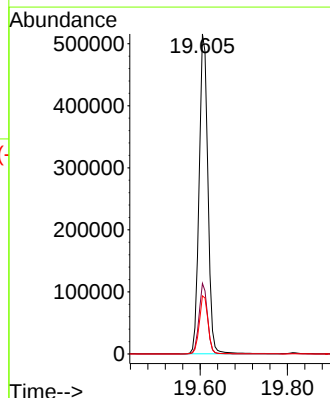
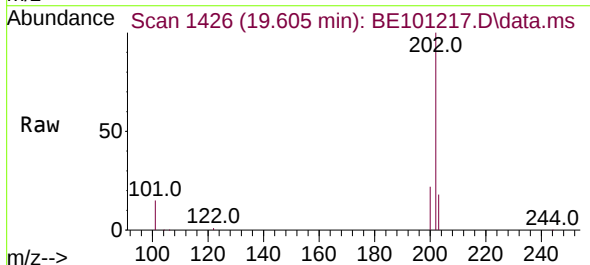




#31
 Terphenyl-d14
 Concen: 5.02 ng
 RT: 19.818 min Scan# 1463
 Delta R.T. 0.000 min
 Lab File: BE101217.D
 Acq: 6 Apr 2021 15:30




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:244 Resp: 557776
 Ion Ratio Lower Upper
 244 100
 212 27.9 21.9 32.9
 122 9.3 7.3 10.9

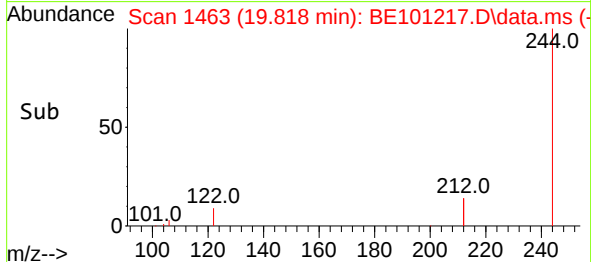

#32
 Benzo(a)anthracene
 Concen: 4.76 ng
 RT: 21.343 min Scan# 1603
 Delta R.T. 0.002 min
 Lab File: BE101217.D
 Acq: 6 Apr 2021 15:30

Tgt Ion:228 Resp: 707408
 Ion Ratio Lower Upper
 228 100
 226 27.7 21.4 32.2
 229 20.6 15.7 23.5





#33

Chrysene

Concen: 4.55 ng

RT: 21.392 min Scan# 1607

Delta R.T. 0.001 min

Lab File: BE101217.D

Acq: 6 Apr 2021 15:30

Instrument :

BNA_E

ClientSampleId :

SSTDICC5.0





Tgt Ion:228 Resp: 746099

Ion Ratio Lower Upper

228 100

226 31.5 24.8 37.2

229 19.9 15.2 22.8

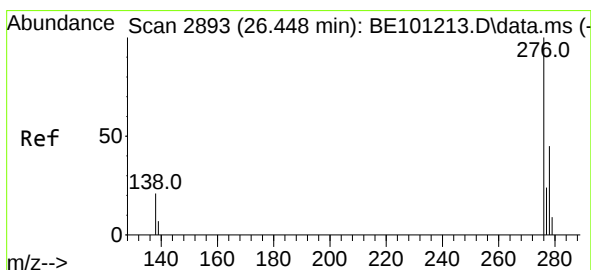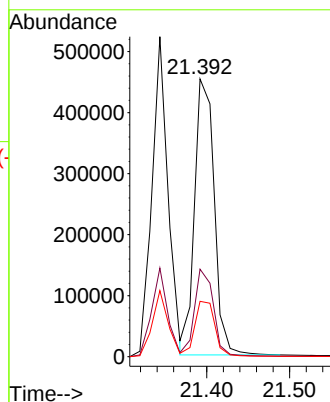

#35

Indeno(1,2,3-cd)pyrene

Concen: 3.21 ng

RT: 26.449 min Scan# 2894

Delta R.T. 0.000 min

Lab File: BE101217.D

Acq: 6 Apr 2021 15:30




Tgt Ion:276 Resp: 462964


Ion Ratio Lower Upper

276 100

138 22.5 17.4 26.0

277 25.3 19.8 29.8


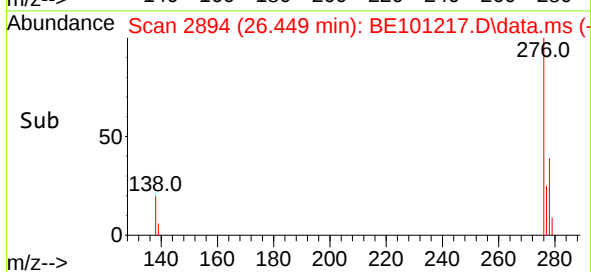
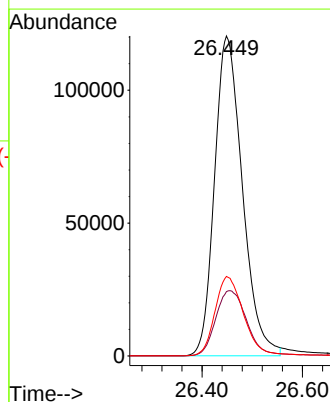
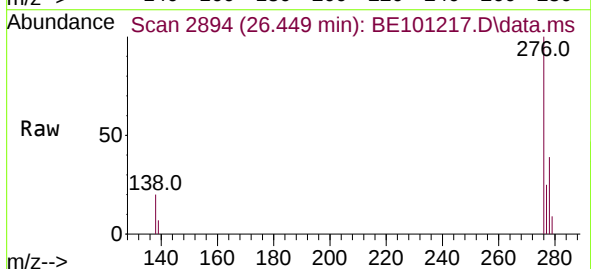




#36
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.837 min Scan# 2166
 Delta R.T. -0.001 min
 Lab File: BE101217.D
 Acq: 6 Apr 2021 15:30




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:264 Resp: 28712
 Ion Ratio Lower Upper
 264 100
 260 24.7 19.3 28.9
 265 26.2 22.4 33.6

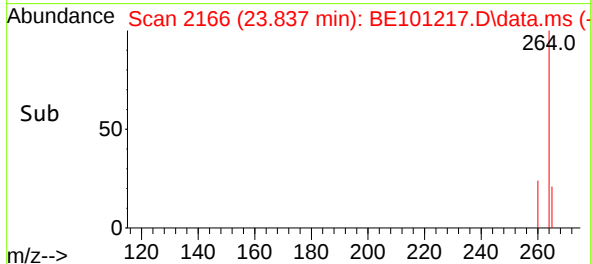

#37
 Benzo(b)fluoranthene
 Concen: 5.75 ng
 RT: 23.078 min Scan# 1953
 Delta R.T. 0.002 min
 Lab File: BE101217.D
 Acq: 6 Apr 2021 15:30

Tgt Ion:252 Resp: 506481
 Ion Ratio Lower Upper
 252 100
 253 22.4 18.1 27.1
 125 9.1 7.6 11.4


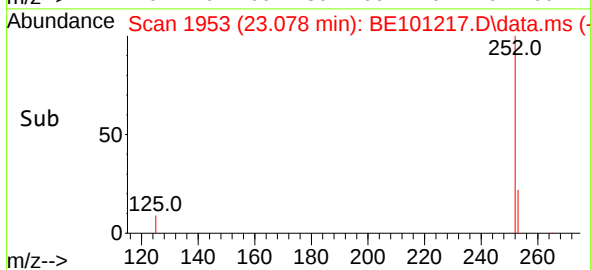

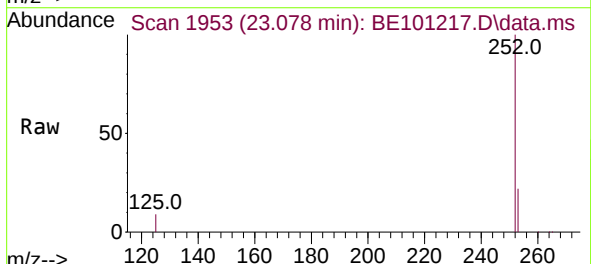




#38
Benzo(k)fluoranthene
Concen: 5.68 ng
RT: 23.128 min Scan# 1967
Delta R.T. 0.002 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 563906
Ion Ratio Lower Upper
252 100
253 22.4 17.8 26.6
125 9.1 7.6 11.4

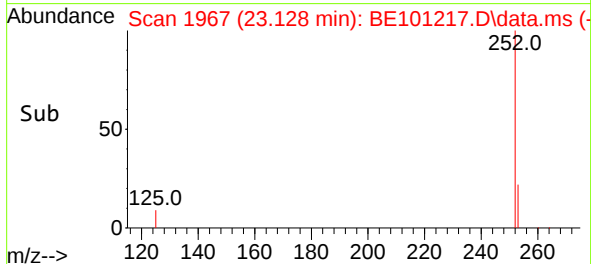

#39
Benzo(a)pyrene
Concen: 5.64 ng
RT: 23.726 min Scan# 2135
Delta R.T. 0.002 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30

Tgt Ion:252 Resp: 439507
Ion Ratio Lower Upper
252 100
253 22.2 18.0 27.0
125 9.9 8.0 12.0


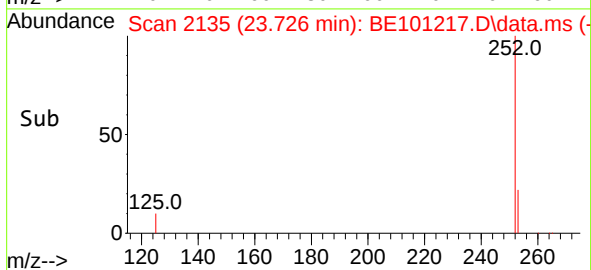






#40
Dibenzo(a,h)anthracene
Concen: 5.38 ng
RT: 26.477 min Scan# 2902
Delta R.T. 0.004 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30

Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0

Tgt Ion:278 Resp: 410032
Ion Ratio Lower Upper
278 100
139 14.6 12.2 18.2
279 24.2 19.3 28.9

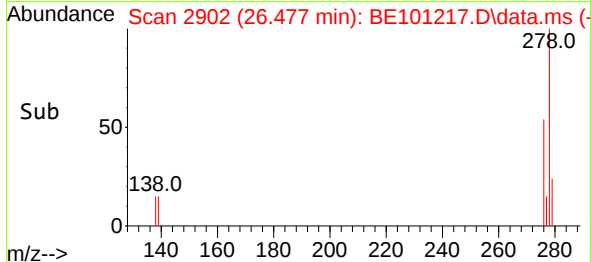

#41
Benzo(g,h,i)perylene
Concen: 4.97 ng
RT: 27.251 min Scan# 3119
Delta R.T. 0.004 min
Lab File: BE101217.D
Acq: 6 Apr 2021 15:30

Tgt Ion:276 Resp: 410189
Ion Ratio Lower Upper
276 100
277 24.2 19.4 29.0
138 19.2 15.2 22.8

