
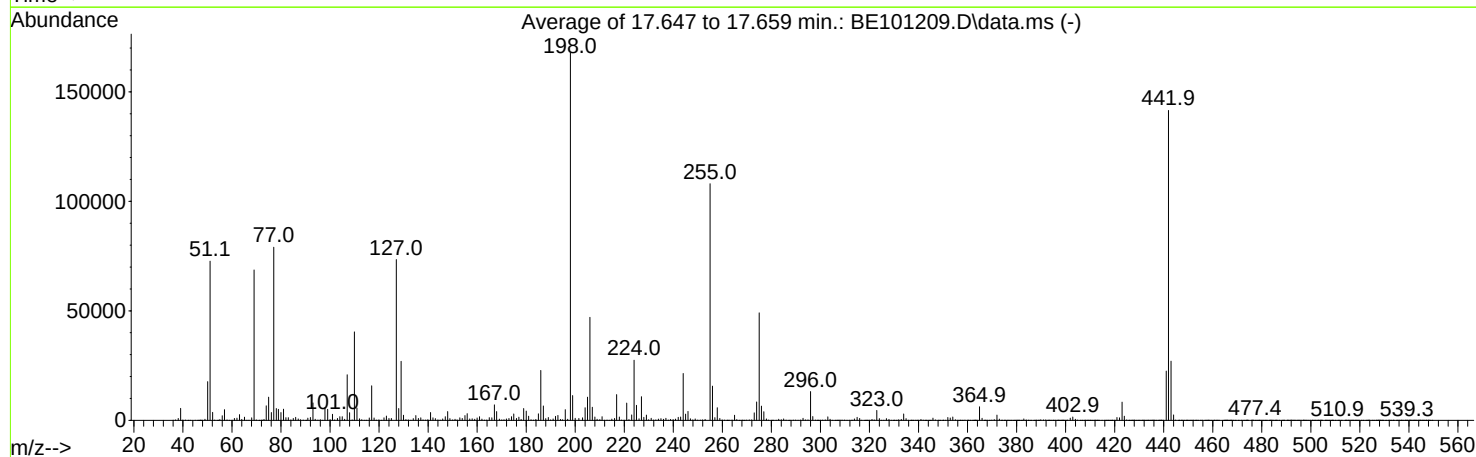


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040621\
 Data File : BE101209.D
 Acq On : 6 Apr 2021 9:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE040621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 06 17:42:42 2021

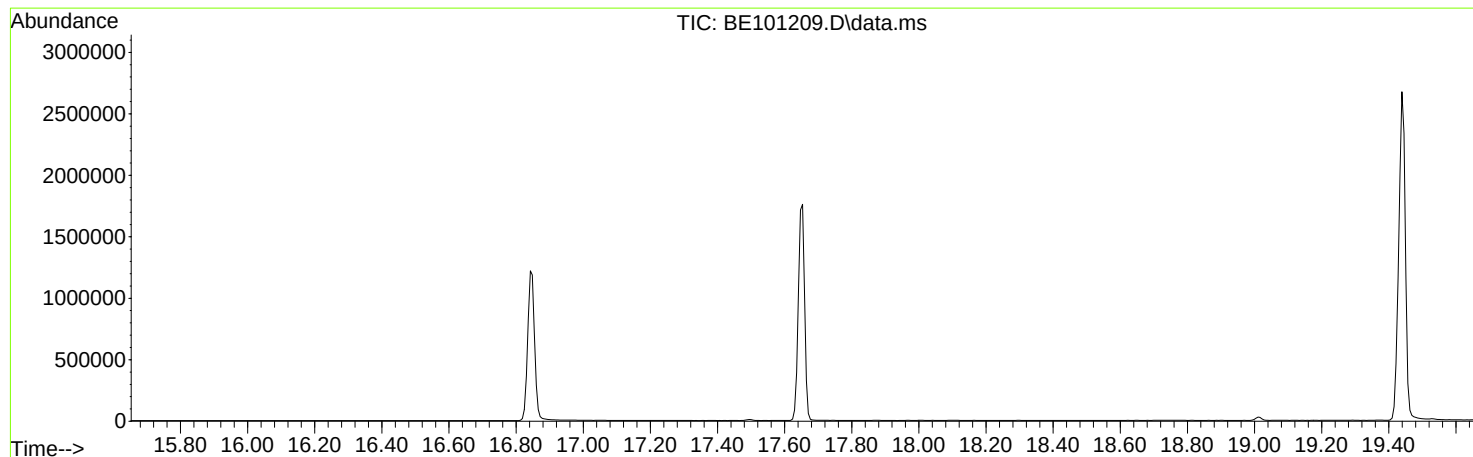

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2554

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	43.3	72693	PASS
68	69	0.00	2	1.7	1169	PASS
69	198	0.00	100	40.9	68666	PASS
70	69	0.00	2	0.4	261	PASS
127	198	10	80	43.7	73421	PASS
197	198	0.00	2	0.3	485	PASS
198	198	100	100	100.0	167961	PASS
199	198	5	9	6.8	11340	PASS
275	198	10	60	29.2	49126	PASS
365	198	1	100	3.7	6253	PASS
441	198	0.01	100	13.4	22504	PASS
442	442	50	100	100.0	141516	PASS
443	442	15	24	19.1	27060	PASS

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/6/2021	BNA_E	<u>BE101209.D</u>
Compound Name	Response	Retention Time
DDT	748463	20.673
DDD	628	20.232
DDE	875	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1503	749966	0.20

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040621\
Data File : BE101209.D
Acq On : 6 Apr 2021 9:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Apr 06 11:20:59 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 10:54:22 2021
Response via : Initial Calibration

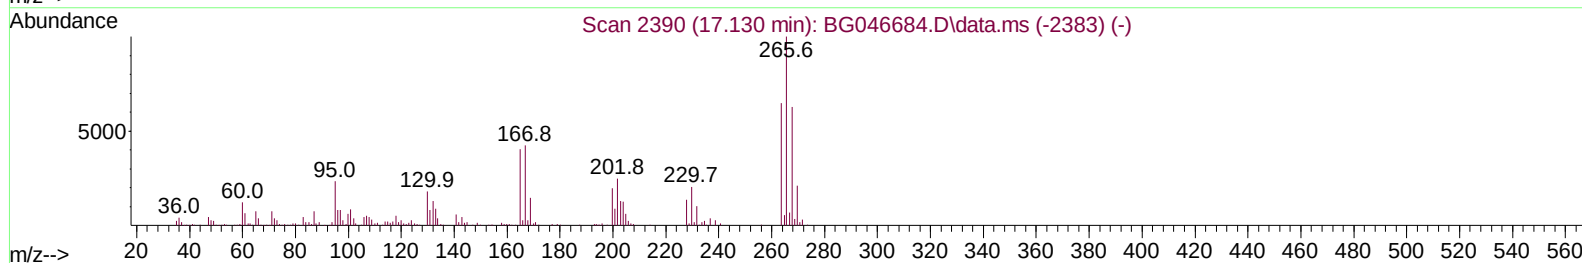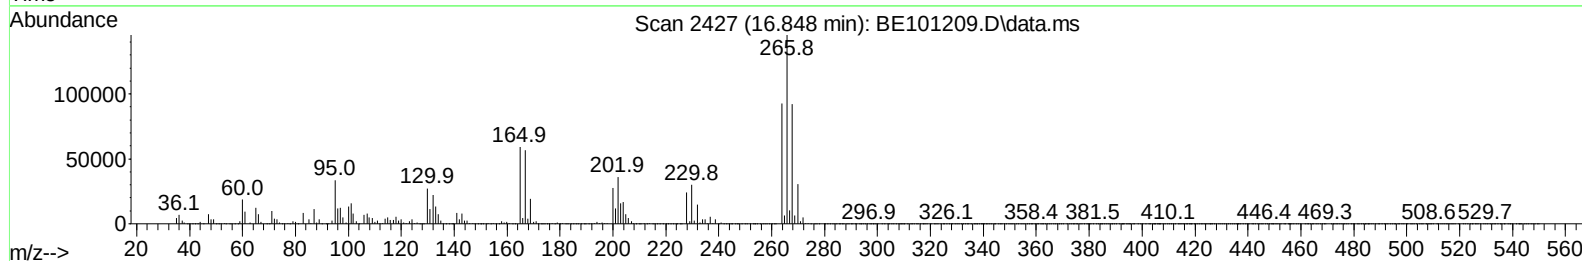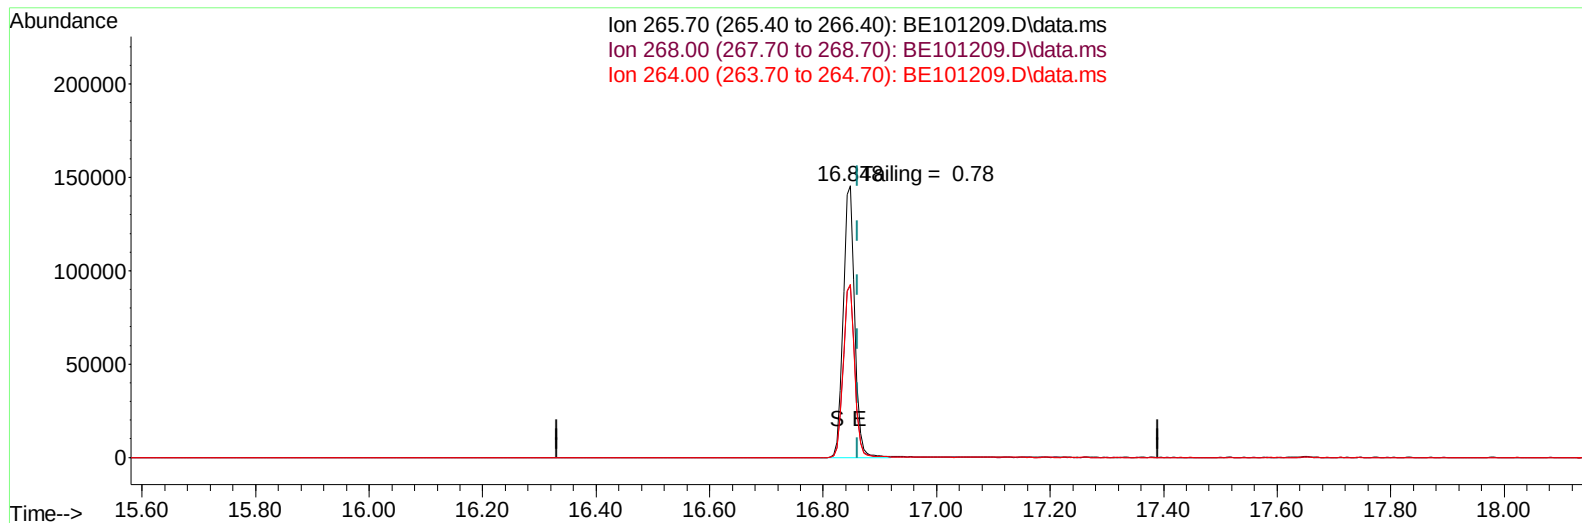

TIC: BE101209.D\data.ms

(70) Pentachlorophenol (C)

16.848min (-0.012) 1461502.03 ng




response 206451

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.26
264.00	61.60	63.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040621\
Data File : BE101209.D
Acq On : 6 Apr 2021 9:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Apr 06 11:20:59 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 10:54:22 2021
Response via : Initial Calibration

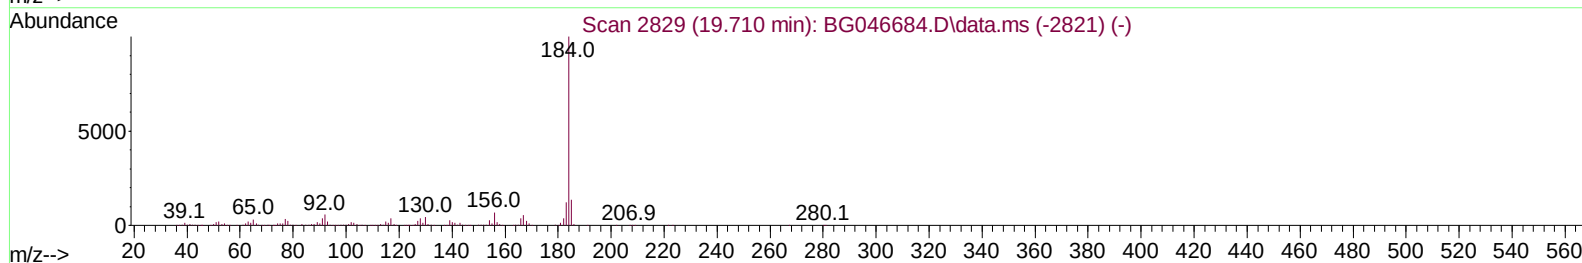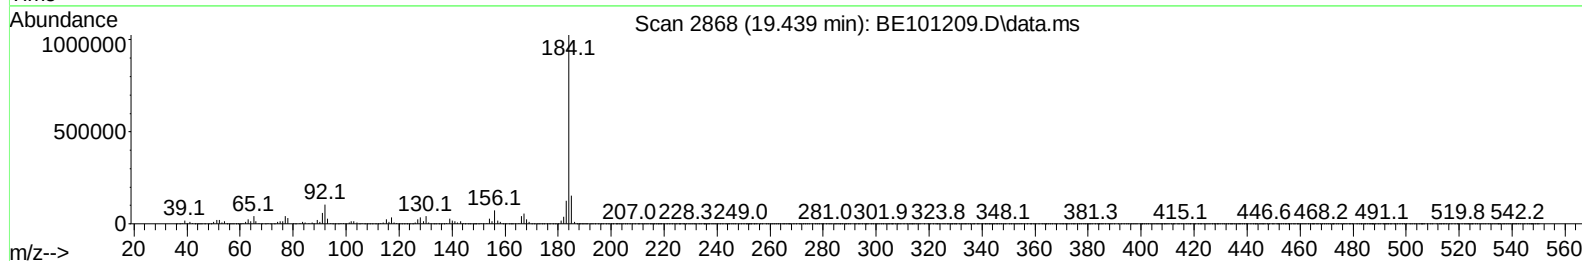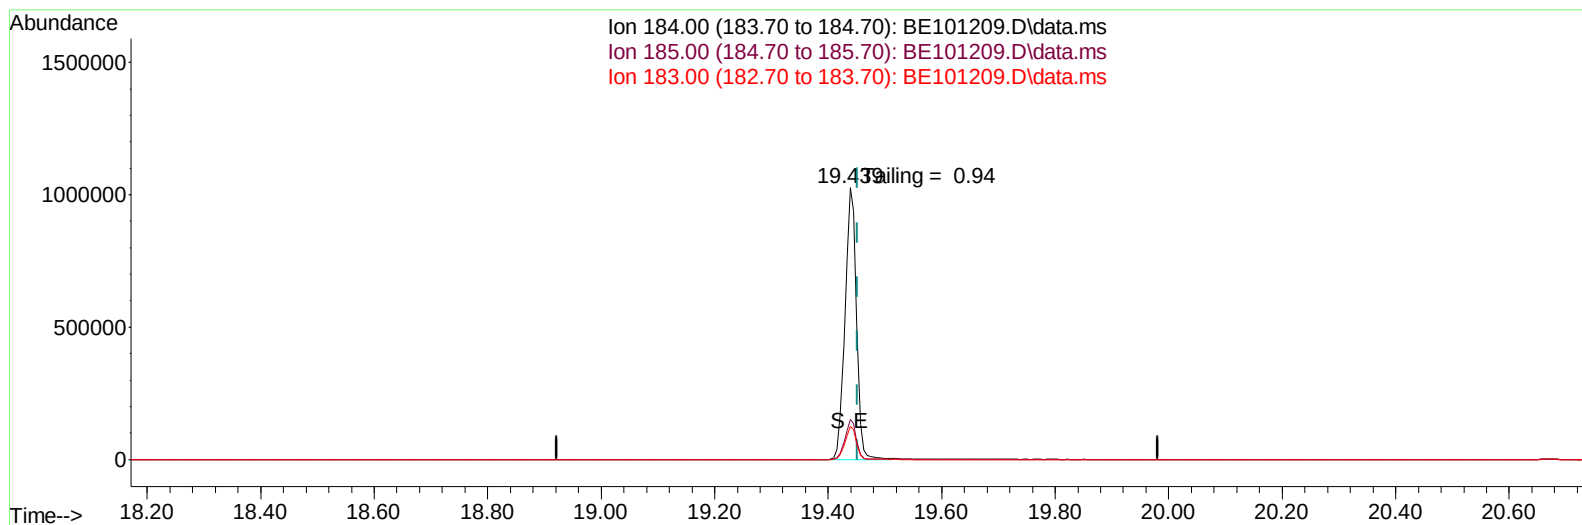

TIC: BE101209.D\data.ms

(77) Benzidine

19.439min (-0.012) 4345.06 ng

response 1457513

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.80
183.00	13.20	12.20
0.00	0.00	0.00