


Data Path : Z:\HPCHEM1\BNA_E\Data\BE040717\
 Data File : BE092890.D
 Acq On : 7 Apr 2017 11:12
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE040417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 04 16:35:54 2017

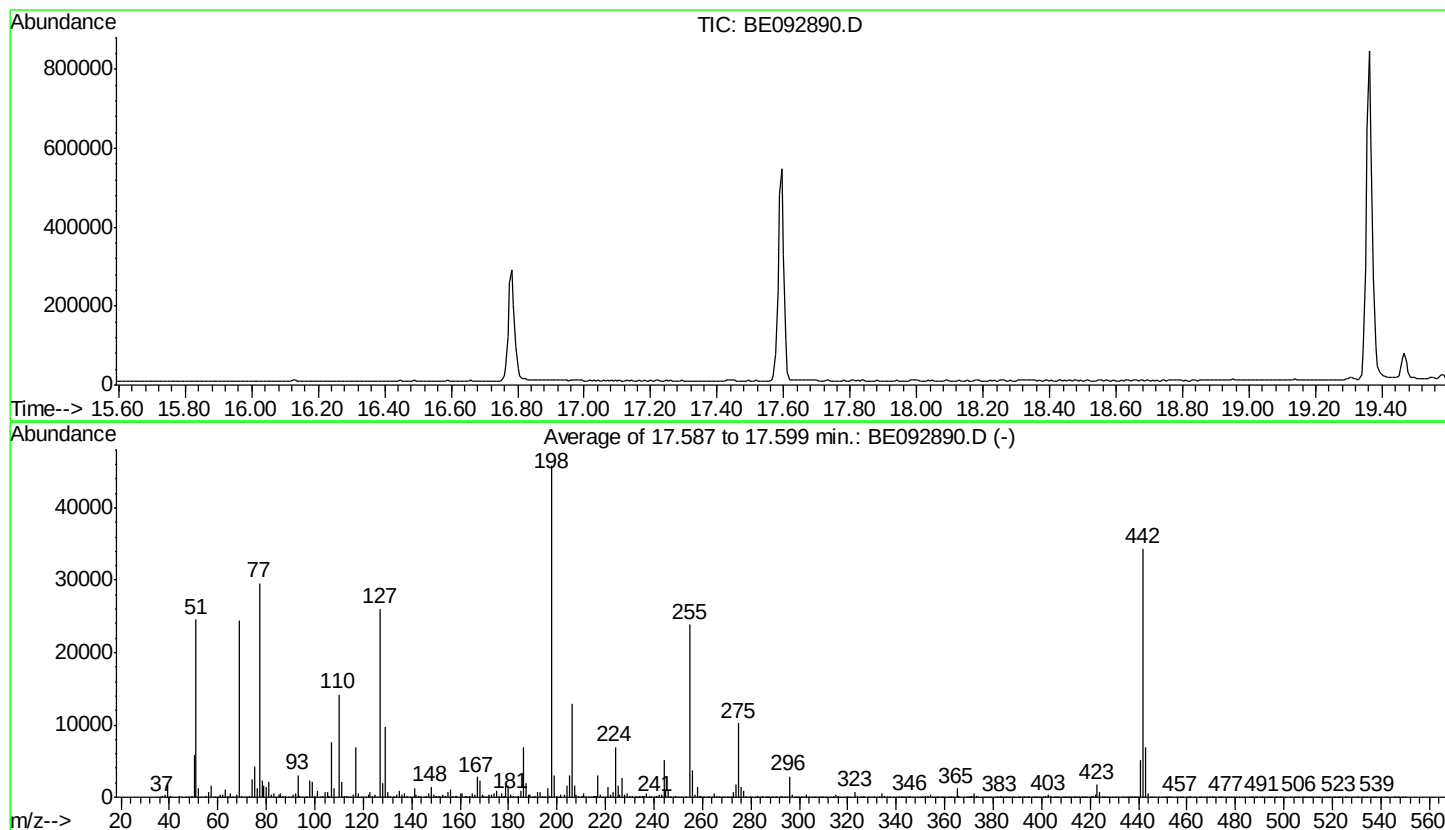

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2546

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.6	24577	PASS
68	69	0.00	2	1.5	371	PASS
69	198	0.00	100	53.1	24357	PASS
70	69	0.00	2	0.7	160	PASS
127	198	10	80	56.9	26093	PASS
197	198	0.00	2	0.2	113	PASS
198	198	100	100	100.0	45836	PASS
199	198	5	9	6.7	3088	PASS
275	198	10	60	22.2	10186	PASS
365	198	1	100	2.6	1183	PASS
441	442	0.01	24	15.0	5138	PASS
442	198	50	100	75.0	34360	PASS
443	442	15	24	20.0	6856	PASS