
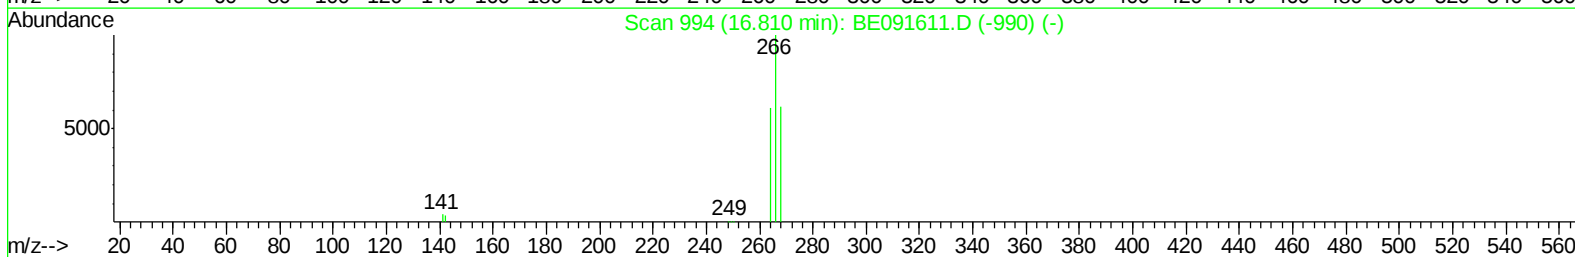
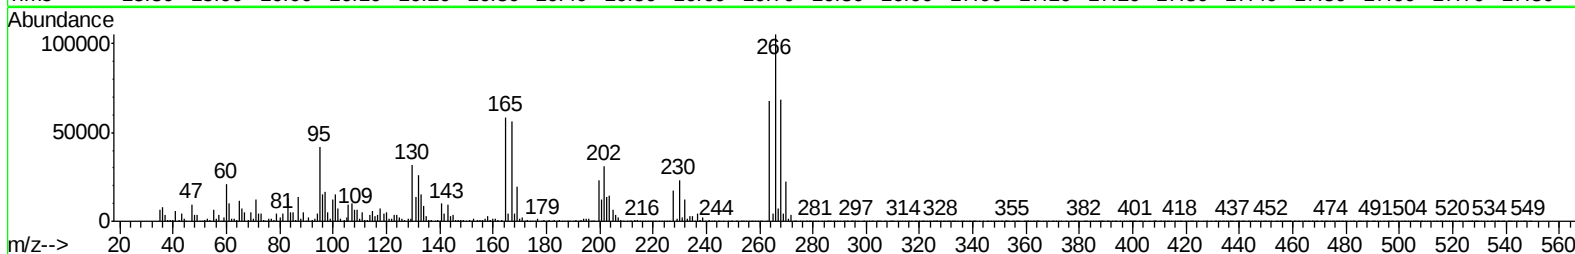


Data Path : Z:\HPCHEM1\BNA E\DATA\BE040816\
Data File : BE091605.D
Acq On : 8 Apr 2016 9:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 19:16:06 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE040816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 16:48:14 2016
Response via : Initial Calibration

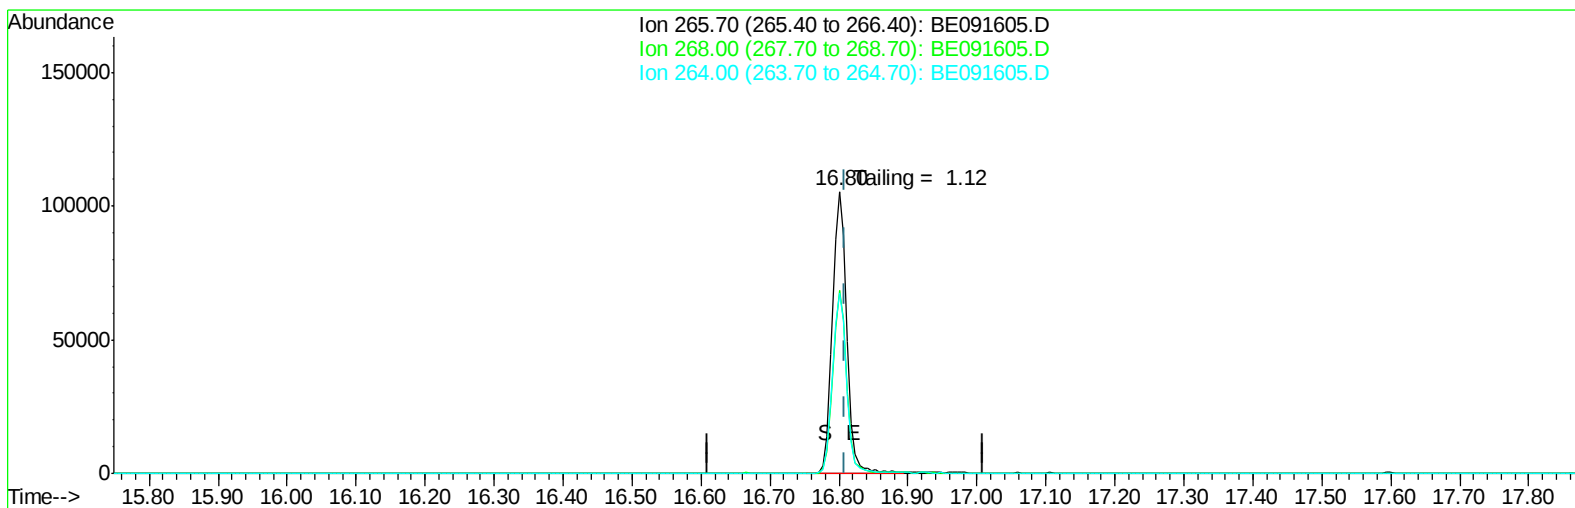

TIC: BE091605.D

(22) Pentachlorophenol




16.800min (-0.010) 59193.17ng

response 151233

Ion	Exp%	Act%
265.70	100	100
268.00	72.70	65.06
264.00	70.30	64.32
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE040816\
Data File : BE091605.D
Acq On : 8 Apr 2016 9:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 19:16:06 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE040816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 16:48:14 2016
Response via : Initial Calibration

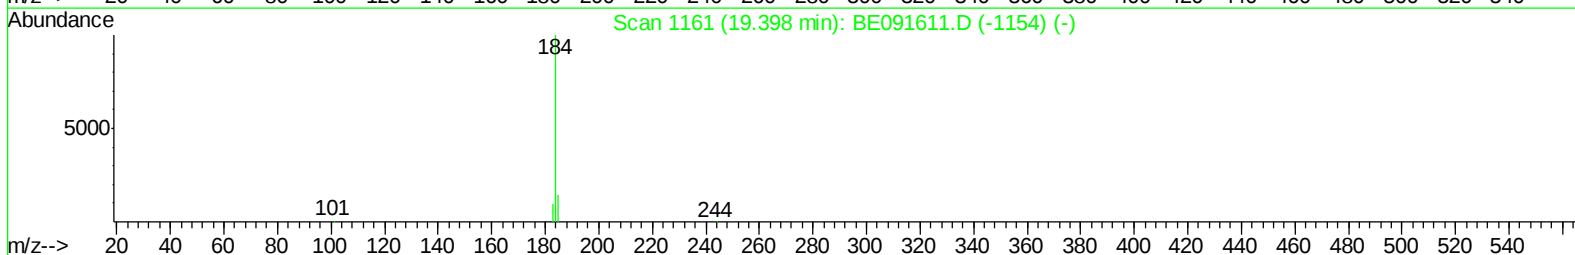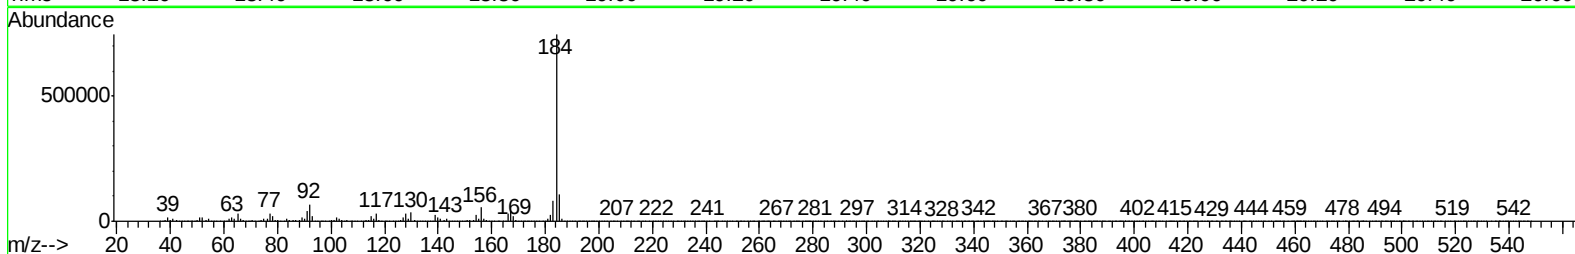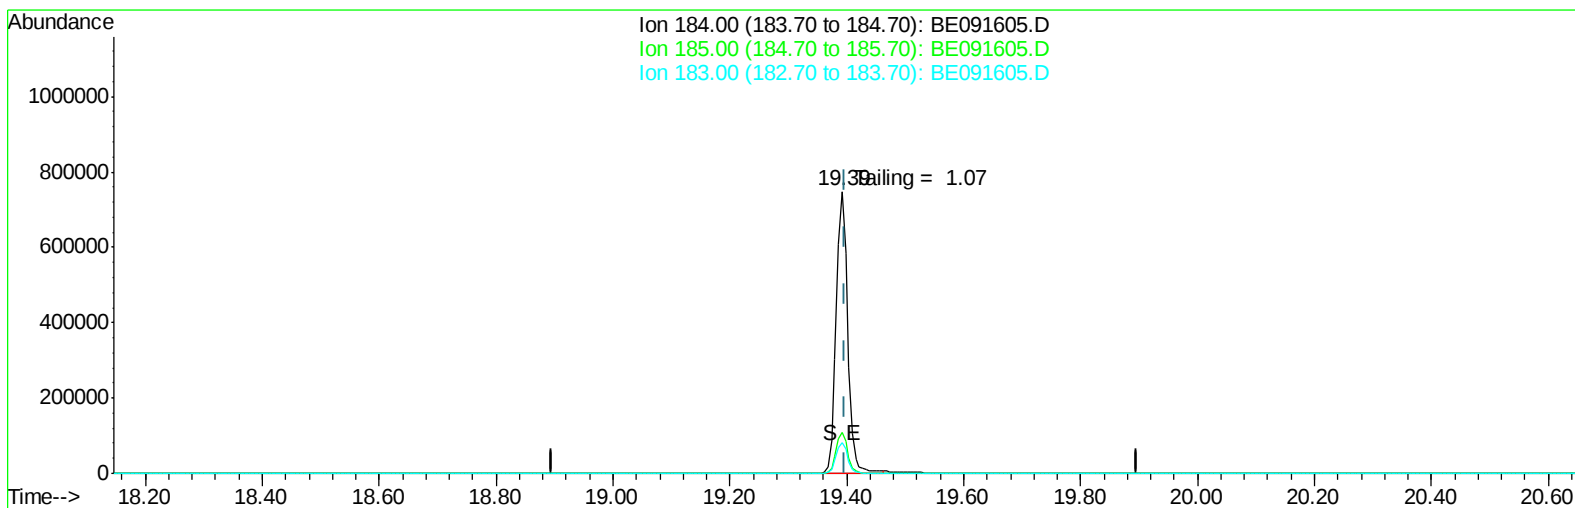

TIC: BE091605.D

(27) Benzidine

19.392min (-0.005) 423.85ng

response 1020211

Ion	Exp%	Act%
184.00	100	100
185.00	27.90	14.36#
183.00	20.50	10.90#
0.00	0.00	0.00